

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039479.D
 Acq On : 19 Apr 2023 04:41
 Operator : CG/JU
 Sample : 02335-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	12	rVB	57504	66236	0.84%	0.099%
2	3.652	76	79	91	rBV	141247	244241	3.11%	0.367%
3	3.969	130	133	139	rVB	19882	28083	0.36%	0.042%
4	7.022	646	652	666	rBV	127618	290852	3.70%	0.436%
5	7.163	670	676	701	rVV	914093	1550567	19.73%	2.327%
6	7.363	703	710	731	rBV	776791	1386809	17.65%	2.081%
7	7.828	782	789	808	rBV	759091	1335723	17.00%	2.004%
8	8.563	908	914	941	rBV	479546	1021315	13.00%	1.533%
9	8.998	981	988	1007	rBV	1030467	1919093	24.42%	2.880%
10	9.722	1102	1111	1129	rBV	811189	1559167	19.84%	2.340%
11	10.275	1198	1205	1224	rBV	977380	2001545	25.47%	3.004%
12	10.639	1259	1267	1283	rBV	1158293	2059766	26.21%	3.091%
13	10.786	1285	1292	1325	rBV	840315	1904973	24.24%	2.859%
14	12.245	1535	1540	1553	rBV3	10605	32493	0.41%	0.049%
15	13.310	1711	1721	1725	rBV4	21800	37510	0.48%	0.056%
16	13.504	1751	1754	1760	rVB2	9357	15161	0.19%	0.023%
17	13.904	1815	1822	1837	rBV	2813928	4064881	51.73%	6.100%
18	14.180	1862	1869	1892	rBV	3228414	4759190	60.57%	7.142%
19	14.374	1896	1902	1908	rVB9	5468	14559	0.19%	0.022%
20	14.486	1913	1921	1934	rBV	1961254	2914322	37.09%	4.373%
21	14.763	1960	1968	1970	rBV5	23009	55276	0.70%	0.083%
22	15.480	2084	2090	2106	rBV	4080228	6014701	76.55%	9.026%
23	15.615	2107	2113	2127	rVV	1293679	2070831	26.36%	3.107%
24	15.721	2129	2131	2142	rVB4	26293	47422	0.60%	0.071%
25	15.851	2148	2153	2160	rBV	77731	112657	1.43%	0.169%
26	17.239	2382	2389	2400	rBV	2282846	3389371	43.14%	5.086%
27	17.339	2400	2406	2430	rVB	4606889	6900956	87.83%	10.356%
28	18.139	2538	2542	2551	rBV2	58045	123559	1.57%	0.185%
29	19.198	2718	2722	2730	rBV	55086	84146	1.07%	0.126%
30	19.274	2730	2735	2740	rBV	52344	85861	1.09%	0.129%
31	19.415	2756	2759	2768	rBV4	42627	90717	1.15%	0.136%
32	19.562	2781	2784	2787	rVB4	13205	15578	0.20%	0.023%
33	19.639	2790	2797	2816	rBV	5467764	7857398	100.00%	11.791%
34	21.139	3048	3052	3059	rBV2	101137	214005	2.72%	0.321%
35	21.427	3096	3101	3117	rBV	2285883	3303165	42.04%	4.957%
36	23.644	3471	3478	3494	rVB2	2992353	6216629	79.12%	9.329%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039479.D
Acq On : 19 Apr 2023 04:41
Operator : CG/JU
Sample : 02335-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	23.797	3497	3504	3518	rVB2	1321549	2851493	36.29%	4.279%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 66640251

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039479.D
Acq On : 19 Apr 2023 04:41
Operator : CG/JU
Sample : 02335-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

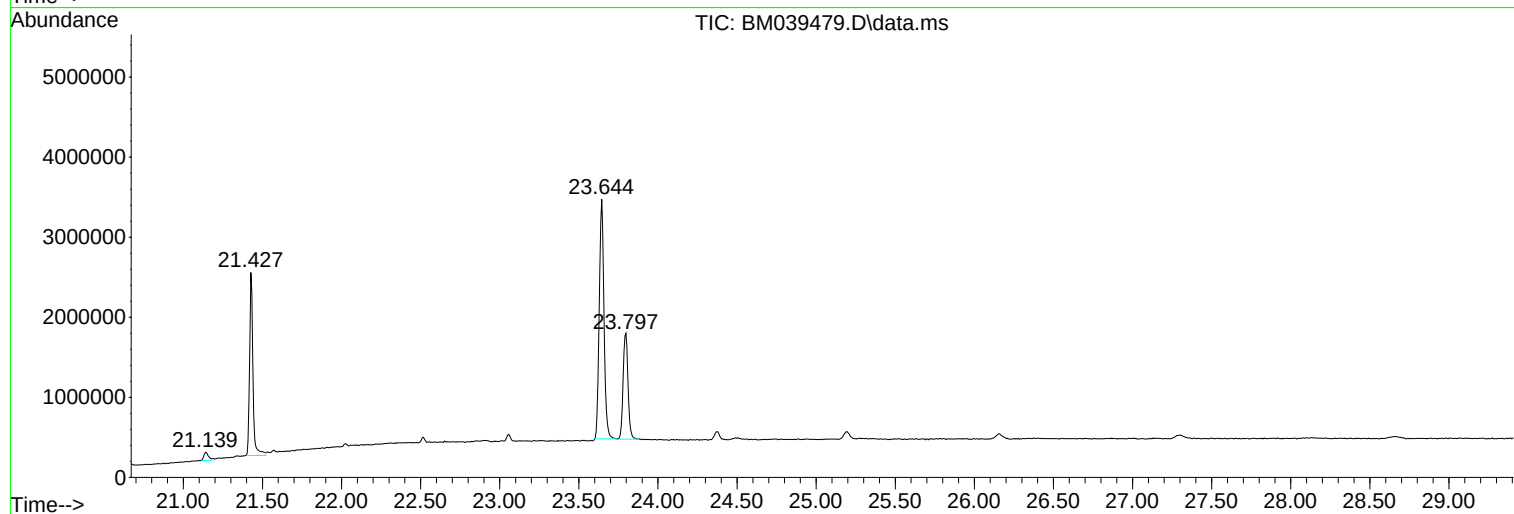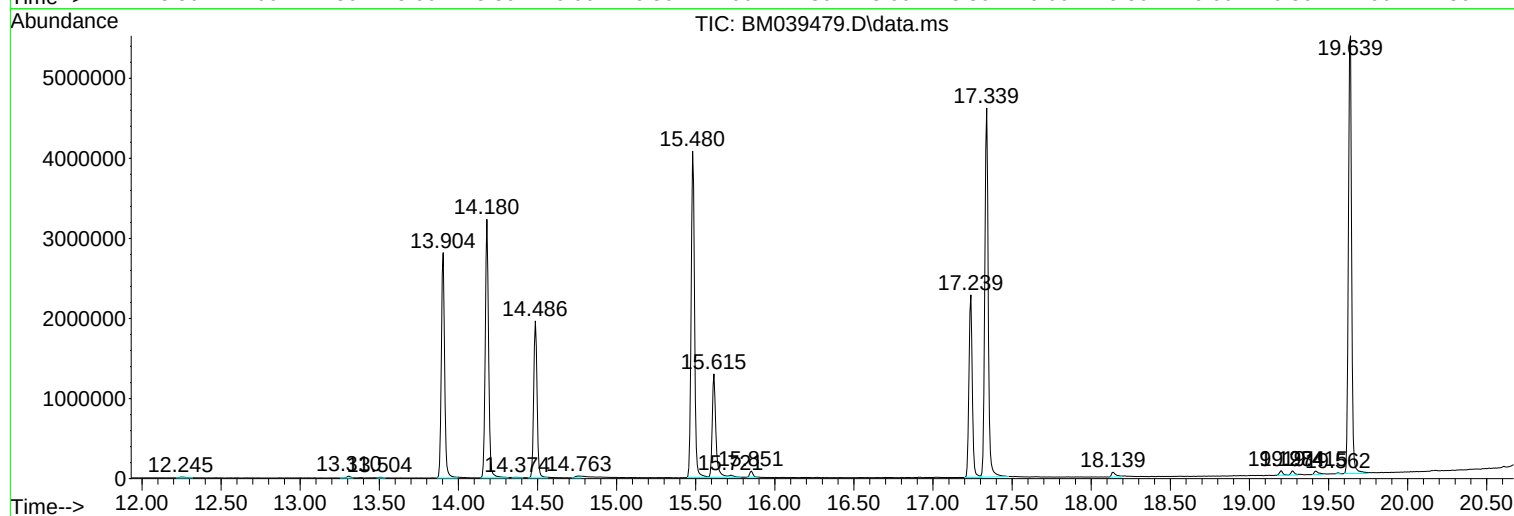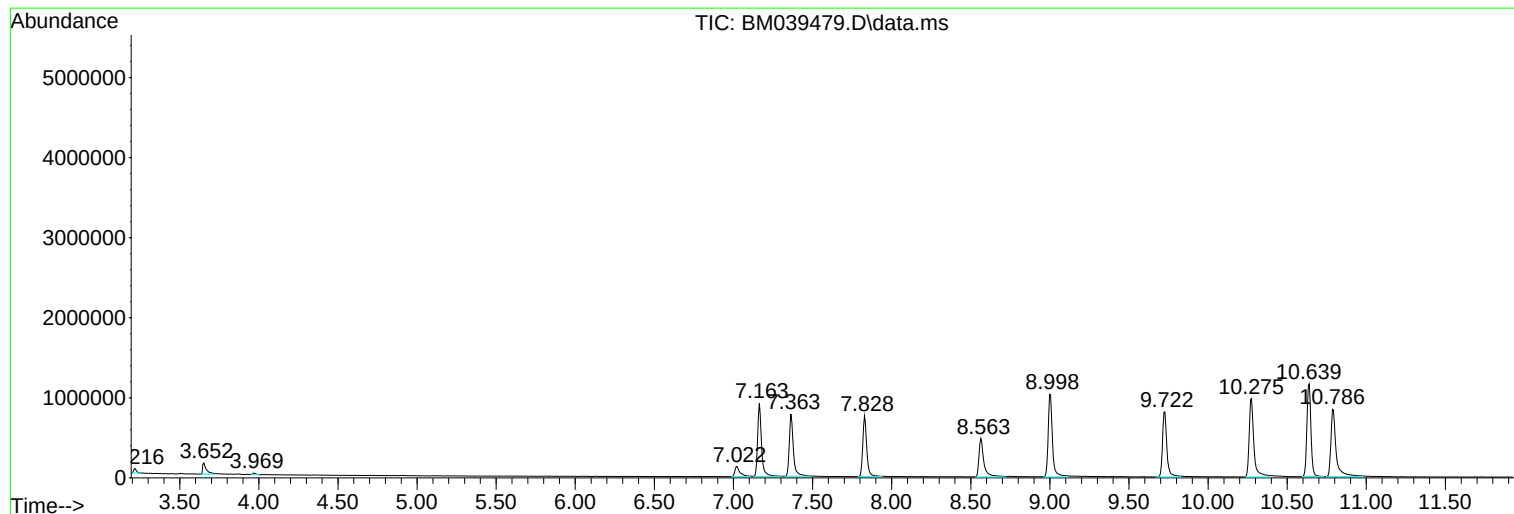

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039479.D
Acq On : 19 Apr 2023 04:41
Operator : CG/JU
Sample : 02335-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039479.D
Acq On : 19 Apr 2023 04:41
Operator : CG/JU
Sample : 02335-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMH6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc