

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039484.D
 Acq On : 19 Apr 2023 08:17
 Operator : CG/JU
 Sample : PB152174BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK174

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	18	rVB	86046	111088	1.56%	0.168%
2	3.657	78	80	98	rBV2	84149	181776	2.55%	0.274%
3	3.969	130	133	143	rVB	17800	27961	0.39%	0.042%
4	7.016	645	651	670	rBV	882584	1680108	23.57%	2.536%
5	7.163	670	676	697	rVB	907761	1519155	21.31%	2.293%
6	7.363	703	710	727	rBV	1062367	1817319	25.49%	2.744%
7	7.828	782	789	809	rBV	819463	1422678	19.96%	2.148%
8	8.557	907	913	941	rBV	1122396	2230460	31.29%	3.367%
9	8.998	982	988	1014	rBV	1004319	1829738	25.66%	2.762%
10	9.722	1104	1111	1131	rBV	838459	1566940	21.98%	2.366%
11	10.269	1197	1204	1231	rBV	919017	2143772	30.07%	3.236%
12	10.633	1259	1266	1280	rBV	1228061	2172695	30.48%	3.280%
13	12.257	1536	1542	1543	rBV5	9068	13212	0.19%	0.020%
14	13.904	1814	1822	1844	rBV	2606214	4046174	56.75%	6.108%
15	14.180	1861	1869	1887	rBV	2538747	3892671	54.60%	5.877%
16	14.486	1914	1921	1938	rBV	2040306	3116436	43.71%	4.705%
17	14.727	1955	1962	1989	rBV	474888	1363354	19.12%	2.058%
18	15.480	2083	2090	2107	rBV	3877887	5665622	79.47%	8.553%
19	15.615	2107	2113	2127	rVV	1258332	1983501	27.82%	2.994%
20	15.721	2128	2131	2141	rVB	25526	49464	0.69%	0.075%
21	15.992	2172	2177	2182	rVB2	24455	35753	0.50%	0.054%
22	17.021	2349	2352	2358	rVB4	4005	7743	0.11%	0.012%
23	17.239	2382	2389	2399	rBV	2490969	3682327	51.65%	5.559%
24	17.339	2399	2406	2429	rVB	4047287	6136707	86.08%	9.264%
25	17.915	2498	2504	2511	rBV7	9961	21266	0.30%	0.032%
26	19.198	2718	2722	2730	rBV4	47168	90251	1.27%	0.136%
27	19.274	2731	2735	2741	rVB2	38659	61046	0.86%	0.092%
28	19.633	2790	2796	2815	rBV	4985480	7129378	100.00%	10.763%
29	21.427	3096	3101	3115	rBV	2485090	3619984	50.78%	5.465%
30	23.644	3471	3478	3496	rBV2	2603882	5506792	77.24%	8.313%
31	23.797	3497	3504	3516	rVB2	1448406	3114102	43.68%	4.701%


Sum of corrected areas: 66239473

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039484.D
Acq On : 19 Apr 2023 08:17
Operator : CG/JU
Sample : PB152174BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK174

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

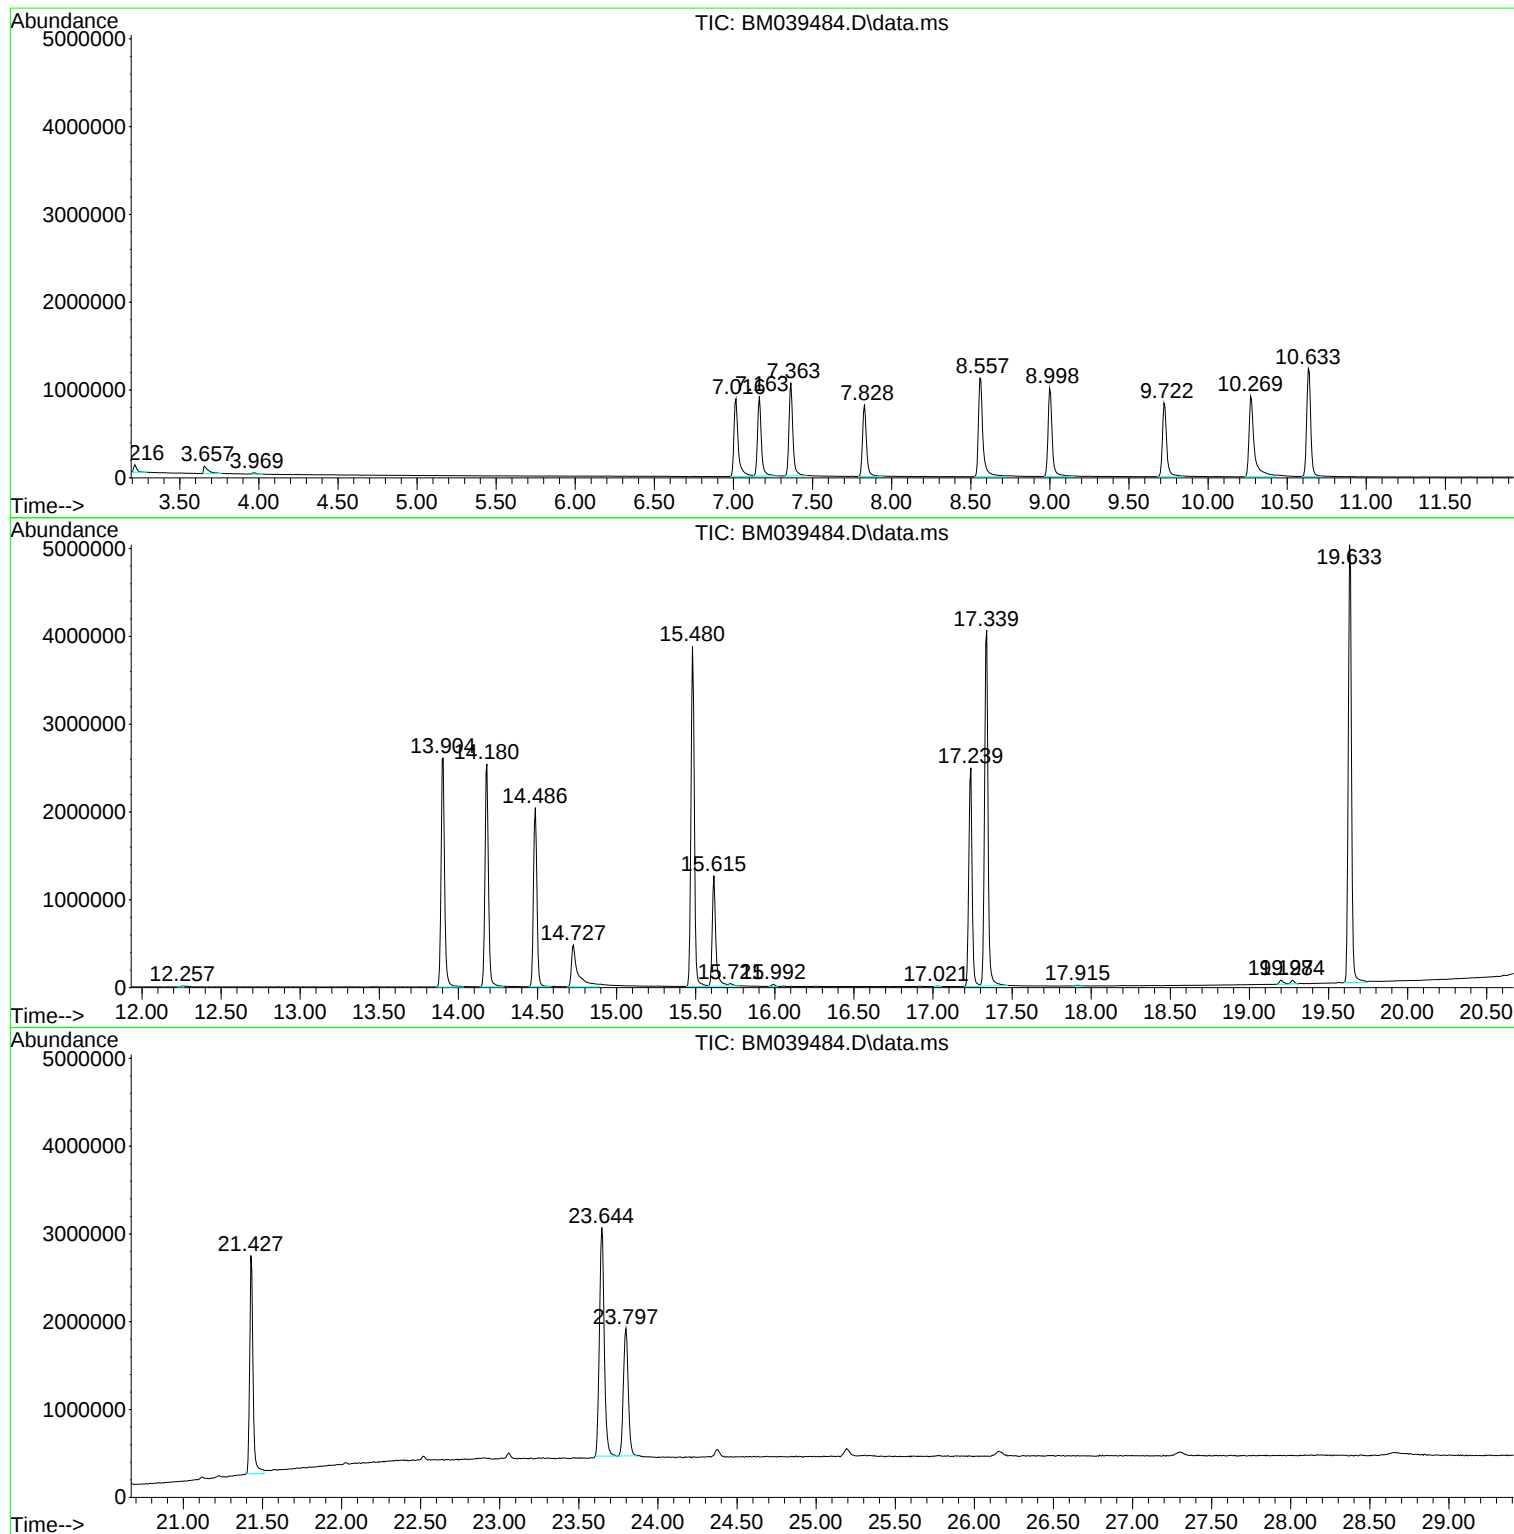

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039484.D
Acq On : 19 Apr 2023 08:17
Operator : CG/JU
Sample : PB152174BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK174

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039484.D
Acq On : 19 Apr 2023 08:17
Operator : CG/JU
Sample : PB152174BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK174

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------