

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039489.D
 Acq On : 19 Apr 2023 11:17
 Operator : CG/JU
 Sample : 02336-03
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	27	30	38	rVB	55323	79006	1.15%	0.127%
2	3.649	101	104	121	rBV	148067	279609	4.06%	0.451%
3	3.966	155	158	164	rVB2	18523	30050	0.44%	0.048%
4	5.090	347	349	354	rVB2	9773	11295	0.16%	0.018%
5	7.019	671	677	694	rBV	134381	316576	4.59%	0.511%
6	7.160	695	701	726	rVV	791772	1379106	20.01%	2.226%
7	7.360	729	735	757	rVV	707394	1291168	18.73%	2.084%
8	7.825	807	814	832	rBV	754402	1330804	19.31%	2.148%
9	8.560	933	939	961	rBV	490178	1015563	14.73%	1.639%
10	9.001	1006	1014	1037	rBV	908594	1696963	24.62%	2.738%
11	9.160	1039	1041	1046	rVB6	5661	8480	0.12%	0.014%
12	9.389	1076	1080	1084	rVB2	11935	16748	0.24%	0.027%
13	9.725	1130	1137	1158	rBV	737983	1397990	20.28%	2.256%
14	10.272	1223	1230	1253	rBV	896686	1892090	27.45%	3.053%
15	10.636	1284	1292	1309	rBV	1211546	2077236	30.14%	3.352%
16	10.789	1311	1318	1348	rBV	443056	1070673	15.53%	1.728%
17	11.889	1499	1505	1509	rVB2	13282	19038	0.28%	0.031%
18	12.242	1560	1565	1576	rVB3	10107	27953	0.41%	0.045%
19	13.301	1739	1745	1751	rBV3	28459	48423	0.70%	0.078%
20	13.507	1775	1780	1784	rVB2	15979	24607	0.36%	0.040%
21	13.901	1840	1847	1863	rBV	2517530	3684508	53.46%	5.946%
22	14.177	1887	1894	1913	rBV	2829159	4238424	61.49%	6.840%
23	14.377	1926	1928	1935	rVB6	5642	9506	0.14%	0.015%
24	14.483	1939	1946	1959	rBV	2070432	3014793	43.74%	4.865%
25	14.754	1987	1992	1993	rBV4	24013	37935	0.55%	0.061%
26	15.065	2039	2045	2048	rBV7	10114	22474	0.33%	0.036%
27	15.477	2109	2115	2132	rBV	3497684	5317112	77.14%	8.580%
28	15.612	2132	2138	2153	rVV	1149202	1746722	25.34%	2.819%
29	15.724	2153	2157	2168	rVB5	21544	46294	0.67%	0.075%
30	15.848	2173	2178	2191	rVB	139479	212698	3.09%	0.343%
31	17.236	2407	2414	2425	rBV	2498629	3584995	52.01%	5.785%
32	17.336	2425	2431	2450	rVV2	4007334	5947779	86.30%	9.598%
33	18.136	2562	2567	2575	rBV	109171	211536	3.07%	0.341%
34	19.195	2744	2747	2753	rVB2	53345	71457	1.04%	0.115%
35	19.271	2756	2760	2766	rBV	46188	73750	1.07%	0.119%
36	19.418	2781	2785	2796	rBV3	50888	99112	1.44%	0.160%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039489.D
Acq On : 19 Apr 2023 11:17
Operator : CG/JU
Sample : 02336-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMG3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	19.636	2816	2822	2839	rVB	5028762	6892377	100.00%	11.122%
38	21.147	3074	3079	3089	rBV4	135513	312846	4.54%	0.505%
39	21.430	3122	3127	3140	rBV	2554588	3473421	50.40%	5.605%
40	23.059	3401	3404	3413	rVB	141140	218065	3.16%	0.352%
41	23.647	3496	3504	3521	rBV	2722253	5695359	82.63%	9.191%
42	23.794	3523	3529	3545	rVB2	1470227	3043644	44.16%	4.912%




Sum of corrected areas: 61968185

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039489.D
Acq On : 19 Apr 2023 11:17
Operator : CG/JU
Sample : 02336-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

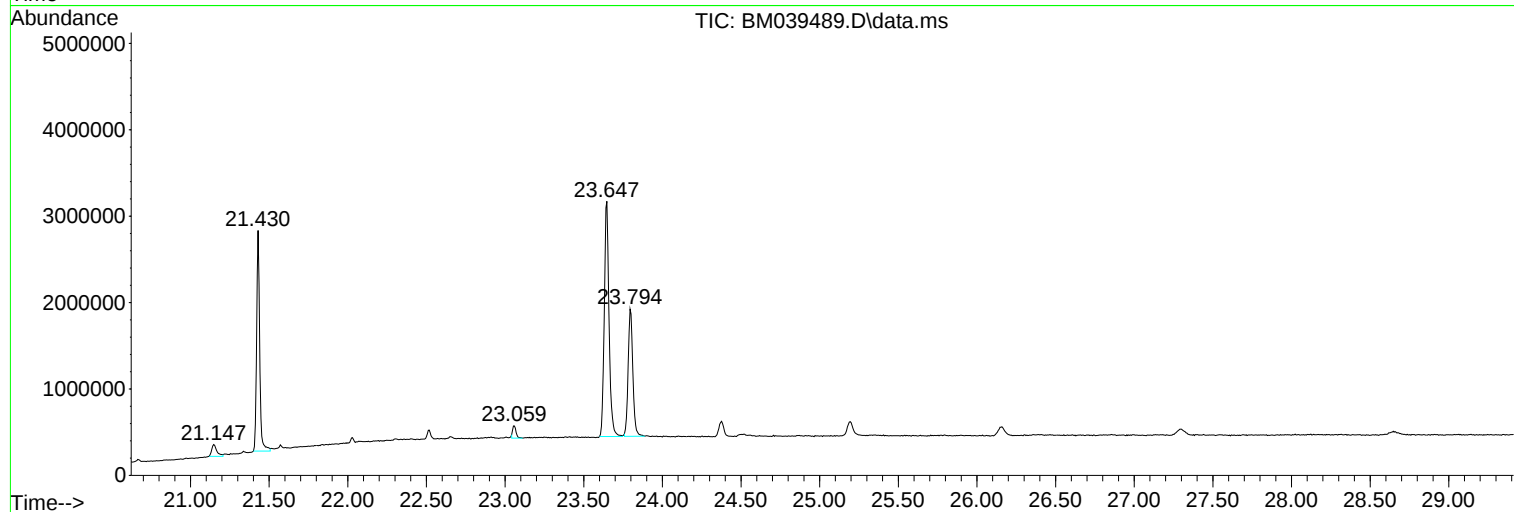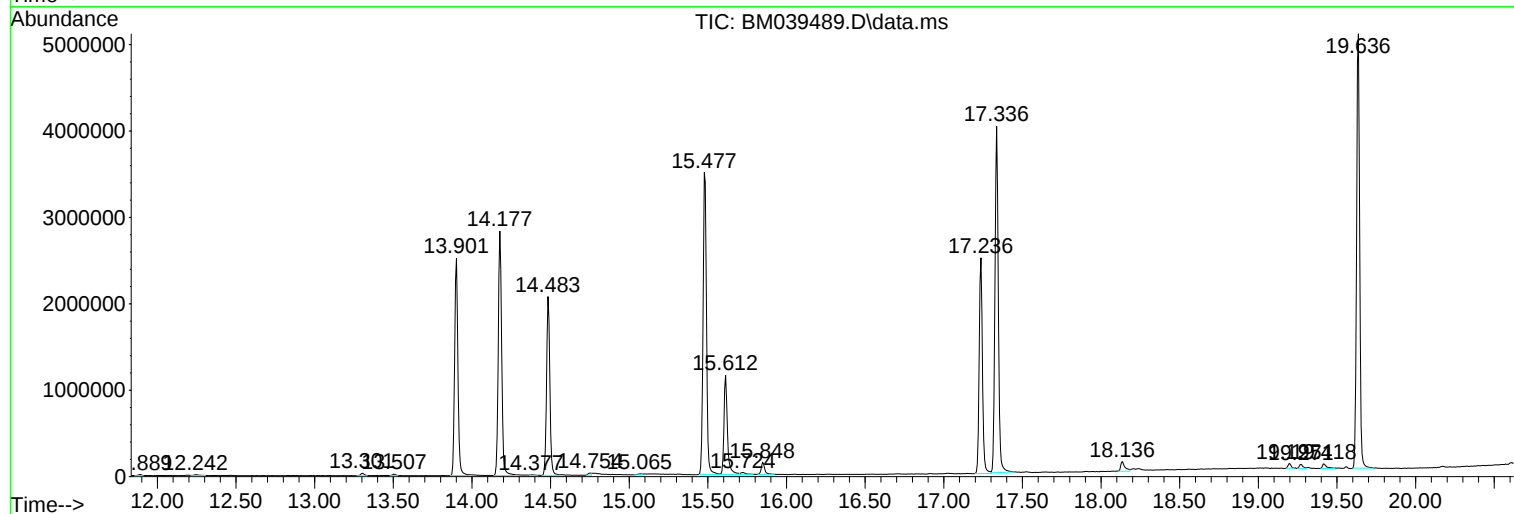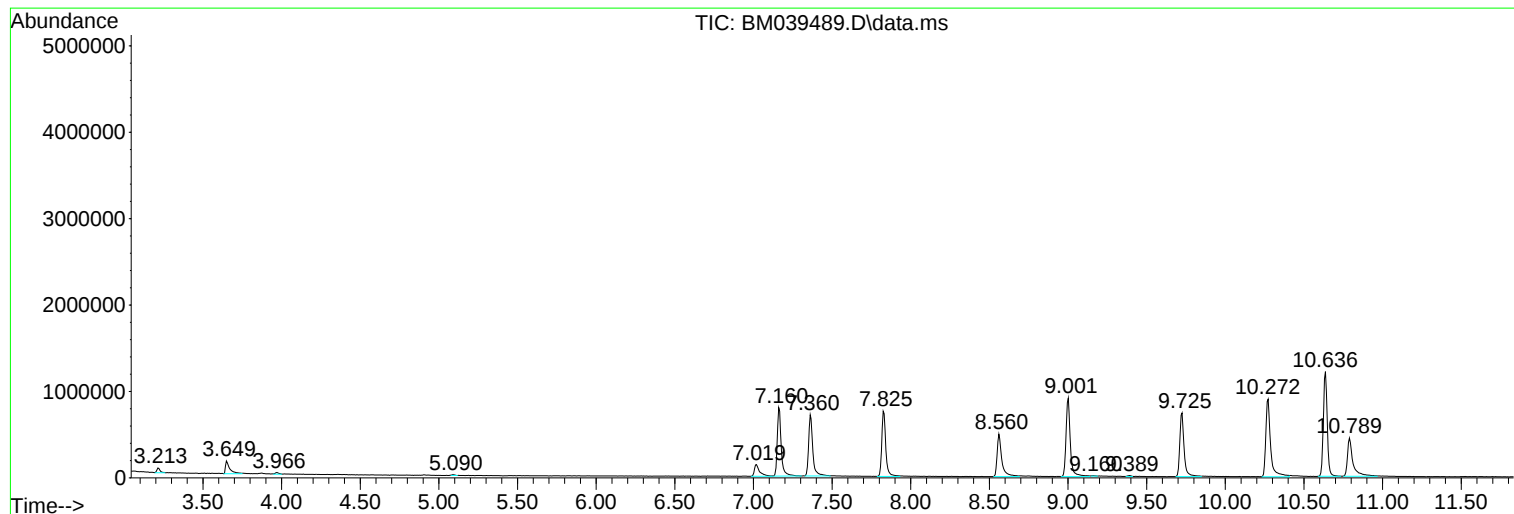

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039489.D
Acq On : 19 Apr 2023 11:17
Operator : CG/JU
Sample : 02336-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0MG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039489.D
Acq On : 19 Apr 2023 11:17
Operator : CG/JU
Sample : 02336-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0MG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc