

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039490.D
 Acq On : 19 Apr 2023 11:53
 Operator : CG/JU
 Sample : 02336-04
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	27	30	40	rVB	60925	89492	1.13%	0.133%
2	3.649	101	104	121	rBV	228143	401018	5.08%	0.596%
3	3.972	155	159	163	rBV	28851	40929	0.52%	0.061%
4	5.307	383	386	392	rVB5	6155	11602	0.15%	0.017%
5	5.443	405	409	413	rBV2	16471	27197	0.34%	0.040%
6	5.813	469	472	480	rVB2	10907	18510	0.23%	0.028%
7	7.019	671	677	694	rBV	143961	337067	4.27%	0.501%
8	7.160	695	701	725	rVV	872391	1501576	19.04%	2.233%
9	7.360	729	735	758	rVV	753553	1341372	17.01%	1.995%
10	7.825	807	814	835	rBV	750577	1319145	16.72%	1.962%
11	8.560	932	939	960	rBV	510011	1071706	13.59%	1.594%
12	9.001	1007	1014	1033	rBV	991020	1859902	23.58%	2.766%
13	9.395	1077	1081	1085	rVB7	5842	8872	0.11%	0.013%
14	9.725	1130	1137	1159	rBV	774779	1467870	18.61%	2.183%
15	10.266	1222	1229	1259	rBV	949643	2014686	25.54%	2.997%
16	10.637	1284	1292	1310	rBV	1208955	2076080	26.32%	3.088%
17	10.789	1310	1318	1339	rBV	552859	1278218	16.21%	1.901%
18	12.183	1549	1555	1561	rBV3	12178	32412	0.41%	0.048%
19	12.242	1561	1565	1570	rVB	12060	21643	0.27%	0.032%
20	13.901	1840	1847	1865	rBV	2890029	4130014	52.36%	6.143%
21	14.177	1886	1894	1911	rBV	3166505	4751556	60.24%	7.067%
22	14.483	1939	1946	1963	rBV	2061297	3038024	38.52%	4.519%
23	14.754	1985	1992	2004	rBV6	28970	128493	1.63%	0.191%
24	15.319	2083	2088	2093	rVB4	6612	13347	0.17%	0.020%
25	15.477	2109	2115	2132	rBV	3937267	5976548	75.77%	8.889%
26	15.613	2132	2138	2152	rVV	1210700	1826012	23.15%	2.716%
27	15.719	2153	2156	2161	rVB5	19151	33074	0.42%	0.049%
28	15.848	2174	2178	2184	rBV	70790	97822	1.24%	0.145%
29	16.913	2356	2359	2363	rBV6	6788	9380	0.12%	0.014%
30	16.989	2367	2372	2376	rBV8	4701	11059	0.14%	0.016%
31	17.036	2376	2380	2384	rVB4	6331	10575	0.13%	0.016%
32	17.236	2407	2414	2424	rBV	2515906	3619241	45.89%	5.383%
33	17.336	2425	2431	2448	rVV	4611326	6650600	84.32%	9.892%
34	18.136	2562	2567	2576	rBV2	48812	102669	1.30%	0.153%
35	18.207	2576	2579	2584	rVB	17301	22849	0.29%	0.034%
36	19.195	2743	2747	2755	rBV3	55539	88766	1.13%	0.132%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039490.D
Acq On : 19 Apr 2023 11:53
Operator : CG/JU
Sample : 02336-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMG4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	19.271	2756	2760	2766	rBV	50965	83718	1.06%	0.125%
38	19.412	2781	2784	2789	rBV4	31723	53363	0.68%	0.079%
39	19.559	2805	2809	2812	rBV3	20950	28274	0.36%	0.042%
40	19.636	2816	2822	2840	rBV	5692293	7887541	100.00%	11.732%
41	21.430	3122	3127	3143	rBV	2712458	3733223	47.33%	5.553%
42	23.647	3496	3504	3521	rBV2	3283405	6765376	85.77%	10.063%
43	23.794	3523	3529	3542	rVB2	1576242	3252231	41.23%	4.837%




Sum of corrected areas: 67233052

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039490.D
Acq On : 19 Apr 2023 11:53
Operator : CG/JU
Sample : 02336-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

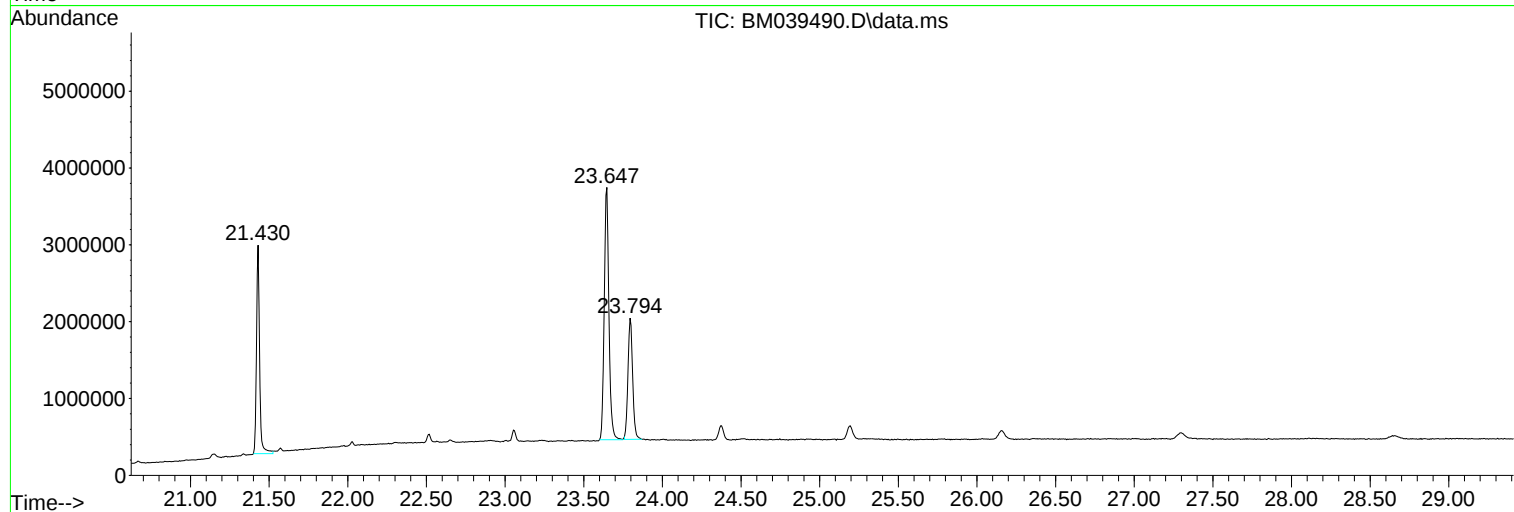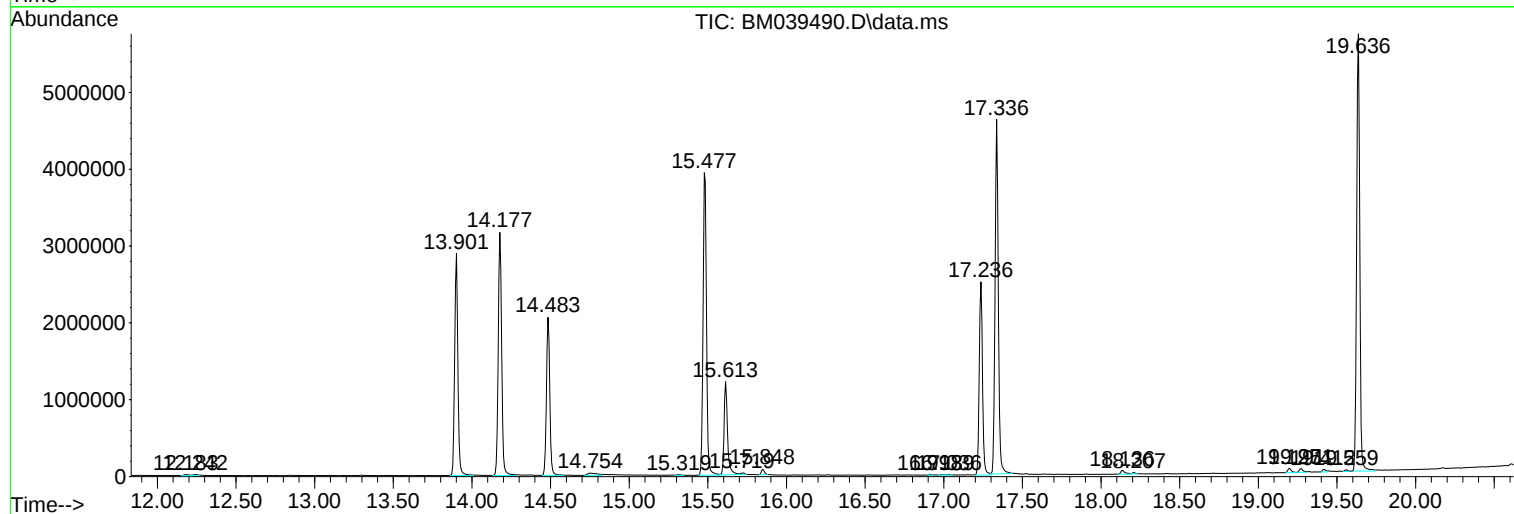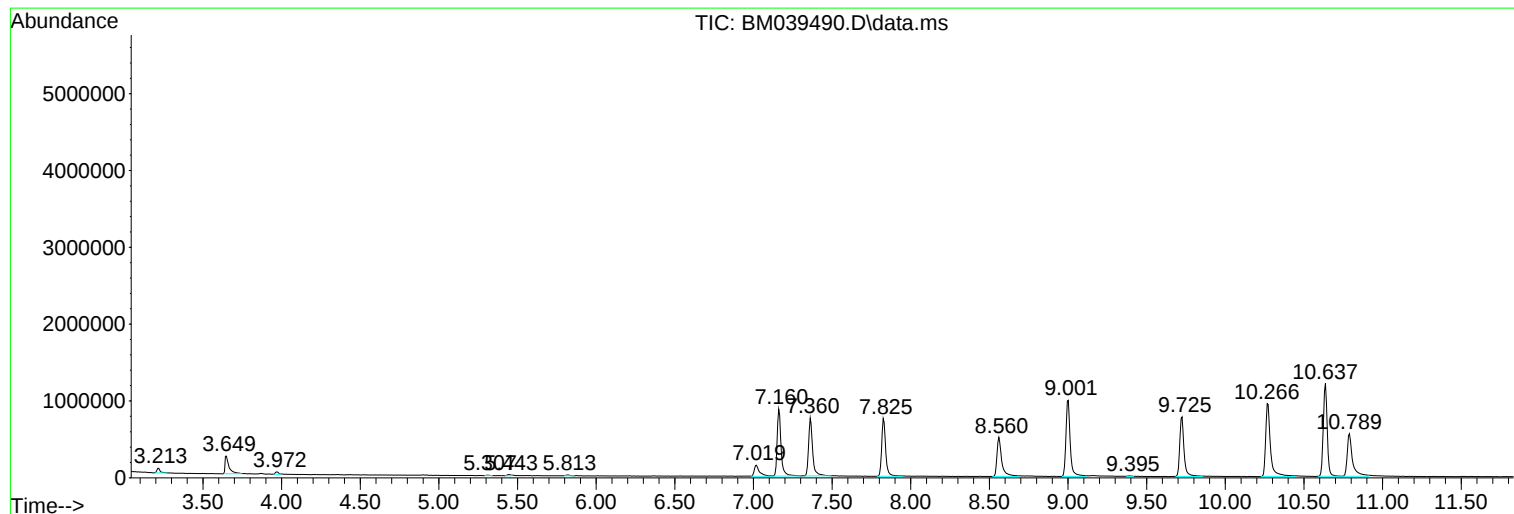

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039490.D
Acq On : 19 Apr 2023 11:53
Operator : CG/JU
Sample : 02336-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0MG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039490.D
Acq On : 19 Apr 2023 11:53
Operator : CG/JU
Sample : 02336-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0MG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc