

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039494.D
 Acq On : 19 Apr 2023 14:17
 Operator : CG/JU
 Sample : 02299-02DL 2X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M

Title : SVOA CALIBRATION

Signal : TIC: BM039494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.178	21	24	28	rBV	58871	86393	2.50%	0.235%
2	3.249	32	36	47	rVB	212285	284116	8.22%	0.774%
3	3.966	156	158	167	rVB	16089	22246	0.64%	0.061%
4	7.019	672	677	691	rBV	48945	137137	3.97%	0.373%
5	7.160	696	701	722	rVV	328628	614796	17.78%	1.674%
6	7.360	729	735	751	rBV	301818	593955	17.18%	1.617%
7	7.825	807	814	829	rBV	679987	1205750	34.88%	3.283%
8	7.943	829	834	844	rVB3	27401	55780	1.61%	0.152%
9	8.566	929	940	959	rBV	182974	452675	13.09%	1.233%
10	9.001	1006	1014	1026	rBV	376525	735507	21.27%	2.003%
11	9.390	1076	1080	1088	rVB	6983	10643	0.31%	0.029%
12	9.725	1130	1137	1155	rBV	305273	623699	18.04%	1.698%
13	10.272	1224	1230	1247	rBV	272451	756421	21.88%	2.060%
14	10.637	1284	1292	1312	rBV	1061664	1904771	55.09%	5.187%
15	11.883	1501	1504	1508	rBV2	6526	9569	0.28%	0.026%
16	12.266	1561	1569	1571	rBV7	3802	8043	0.23%	0.022%
17	13.378	1753	1758	1764	rBV3	9535	17043	0.49%	0.046%
18	13.901	1840	1847	1861	rBV	1145458	1792553	51.85%	4.881%
19	14.177	1887	1894	1913	rBV	1326002	2039058	58.98%	5.552%
20	14.483	1939	1946	1957	rBV	1874667	2798331	80.94%	7.620%
21	14.789	1994	1998	2000	rBV4	5925	8902	0.26%	0.024%
22	14.813	2000	2002	2006	rVB5	3389	5102	0.15%	0.014%
23	15.242	2071	2075	2076	rBV4	3323	4173	0.12%	0.011%
24	15.277	2078	2081	2085	rVV6	2544	4620	0.13%	0.013%
25	15.324	2087	2089	2092	rVB4	4021	4355	0.13%	0.012%
26	15.477	2108	2115	2133	rBV	1742739	2636489	76.26%	7.179%
27	15.613	2133	2138	2153	rVV	378816	668698	19.34%	1.821%
28	15.854	2174	2179	2188	rVB	21080	40099	1.16%	0.109%
29	16.189	2233	2236	2237	rBV3	3849	4207	0.12%	0.011%
30	17.007	2369	2375	2376	rBV6	2999	5976	0.17%	0.016%
31	17.024	2376	2378	2384	rVB6	4836	6980	0.20%	0.019%
32	17.236	2407	2414	2425	rBV	2316990	3366204	97.37%	9.166%
33	17.336	2425	2431	2453	rVB	1882081	2956909	85.53%	8.052%
34	17.518	2459	2462	2472	rVB3	9867	17656	0.51%	0.048%
35	17.907	2525	2528	2529	rBV3	5481	4569	0.13%	0.012%
36	18.136	2563	2567	2572	rBV4	27214	50253	1.45%	0.137%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039494.D
Acq On : 19 Apr 2023 14:17
Operator : CG/JU
Sample : 02299-02DL 2X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	18.212	2576	2580	2584	rVB	12995	21037	0.61%	0.057%
38	19.201	2744	2748	2755	rBV4	24000	38836	1.12%	0.106%
39	19.271	2756	2760	2764	rBV	20696	30888	0.89%	0.084%
40	19.418	2782	2785	2791	rBV7	15904	30666	0.89%	0.084%
41	19.630	2816	2821	2832	rBV	2439900	3457271	100.00%	9.414%
42	21.430	3122	3127	3141	rBV	2310481	3353727	97.01%	9.132%
43	23.642	3496	3503	3519	rBV2	1332244	2895846	83.76%	7.885%
44	23.794	3522	3529	3540	rVB	1422725	2962895	85.70%	8.068%




Sum of corrected areas: 36724844

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039494.D
Acq On : 19 Apr 2023 14:17
Operator : CG/JU
Sample : 02299-02DL 2X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

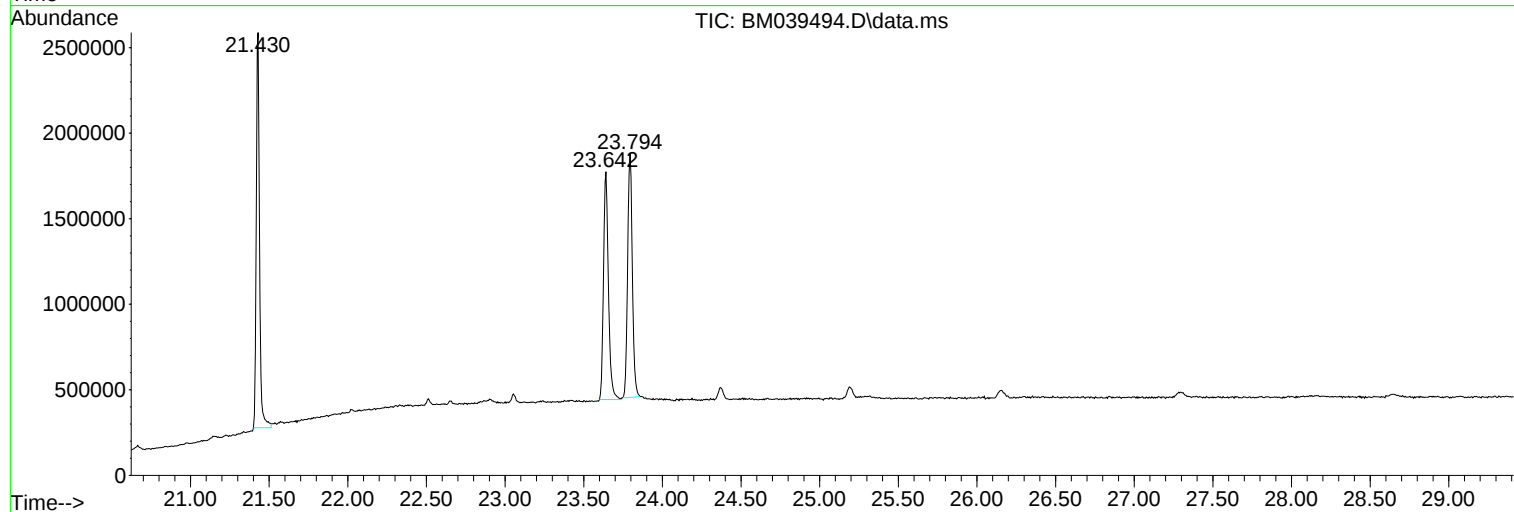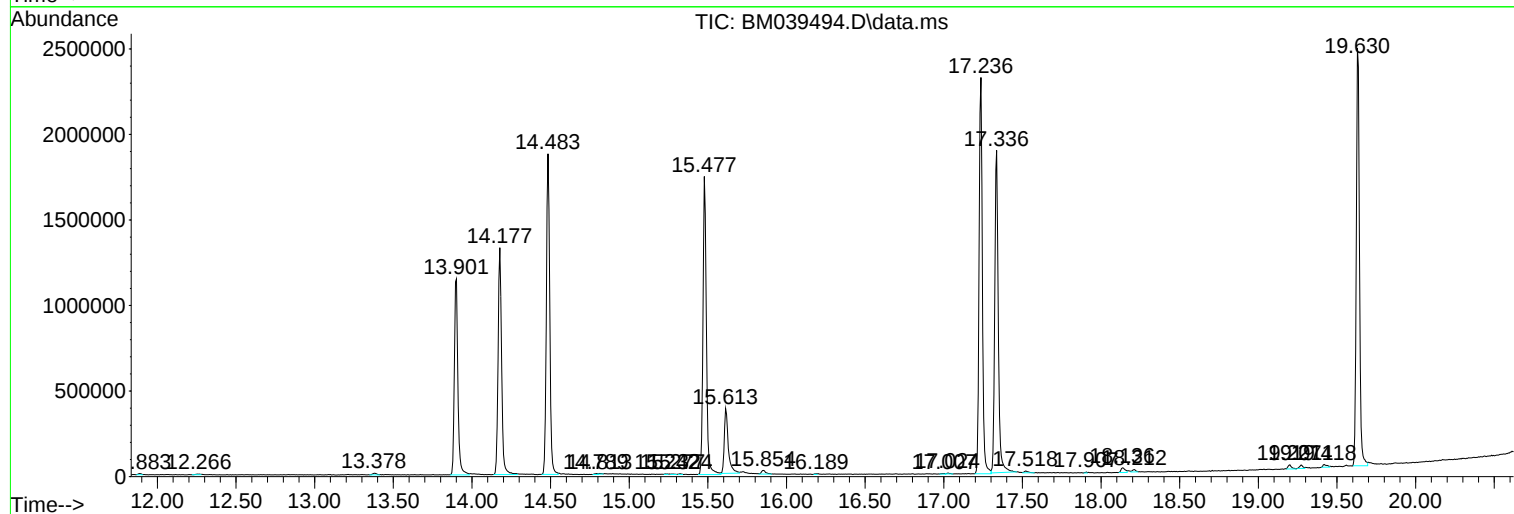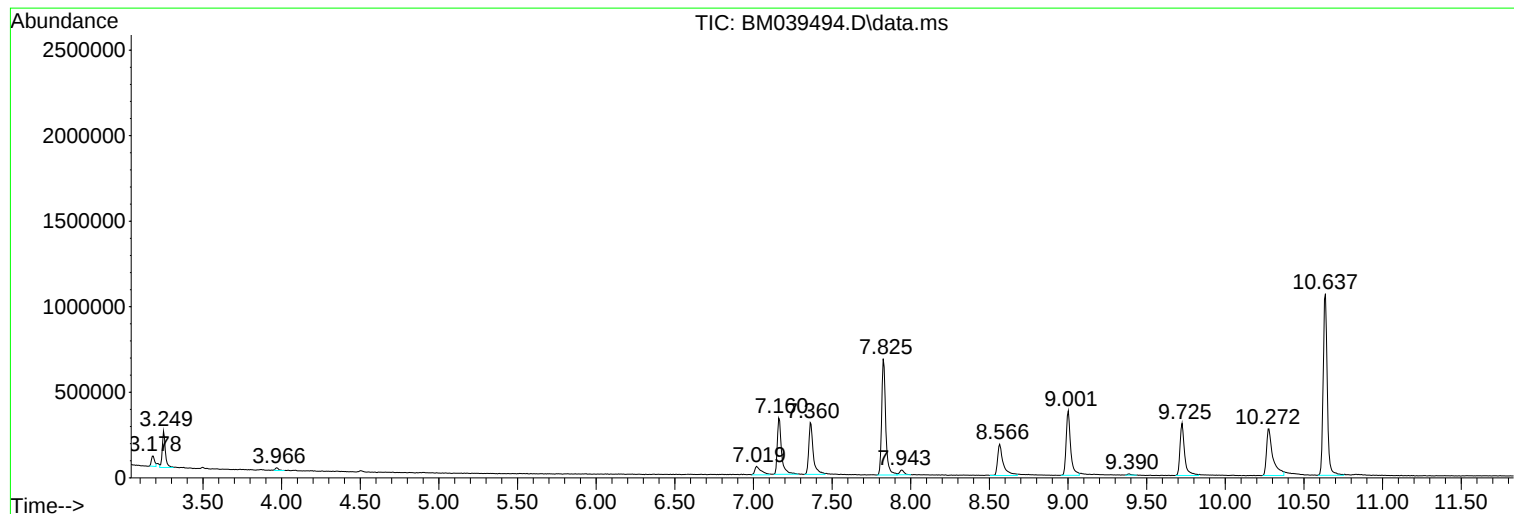

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039494.D
Acq On : 19 Apr 2023 14:17
Operator : CG/JU
Sample : 02299-02DL 2X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039494.D
Acq On : 19 Apr 2023 14:17
Operator : CG/JU
Sample : 02299-02DL 2X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc