

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039497.D
 Acq On : 19 Apr 2023 16:16
 Operator : CG/JU
 Sample : PB152215BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	26	30	38	rBV	62649	85518	1.43%	0.143%
2	3.643	100	103	125	rBV	619928	1106756	18.45%	1.851%
3	3.966	155	158	164	rVB	12927	19832	0.33%	0.033%
4	7.013	669	676	695	rBV	696960	1344037	22.41%	2.248%
5	7.160	695	701	723	rVB	706300	1234593	20.58%	2.065%
6	7.360	729	735	749	rBV	831902	1435875	23.94%	2.401%
7	7.825	807	814	827	rBV	670736	1196156	19.94%	2.000%
8	8.560	932	939	964	rBV	902074	1788373	29.82%	2.991%
9	9.001	1007	1014	1039	rBV	816065	1500114	25.01%	2.509%
10	9.725	1130	1137	1155	rBV	674813	1272517	21.22%	2.128%
11	10.272	1222	1230	1256	rBV	854870	1787474	29.80%	2.989%
12	10.637	1285	1292	1310	rBV	1105236	1888721	31.49%	3.159%
13	10.789	1310	1318	1352	rBV	800290	1818570	30.32%	3.041%
14	12.260	1562	1568	1572	rBV6	6797	16057	0.27%	0.027%
15	13.383	1752	1759	1764	rBV3	7599	14491	0.24%	0.024%
16	13.901	1840	1847	1862	rBV	2234705	3301097	55.04%	5.520%
17	14.177	1887	1894	1914	rBV	2494093	3803975	63.42%	6.361%
18	14.483	1939	1946	1964	rBV	1809187	2782704	46.39%	4.654%
19	14.725	1981	1987	2015	rBV	323354	1033625	17.23%	1.729%
20	15.483	2109	2116	2133	rBV	3143016	4697512	78.32%	7.856%
21	15.613	2133	2138	2153	rVV	892572	1508052	25.14%	2.522%
22	15.719	2153	2156	2165	rVB3	20656	40364	0.67%	0.068%
23	16.266	2241	2249	2255	rBV3	4094	9264	0.15%	0.015%
24	17.236	2408	2414	2425	rBV	2255102	3298752	55.00%	5.517%
25	17.336	2425	2431	2453	rVB2	3443199	5148013	85.83%	8.609%
26	19.201	2744	2748	2755	rBV2	40918	55060	0.92%	0.092%
27	19.271	2756	2760	2768	rBV	31690	53380	0.89%	0.089%
28	19.636	2816	2822	2833	rBV	4443176	5998011	100.00%	10.031%
29	21.430	3122	3127	3145	rBV	2313493	3407706	56.81%	5.699%
30	23.647	3497	3504	3517	rBV	2514515	5094243	84.93%	8.519%
31	23.800	3523	3530	3547	rVB	1453441	3056788	50.96%	5.112%




Sum of corrected areas: 59797630

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039497.D
Acq On : 19 Apr 2023 16:16
Operator : CG/JU
Sample : PB152215BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

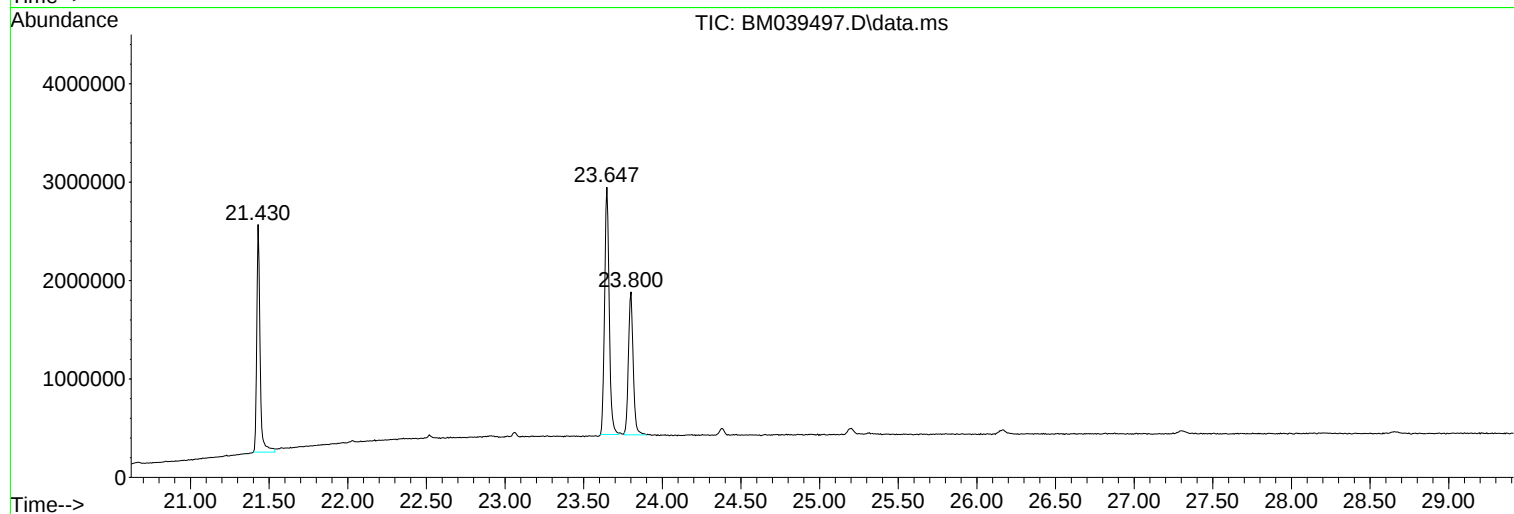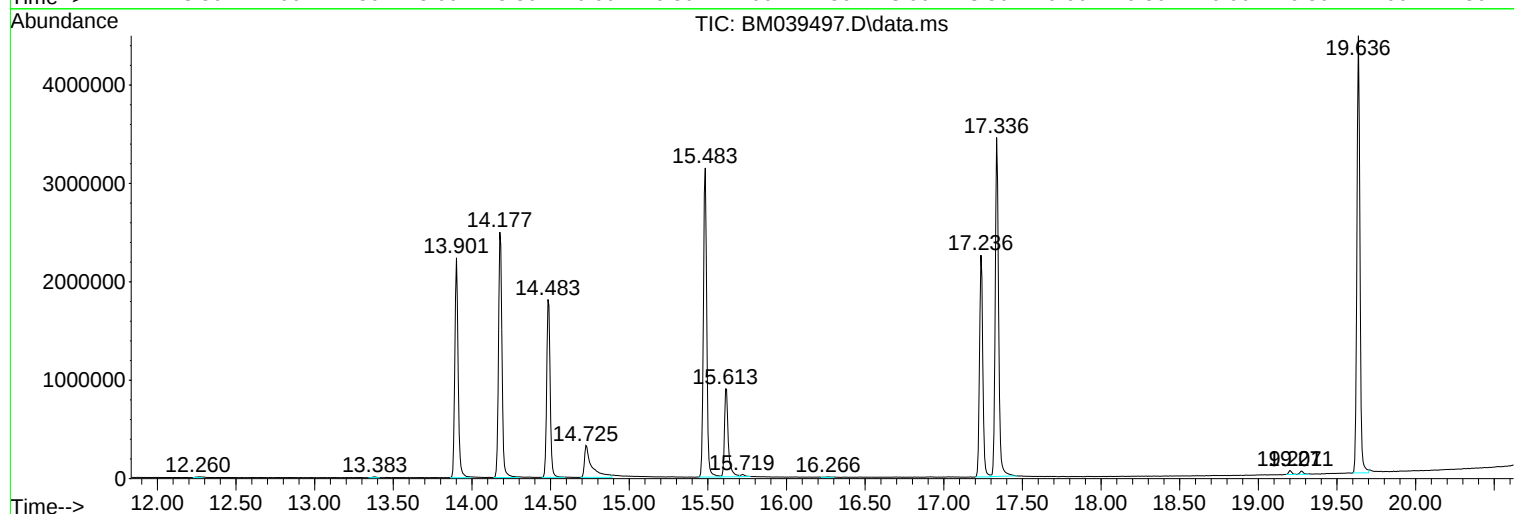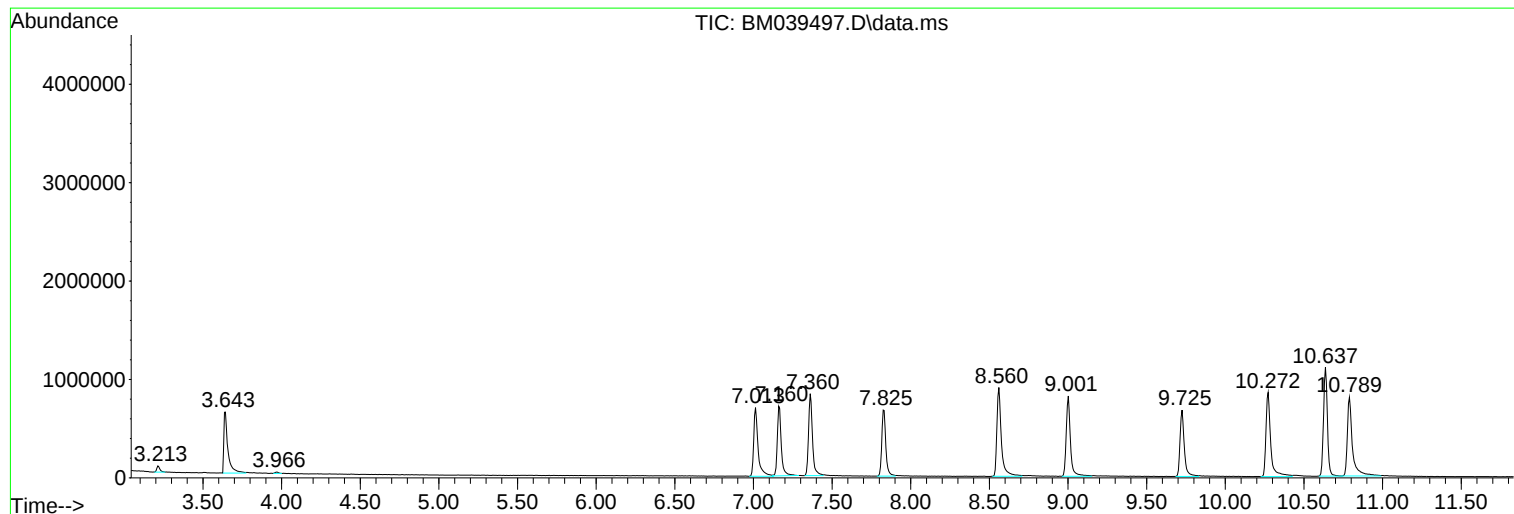

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039497.D
Acq On : 19 Apr 2023 16:16
Operator : CG/JU
Sample : PB152215BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039497.D
Acq On : 19 Apr 2023 16:16
Operator : CG/JU
Sample : PB152215BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc