

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039502.D
 Acq On : 19 Apr 2023 19:17
 Operator : CG/JU
 Sample : 02296-17
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCBM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039502.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	27	30	36	rVB	49041	65365	1.26%	0.142%
2	3.966	155	158	166	rVB	16470	24189	0.47%	0.053%
3	7.013	670	676	695	rBV	125427	303681	5.86%	0.660%
4	7.160	695	701	722	rVV	724554	1240081	23.92%	2.694%
5	7.360	729	735	753	rBV	691541	1223881	23.60%	2.658%
6	7.825	808	814	828	rBV	556132	967657	18.66%	2.102%
7	8.560	932	939	954	rBV	425643	866641	16.71%	1.882%
8	9.001	1006	1014	1035	rBV	799593	1504693	29.02%	3.268%
9	9.725	1129	1137	1154	rBV	649313	1248569	24.08%	2.712%
10	10.272	1222	1230	1257	rBV	718584	1668728	32.18%	3.625%
11	10.636	1283	1292	1308	rBV	809725	1476111	28.47%	3.206%
12	10.801	1313	1320	1341	rVV	82593	251379	4.85%	0.546%
13	12.242	1559	1565	1574	rBV5	12019	33971	0.66%	0.074%
14	13.377	1753	1758	1767	rVV	19412	33470	0.65%	0.073%
15	13.471	1769	1774	1776	rVB5	4070	6422	0.12%	0.014%
16	13.901	1840	1847	1861	rBV	1955627	2891088	55.76%	6.280%
17	14.177	1887	1894	1911	rBV	2300416	3602709	69.48%	7.826%
18	14.483	1939	1946	1954	rBV	1230908	1859285	35.86%	4.039%
19	14.777	1988	1996	2008	rBV7	18870	85740	1.65%	0.186%
20	14.895	2013	2016	2022	rVB3	10360	18723	0.36%	0.041%
21	15.477	2107	2115	2132	rBV	2824290	4309578	83.12%	9.361%
22	15.613	2132	2138	2154	rVV	748193	1240037	23.92%	2.694%
23	15.724	2154	2157	2165	rVB3	17239	33953	0.65%	0.074%
24	15.995	2197	2203	2207	rBV9	4794	11665	0.22%	0.025%
25	16.912	2353	2359	2362	rBV8	6686	11923	0.23%	0.026%
26	17.236	2408	2414	2420	rBV	1431255	2071201	39.95%	4.499%
27	17.336	2425	2431	2453	rVB	2979059	4566815	88.08%	9.920%
28	18.142	2564	2568	2573	rBV7	16043	34437	0.66%	0.075%
29	19.201	2743	2748	2754	rBV3	42453	74791	1.44%	0.162%
30	19.271	2756	2760	2763	rVV	34154	54616	1.05%	0.119%
31	19.301	2763	2765	2772	rVB	37041	60225	1.16%	0.131%
32	19.636	2816	2822	2836	rBV	3604551	5185047	100.00%	11.263%
33	21.430	3122	3127	3139	rBV	1395275	2071521	39.95%	4.500%
34	23.641	3496	3503	3518	rVB	2337208	4840344	93.35%	10.514%
35	23.794	3523	3529	3542	rVB2	1023088	2099229	40.49%	4.560%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039502.D
Acq On : 19 Apr 2023 19:17
Operator : CG/JU
Sample : 02296-17
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCBM4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 46037765

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039502.D
Acq On : 19 Apr 2023 19:17
Operator : CG/JU
Sample : 02296-17
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCBM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

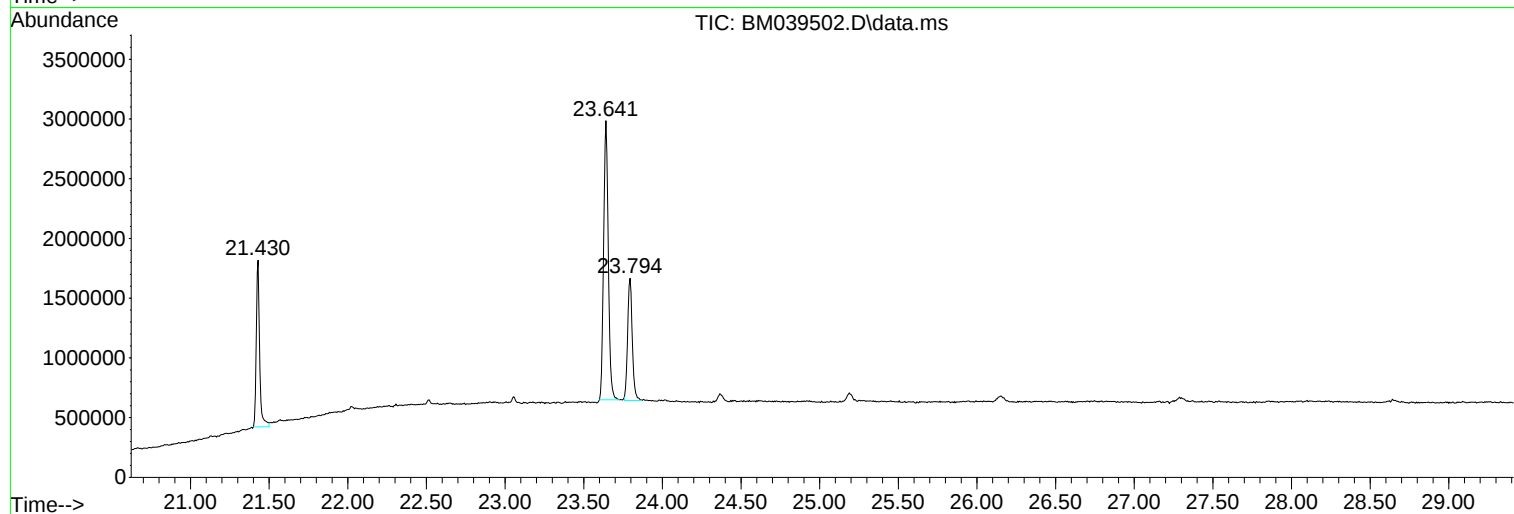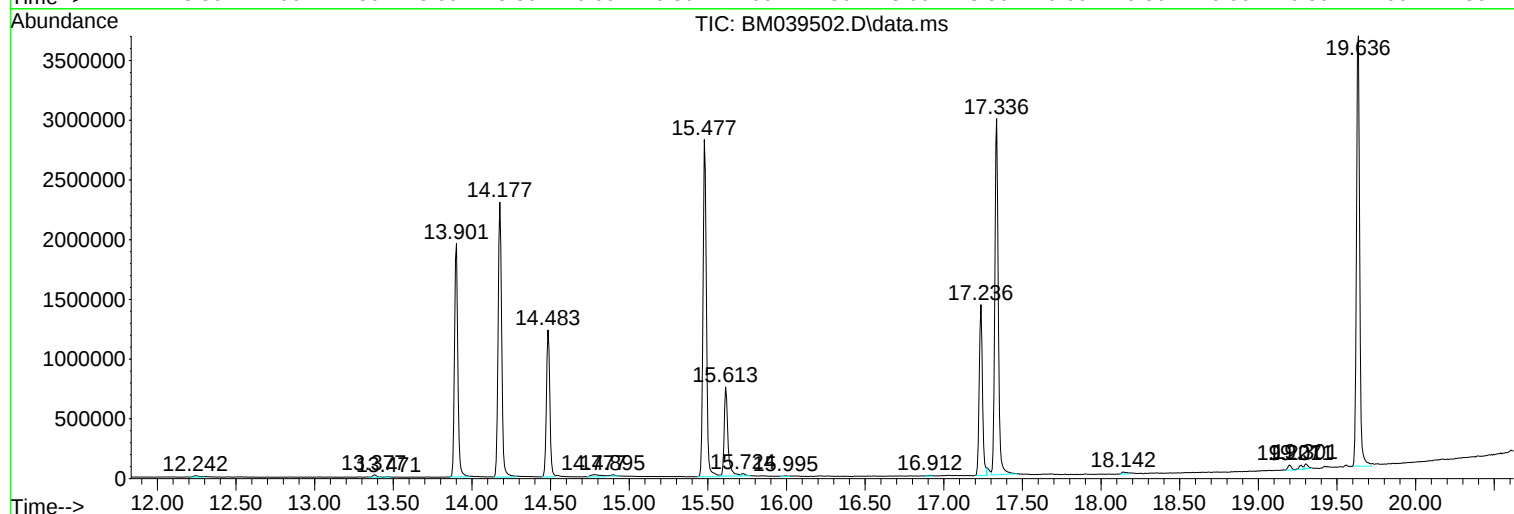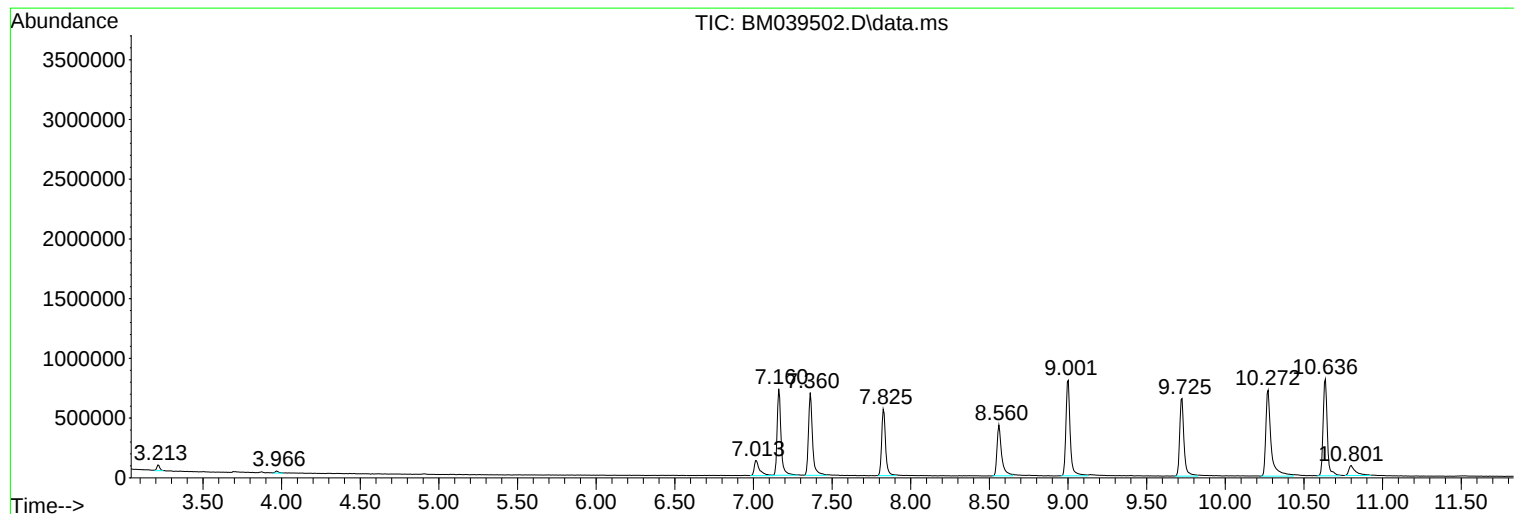

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039502.D
Acq On : 19 Apr 2023 19:17
Operator : CG/JU
Sample : 02296-17
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCBM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039502.D
Acq On : 19 Apr 2023 19:17
Operator : CG/JU
Sample : 02296-17
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCBM4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc