

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039503.D
 Acq On : 19 Apr 2023 19:54
 Operator : CG/JU
 Sample : 02296-18
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCBM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	27	30	37	rVB	54058	66683	1.22%	0.134%
2	3.660	104	106	116	rBV	39938	77742	1.42%	0.156%
3	3.966	156	158	166	rVB2	16555	23661	0.43%	0.048%
4	7.013	670	676	692	rBV	156580	353728	6.45%	0.711%
5	7.160	695	701	723	rVB	772215	1315013	23.99%	2.644%
6	7.360	729	735	754	rBV	752366	1328861	24.25%	2.672%
7	7.825	807	814	825	rBV	578932	1000654	18.26%	2.012%
8	8.560	931	939	957	rBV	504417	1059239	19.33%	2.130%
9	9.001	1005	1014	1036	rBV	859730	1625424	29.66%	3.268%
10	9.160	1038	1041	1049	rVB7	9576	21182	0.39%	0.043%
11	9.719	1128	1136	1153	rBV	704933	1330912	24.28%	2.676%
12	10.272	1222	1230	1254	rBV	815629	1839702	33.57%	3.699%
13	10.636	1283	1292	1309	rBV	836553	1518059	27.70%	3.053%
14	10.795	1312	1319	1330	rBV	154074	408467	7.45%	0.821%
15	12.242	1558	1565	1574	rBV4	11870	27703	0.51%	0.056%
16	13.383	1753	1759	1764	rVB2	15666	28428	0.52%	0.057%
17	13.460	1767	1772	1775	rBV7	4237	7687	0.14%	0.015%
18	13.519	1778	1782	1788	rVB7	3943	6769	0.12%	0.014%
19	13.901	1838	1847	1863	rBV	2131656	3170750	57.85%	6.376%
20	14.177	1887	1894	1912	rBV	2542207	3875513	70.71%	7.793%
21	14.483	1939	1946	1954	rBV	1344227	1990059	36.31%	4.002%
22	14.542	1954	1956	1966	rVB3	20851	36062	0.66%	0.073%
23	14.766	1986	1994	1995	rBV4	24839	49766	0.91%	0.100%
24	14.895	2012	2016	2021	rVB	12624	19327	0.35%	0.039%
25	15.218	2064	2071	2075	rBV3	10246	23112	0.42%	0.046%
26	15.354	2091	2094	2099	rBV7	5495	7582	0.14%	0.015%
27	15.477	2108	2115	2132	rBV	3112244	4664844	85.11%	9.380%
28	15.613	2132	2138	2153	rVV	841342	1337320	24.40%	2.689%
29	15.724	2153	2157	2166	rVB5	19211	39867	0.73%	0.080%
30	15.818	2169	2173	2175	rBV3	4805	7280	0.13%	0.015%
31	15.942	2189	2194	2201	rBV	23859	38634	0.70%	0.078%
32	16.218	2237	2241	2248	rBV6	8847	16050	0.29%	0.032%
33	16.518	2289	2292	2296	rBV6	4498	6873	0.13%	0.014%
34	16.642	2305	2313	2320	rBV4	21614	61364	1.12%	0.123%
35	16.901	2351	2357	2363	rVB3	19982	38533	0.70%	0.077%
36	17.030	2377	2379	2381	rBV3	4869	5557	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039503.D
 Acq On : 19 Apr 2023 19:54
 Operator : CG/JU
 Sample : 02296-18
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCBM6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	17.054	2381	2383	2391	rVB5	9900	16059	0.29%	0.032%
38	17.236	2403	2414	2420	rBV	1513686	2324019	42.40%	4.673%
39	17.336	2425	2431	2449	rVB	3164876	4821516	87.97%	9.695%
40	18.136	2564	2567	2571	rBV4	18986	29606	0.54%	0.060%
41	18.942	2702	2704	2711	rVB7	17889	26912	0.49%	0.054%
42	19.195	2742	2747	2753	rBV2	84124	145097	2.65%	0.292%
43	19.265	2756	2759	2762	rVV	42253	64248	1.17%	0.129%
44	19.301	2762	2765	2771	rVB	42046	65132	1.19%	0.131%
45	19.630	2815	2821	2832	rBV	3960429	5480674	100.00%	11.021%
46	21.430	3122	3127	3138	rBV	1487368	2168356	39.56%	4.360%
47	23.641	3496	3503	3517	rVB2	2472438	4986092	90.98%	10.026%
48	23.794	3523	3529	3540	rVB2	1066989	2174270	39.67%	4.372%




Sum of corrected areas: 49730388

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039503.D
Acq On : 19 Apr 2023 19:54
Operator : CG/JU
Sample : 02296-18
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCBM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

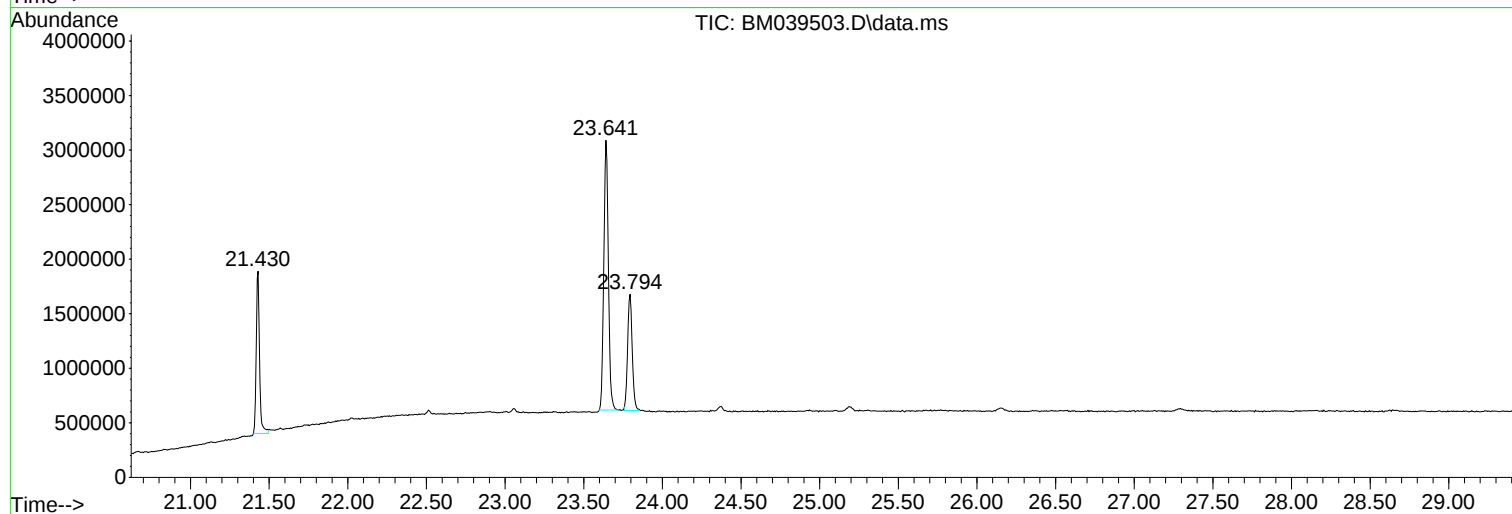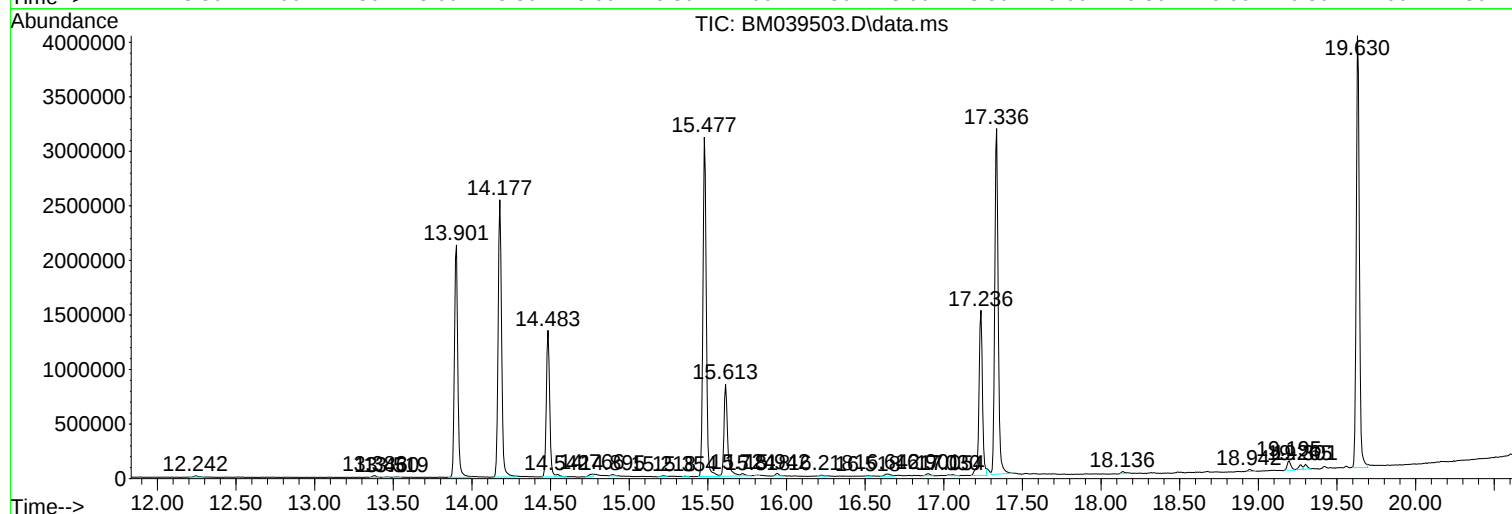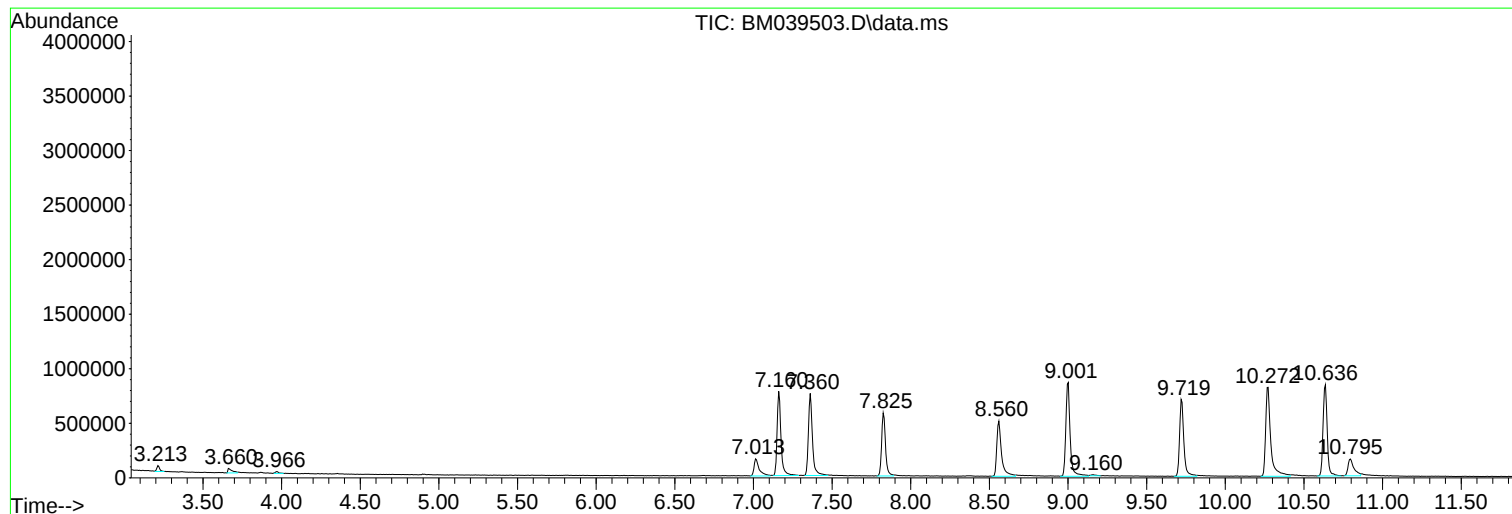

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039503.D
Acq On : 19 Apr 2023 19:54
Operator : CG/JU
Sample : 02296-18
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCBM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039503.D
Acq On : 19 Apr 2023 19:54
Operator : CG/JU
Sample : 02296-18
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCBM6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc