

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039510.D
 Acq On : 20 Apr 2023 00:42
 Operator : CG/JU
 Sample : PB152215BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	26	30	38	rVB	77708	104699	1.73%	0.161%
2	3.637	99	102	123	rBV	820712	1284512	21.17%	1.977%
3	3.966	155	158	163	rVB	16581	20346	0.34%	0.031%
4	7.007	669	675	695	rBV	892659	1666430	27.46%	2.565%
5	7.160	695	701	723	rVB	866035	1478568	24.36%	2.276%
6	7.360	728	735	752	rBV	1029190	1795993	29.60%	2.765%
7	7.825	807	814	830	rBV	855179	1472568	24.27%	2.267%
8	8.554	931	938	956	rBV	1165555	2188075	36.06%	3.368%
9	8.995	1006	1013	1032	rBV	959609	1761474	29.03%	2.711%
10	9.719	1129	1136	1160	rBV	810400	1536602	25.32%	2.365%
11	10.266	1222	1229	1257	rBV	1082942	2208561	36.39%	3.400%
12	10.630	1282	1291	1308	rBV	1314699	2288623	37.71%	3.523%
13	10.783	1310	1317	1354	rVV	980683	2171250	35.78%	3.342%
14	11.060	1362	1364	1374	rVB10	5563	8291	0.14%	0.013%
15	12.254	1561	1567	1568	rBV4	8875	15388	0.25%	0.024%
16	13.377	1752	1758	1766	rBV3	14336	24332	0.40%	0.037%
17	13.901	1838	1847	1867	rBV	2449954	3731359	61.49%	5.744%
18	14.177	1886	1894	1912	rBV	2872453	4404396	72.58%	6.780%
19	14.483	1939	1946	1961	rBV	2084625	3191256	52.59%	4.912%
20	14.724	1981	1987	2008	rBV	318649	983202	16.20%	1.513%
21	15.477	2108	2115	2132	rBV	3544613	5310413	87.51%	8.174%
22	15.613	2132	2138	2152	rVV	889898	1423023	23.45%	2.190%
23	15.713	2153	2155	2164	rVB2	23002	41447	0.68%	0.064%
24	16.907	2354	2358	2363	rBV6	3542	6718	0.11%	0.010%
25	17.236	2407	2414	2424	rBV	2328615	3614648	59.56%	5.564%
26	17.336	2424	2431	2455	rVB	3584439	5579894	91.95%	8.589%
27	19.195	2743	2747	2755	rBV3	42000	63871	1.05%	0.098%
28	19.271	2756	2760	2763	rBV	35280	47817	0.79%	0.074%
29	19.630	2815	2821	2840	rBV	4279877	6068501	100.00%	9.341%
30	21.424	3121	3126	3143	rBV	2031847	3024985	49.85%	4.656%
31	23.636	3495	3502	3519	rBV2	2226549	4723515	77.84%	7.271%
32	23.788	3521	3528	3543	rVB2	1280623	2724086	44.89%	4.193%




Sum of corrected areas: 64964843

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039510.D
Acq On : 20 Apr 2023 00:42
Operator : CG/JU
Sample : PB152215BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

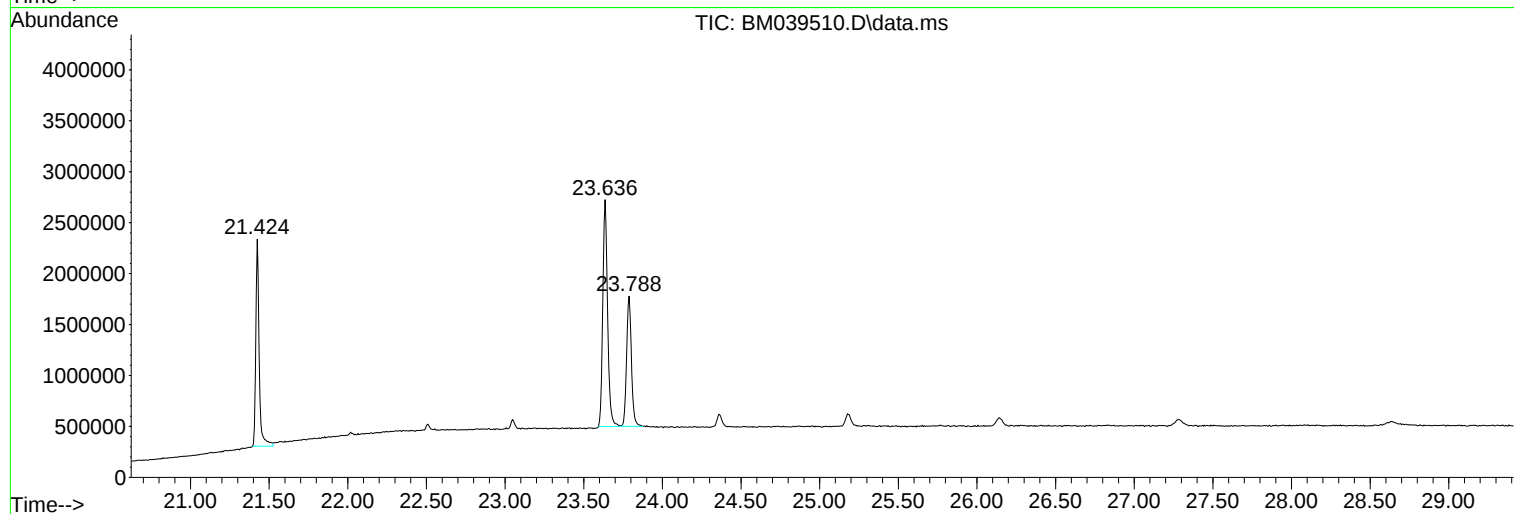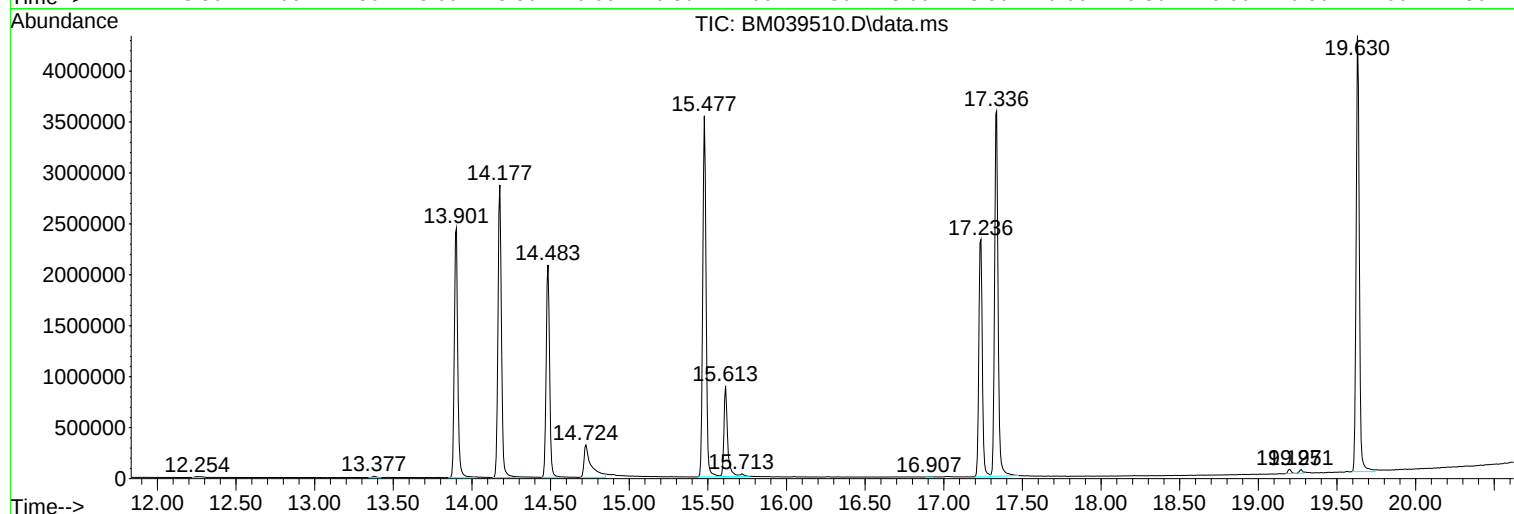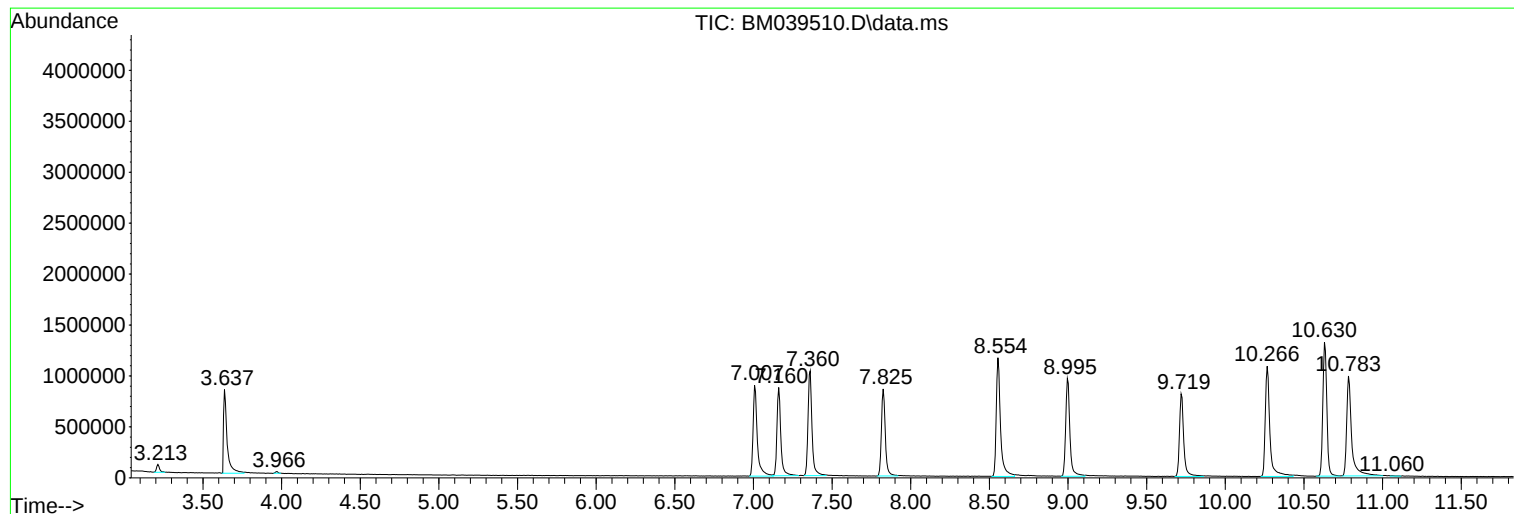

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039510.D
Acq On : 20 Apr 2023 00:42
Operator : CG/JU
Sample : PB152215BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039510.D
Acq On : 20 Apr 2023 00:42
Operator : CG/JU
Sample : PB152215BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------