

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
 Data File : BM039511.D
 Acq On : 20 Apr 2023 01:18
 Operator : CG/JU
 Sample : PB152217BL
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	26	30	39	rVB	65909	92617	1.78%	0.170%
2	3.637	100	102	117	rBV	670204	1062098	20.39%	1.947%
3	3.966	156	158	163	rVB3	15228	18504	0.36%	0.034%
4	7.007	668	675	695	rBV	724570	1373948	26.37%	2.519%
5	7.160	695	701	722	rVB	709818	1208135	23.19%	2.215%
6	7.360	728	735	757	rVB	826111	1477147	28.35%	2.708%
7	7.825	807	814	830	rBV	713139	1232903	23.66%	2.260%
8	8.554	931	938	960	rBV	923281	1801755	34.58%	3.303%
9	8.754	970	972	977	rVB4	4964	6115	0.12%	0.011%
10	8.995	1006	1013	1031	rBV	785802	1447706	27.79%	2.654%
11	9.719	1129	1136	1153	rBV	656580	1238630	23.77%	2.271%
12	10.266	1222	1229	1254	rBV	868909	1796367	34.48%	3.293%
13	10.630	1282	1291	1307	rBV	1120842	1926618	36.98%	3.532%
14	10.783	1311	1317	1354	rVV	771909	1762805	33.84%	3.232%
15	13.377	1752	1758	1766	rBV	26960	44956	0.86%	0.082%
16	13.895	1839	1846	1871	rBV	2089517	3125506	59.99%	5.730%
17	14.177	1886	1894	1913	rBV	2271230	3643056	69.93%	6.679%
18	14.483	1939	1946	1956	rBV	1736129	2694440	51.72%	4.940%
19	14.724	1979	1987	2014	rBV	219384	831170	15.95%	1.524%
20	15.477	2107	2115	2132	rBV	2965094	4480346	86.00%	8.214%
21	15.612	2132	2138	2152	rVV	701509	1169682	22.45%	2.144%
22	15.718	2153	2156	2163	rVB2	19179	33026	0.63%	0.061%
23	17.024	2375	2378	2381	rBV4	4947	7114	0.14%	0.013%
24	17.230	2407	2413	2424	rBV	2069129	3123259	59.95%	5.726%
25	17.330	2424	2430	2452	rVB	3024695	4704677	90.30%	8.625%
26	17.900	2523	2527	2531	rBV6	3968	7564	0.15%	0.014%
27	19.195	2743	2747	2753	rBV	37396	57676	1.11%	0.106%
28	19.271	2756	2760	2764	rBV	29072	46911	0.90%	0.086%
29	19.630	2815	2821	2833	rBV	3801125	5209929	100.00%	9.552%
30	21.424	3121	3126	3142	rBV	1721453	2629823	50.48%	4.821%
31	23.635	3495	3502	3517	rBV2	1894718	3936533	75.56%	7.217%
32	23.782	3521	3527	3542	rVB2	1077935	2354499	45.19%	4.317%




Sum of corrected areas: 54545515

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039511.D
Acq On : 20 Apr 2023 01:18
Operator : CG/JU
Sample : PB152217BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

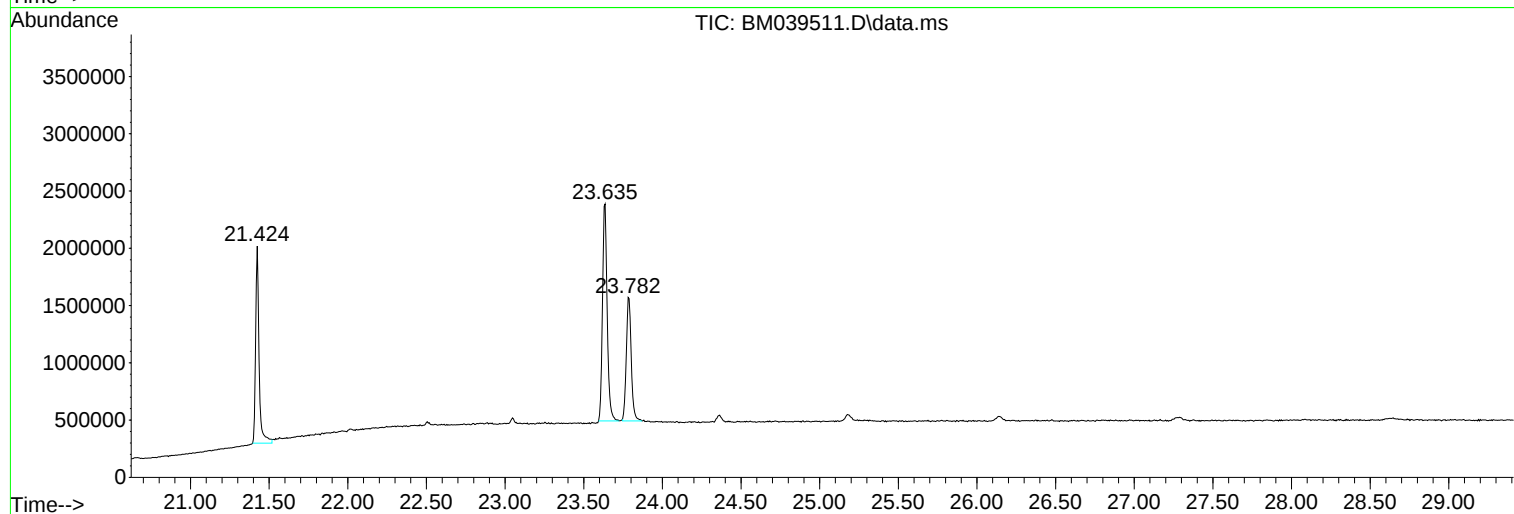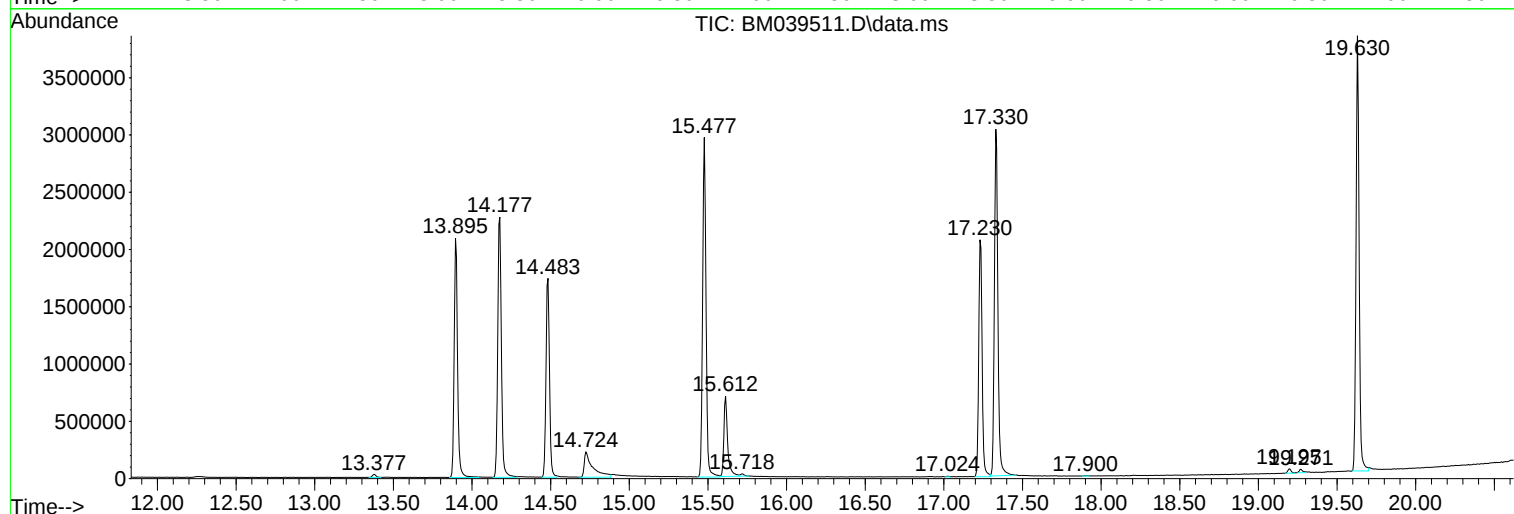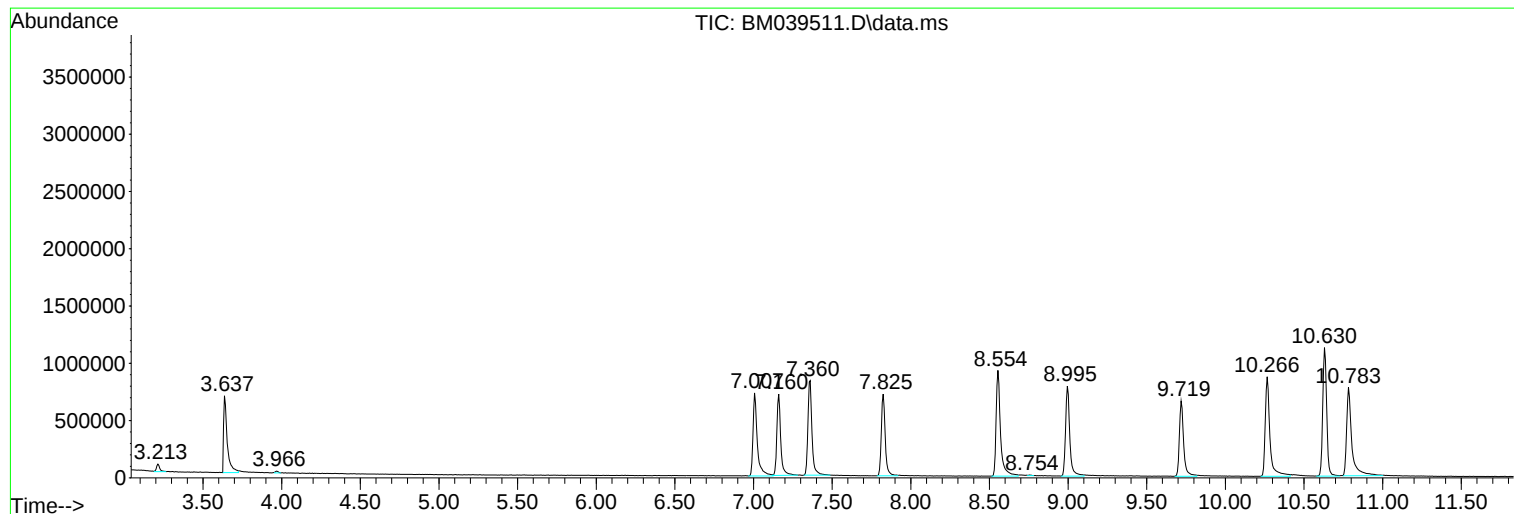

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039511.D
Acq On : 20 Apr 2023 01:18
Operator : CG/JU
Sample : PB152217BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041823\
Data File : BM039511.D
Acq On : 20 Apr 2023 01:18
Operator : CG/JU
Sample : PB152217BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc