

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041917\
 Data File : BM009670.D
 Acq On : 19 Apr 2017 15:52
 Operator : SJ/MA
 Sample : I2691-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAB57

Quant Time: Apr 19 16:38:06 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 19 05:34:35 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	145706	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	553299	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	302275	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.23	188	695401	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	958074	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	949922	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	4190	1.06	ng/uL	0.00
5) Phenol-d5	6.99	99	99711	7.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	72649	7.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	71608	7.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	75218	7.67	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	33257	7.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	32324	7.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	64821	7.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	71055	7.90	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	204596	8.39	ng/ul	0.00
46) Acenaphthylene-d8	14.17	160	249189	8.08	ng/ul	0.00
51) 4-Nitrophenol-d4	14.68	143	21725	4.96	ng/ul	0.00
57) Fluorene-d10	15.47	176	207528	9.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	16440	3.71	ng/ul	0.00
70) Anthracene-d10	17.33	188	335587	9.96	ng/ul	0.00
76) Pyrene-d10	19.62	212	423978	10.28	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	457625	10.65	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.93	163	134522	5.49	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041917\
Data File : BM009670.D
Acq On : 19 Apr 2017 15:52
Operator : SJ/MA
Sample : I2691-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAB57

Quant Time: Apr 19 16:38:06 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041717.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 05:34:35 2017
Response via : Initial Calibration

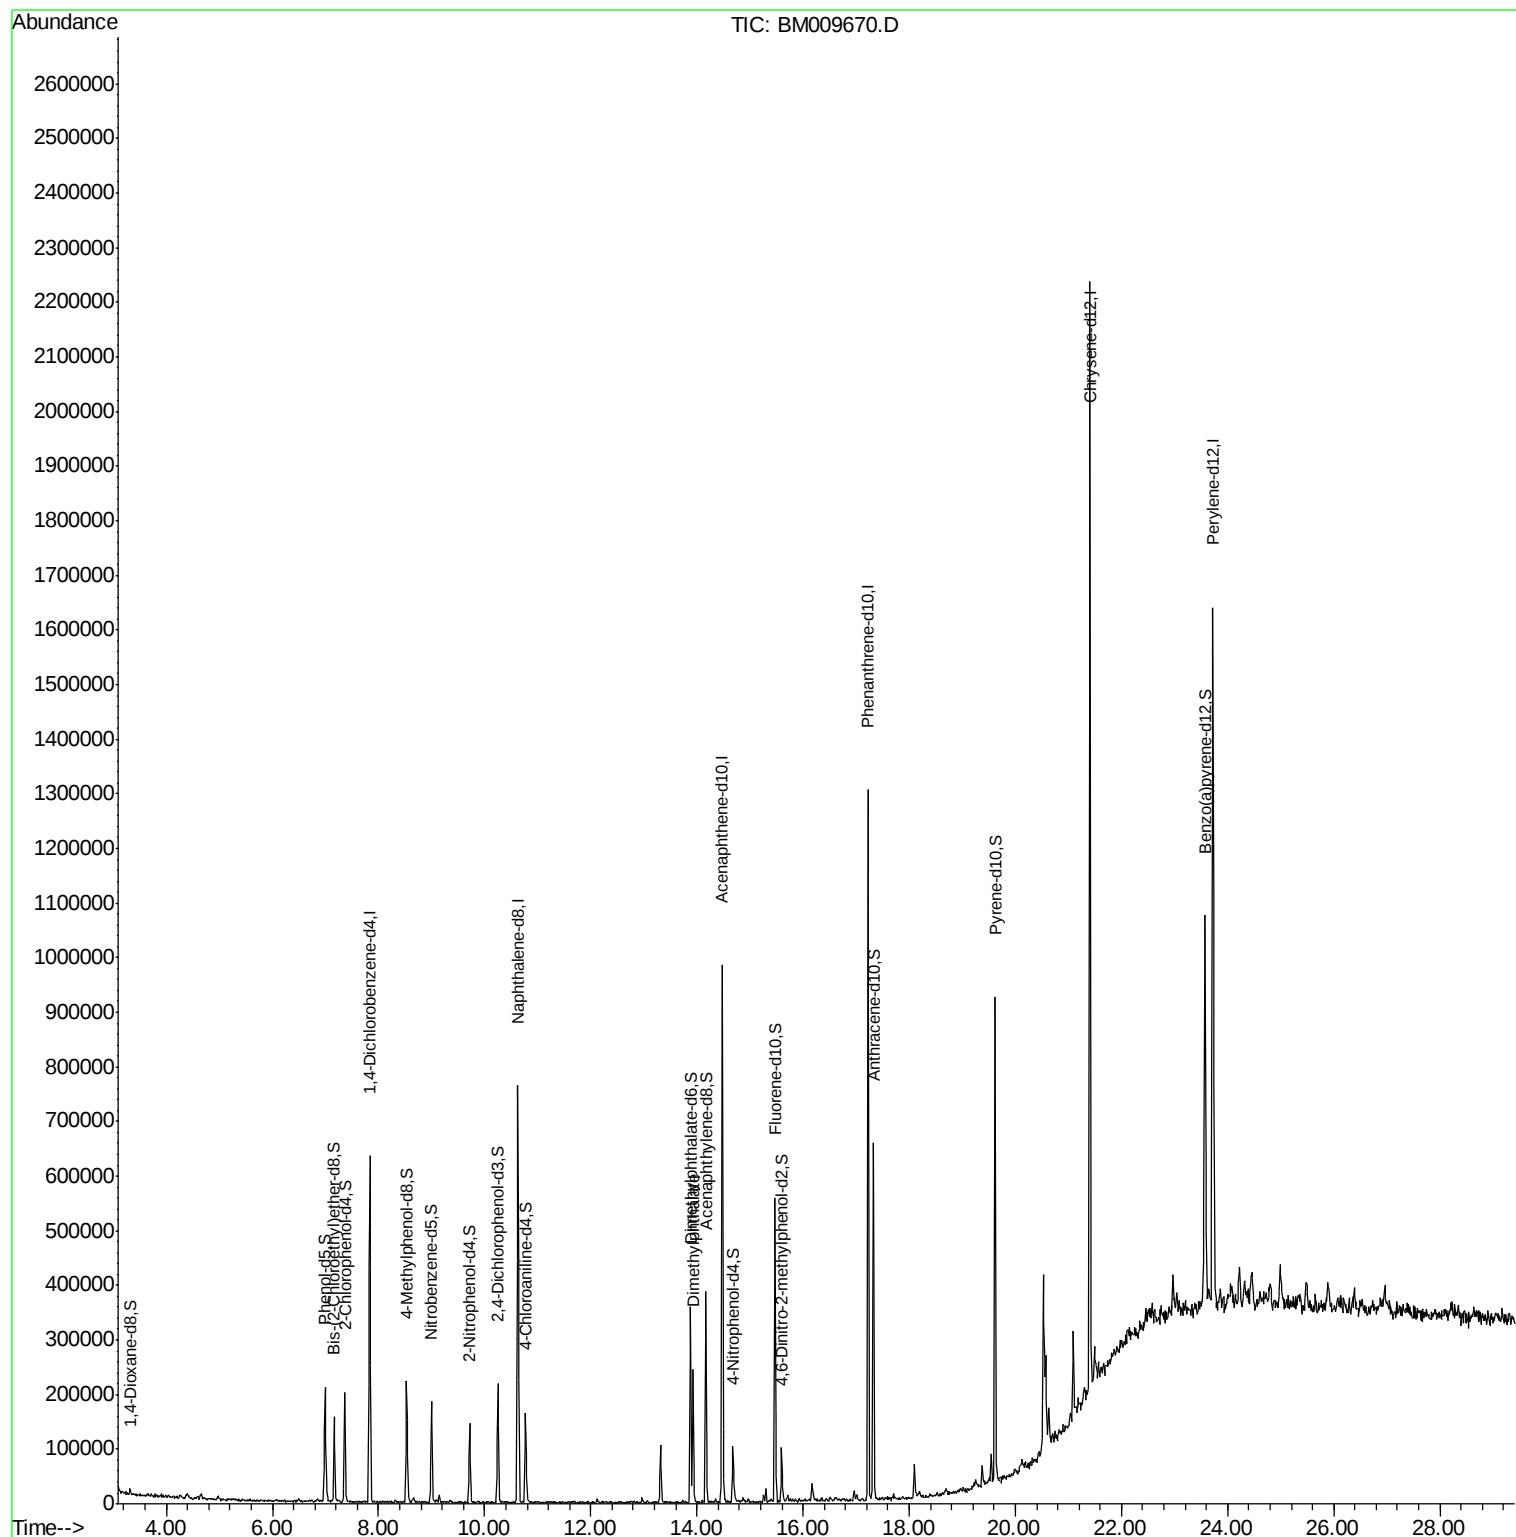

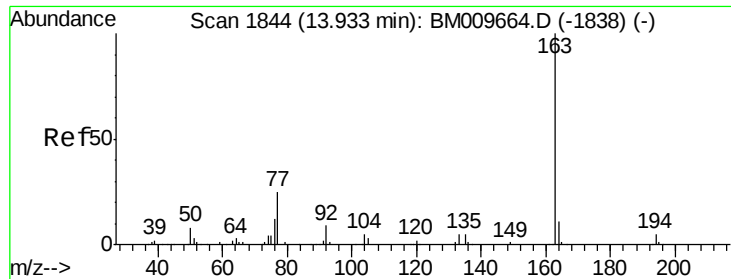

#44

Dimethylphthalate

Concen: 5.49 ng/ul

RT: 13.93 min Scan# 1843

Delta R.T. -0.01 min

Lab File: BM009670.D

Acq: 19 Apr 2017 15:52

Instrument :

BNA_M

ClientSampleId :

YAB57


Tgt Ion:163 Resp: 134522

Ion Ratio Lower Upper

163 100

194 4.0 3.0 4.6

164 11.5 8.6 12.8

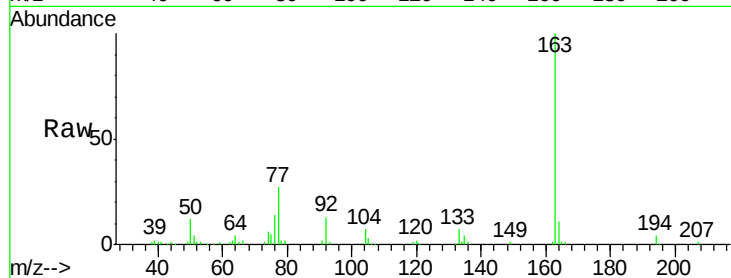

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

