


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041917\
 Data File : BM009663.D
 Acq On : 19 Apr 2017 11:36
 Operator : SJ/MA
 Sample : DFTPP03
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP03

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
 Title : SVOA CALIBRATION
 Last Update : Wed Nov 30 00:32:18 2016

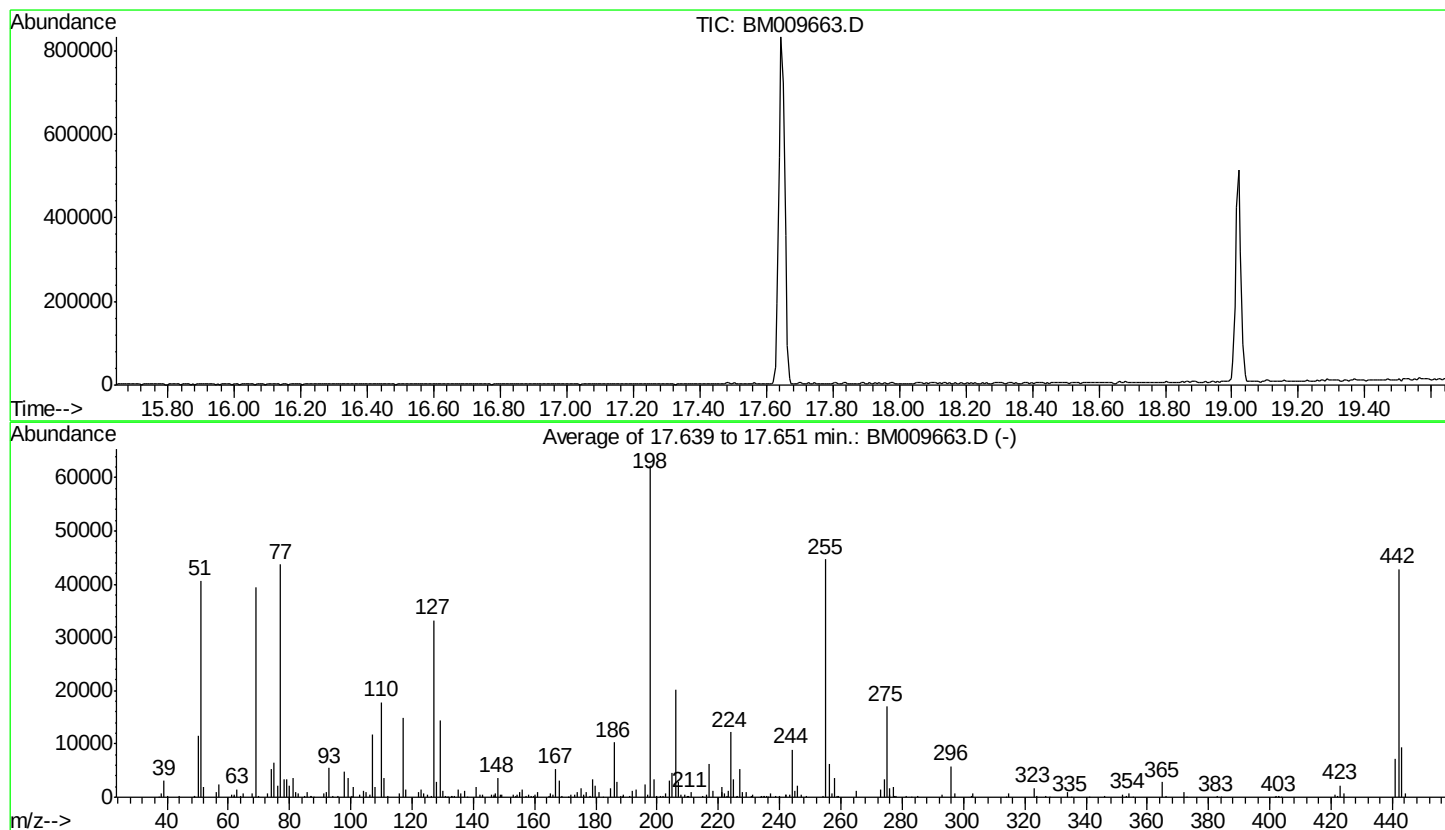

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.3	40666	PASS
68	69	0.00	2	1.8	717	PASS
69	198	0.00	100	63.4	39504	PASS
70	69	0.00	2	0.4	170	PASS
127	198	10	80	53.4	33253	PASS
197	198	0.00	2	1.0	598	PASS
198	198	100	100	100.0	62261	PASS
199	198	5	9	5.6	3465	PASS
275	198	10	60	27.3	16981	PASS
365	198	1	100	4.5	2821	PASS
441	443	0.01	100	77.8	7235	PASS
442	198	50	100	68.9	42906	PASS
443	442	15	24	21.7	9304	PASS

m/z	Abundance
38.00	623.0
39.10	3181.0
39.90	920.0
44.10	473.0
49.20	374.0
50.00	9834.0
51.10	39704.0
52.00	1885.0
56.00	967.0
57.00	1599.0
61.00	628.0
61.80	428.0
62.90	1156.0
65.10	613.0
67.90	805.0
69.00	33504.0
73.00	1581.0
74.10	4358.0
75.00	6295.0
75.90	1844.0
77.10	37920.0
78.00	2300.0
79.00	2190.0
80.00	1703.0
80.90	2926.0
81.90	998.0
82.90	524.0
84.90	555.0
85.90	857.0
87.20	386.0
91.00	385.0
91.90	845.0
92.90	4822.0
96.00	599.0
98.00	4347.0
99.00	3528.0
100.90	1362.0
103.00	421.0
104.00	1058.0
105.00	869.0
106.00	336.0
107.00	10642.0
108.00	1949.0
110.00	14210.0
110.90	2765.0
116.00	624.0
117.00	13347.0
118.00	1326.0
122.00	1082.0
123.10	1390.0
123.90	489.0
127.00	26808.0
127.90	2118.0
129.00	11480.0
129.90	1055.0
130.90	410.0
131.90	349.0
132.80	351.0
135.00	953.0
136.00	640.0
137.00	854.0
140.90	1134.0
141.90	410.0
142.90	1019.0
146.80	897.0
147.20	872.0
147.90	3184.0
148.90	618.0
152.90	301.0
153.90	473.0
155.10	1094.0
155.90	1541.0
158.00	544.0
159.10	332.0
160.00	402.0
161.00	1048.0
164.80	972.0
165.90	412.0
167.00	4222.0
168.00	1951.0
169.10	348.0
172.10	340.0
172.90	500.0
174.10	562.0
175.00	1588.0
175.80	413.0
176.80	827.0
178.90	2298.0
179.90	2033.0
180.90	1235.0
185.00	999.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

186.00	6680.0
187.00	1970.0
188.90	888.0
192.00	1304.0
193.00	1124.0
196.00	1685.0
196.70	436.0
197.90	47592.0
198.90	2931.0
200.00	490.0
201.10	334.0
203.00	521.0
203.90	2779.0
204.90	3882.0
206.00	14651.0
207.00	4451.0
207.90	1079.0
208.90	321.0
211.10	545.0
216.90	4506.0
217.90	611.0
220.90	2777.0
221.90	430.0
222.80	890.0
223.20	925.0
224.00	9551.0
225.00	2667.0
225.70	301.0
226.90	3618.0
227.90	602.0
229.00	707.0
230.80	516.0
235.70	448.0
236.90	441.0
241.90	618.0
243.00	380.0
244.00	6245.0
245.00	963.0
246.00	1344.0
247.10	326.0
255.00	29328.0
256.00	4179.0
256.80	561.0
257.90	2429.0
264.90	885.0
273.00	1047.0
274.00	2371.0
275.00	11129.0
275.80	1455.0
277.00	1654.0
293.00	607.0
296.00	4330.0
297.10	528.0
303.00	618.0
313.70	376.0
314.90	554.0
323.00	1279.0
324.00	429.0
333.90	618.0
353.90	745.0
365.00	1395.0
366.00	335.0
372.10	804.0
401.80	364.0
421.10	584.0
422.90	1629.0
424.00	425.0
441.00	4187.0
442.00	26088.0
443.00	5282.0
444.00	420.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

m/z	Abundance
38.00	879.0
39.00	3582.0
40.10	786.0
43.90	646.0
49.10	519.0
50.10	13647.0
51.00	47120.0
52.00	2027.0
56.00	1274.0
57.00	2704.0
60.90	918.0
62.00	544.0
63.00	2048.0
64.00	454.0
64.90	751.0
67.90	1346.0
69.00	47112.0
70.00	511.0
73.00	924.0
74.00	7049.0
75.00	7220.0
76.00	2559.0
77.10	52456.0
78.00	3522.0
79.00	4535.0
80.00	2908.0
81.00	4221.0
82.00	967.0
82.90	997.0
84.80	533.0
85.90	1155.0
86.90	492.0
91.00	1141.0
92.00	1185.0
93.00	6194.0
94.00	475.0
95.90	431.0
97.90	5426.0
99.00	3247.0
99.90	306.0
101.00	2526.0
102.90	899.0
104.00	1325.0
104.90	1305.0
106.10	789.0
106.90	14122.0
107.90	2378.0
110.00	20112.0
111.00	4685.0
112.00	437.0
116.00	876.0
117.00	17584.0
118.10	1784.0
122.00	1267.0
122.90	1756.0
123.90	788.0
125.00	736.0
127.00	39840.0
128.00	3506.0
129.00	17216.0
130.00	1242.0
132.80	323.0
133.90	555.0
135.00	1946.0
136.10	879.0
137.10	1882.0
137.90	318.0
141.00	2385.0
142.00	846.0
143.10	594.0
146.00	966.0
147.00	1521.0
148.00	3804.0
148.80	532.0
153.00	499.0
154.10	421.0
155.10	1406.0
156.00	1643.0
157.20	351.0
157.90	551.0
159.00	558.0
159.90	837.0
160.80	1150.0
165.10	1323.0
165.80	465.0
167.00	7079.0
167.90	4743.0
169.00	427.0
170.80	323.0
171.10	305.0
171.90	637.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

172.90	913.0
174.00	1305.0
174.90	1663.0
176.20	563.0
176.90	805.0
178.10	549.0
178.90	3731.0
180.00	2332.0
181.00	934.0
182.10	345.0
185.00	1541.0
186.00	13094.0
186.90	3142.0
187.90	574.0
188.90	891.0
191.00	365.0
191.90	1336.0
193.00	1621.0
196.00	2609.0
196.80	949.0
197.90	73096.0
198.90	4446.0
201.20	560.0
201.80	399.0
202.80	939.0
204.00	3841.0
205.00	5219.0
206.00	25024.0
207.00	4734.0
207.80	742.0
208.90	631.0
210.40	612.0
211.00	1194.0
214.80	450.0
215.90	792.0
216.90	6771.0
218.00	2057.0
221.20	3269.0
221.80	1469.0
223.00	1192.0
224.00	14424.0
225.00	4134.0
226.00	534.0
226.90	5828.0
227.90	1113.0
228.90	1511.0
231.00	614.0
233.80	373.0
234.90	738.0
235.80	308.0
236.90	1487.0
238.80	611.0
239.80	348.0
241.70	840.0
242.10	788.0
243.10	710.0
244.00	11277.0
244.90	1549.0
245.90	2532.0
247.00	475.0
248.80	444.0
254.10	554.0
255.00	53944.0
256.00	7992.0
256.90	589.0
258.00	5000.0
258.90	1101.0
264.80	951.0
273.00	1747.0
274.00	4021.0
275.00	18032.0
276.00	2766.0
277.00	1988.0
277.70	450.0
281.20	436.0
285.00	499.0
293.00	324.0
296.00	6210.0
297.00	1153.0
302.70	675.0
303.00	670.0
314.80	543.0
323.00	1943.0
324.00	354.0
326.90	493.0
333.90	1478.0
335.00	325.0
341.00	325.0
352.10	460.0
353.00	440.0
353.90	462.0
355.10	348.0
365.00	3697.0
372.00	903.0
384.10	383.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

402.10	556.0
402.70	328.0
421.10	728.0
421.90	419.0
423.00	2533.0
424.10	879.0
441.00	9052.0
442.00	48680.0
443.10	10902.0
444.00	781.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

m/z	Abundance
37.10	330.0
38.00	533.0
39.00	2605.0
39.90	703.0
44.10	728.0
48.90	389.0
50.10	11194.0
51.10	35176.0
52.10	2089.0
56.10	1027.0
57.00	2821.0
61.90	731.0
63.00	1351.0
64.10	306.0
65.00	721.0
69.00	37896.0
73.00	1434.0
74.00	4561.0
75.00	5844.0
76.00	1918.0
77.00	40664.0
78.10	4155.0
78.90	3175.0
79.90	1958.0
81.00	3451.0
82.00	753.0
83.00	713.0
85.90	795.0
87.90	306.0
91.00	930.0
92.00	714.0
93.00	5286.0
94.00	548.0
98.00	4527.0
98.90	3784.0
100.30	426.0
101.00	1601.0
102.80	392.0
104.00	1588.0
104.90	822.0
106.90	10592.0
108.00	1376.0
110.00	19168.0
111.00	3430.0
116.00	880.0
117.00	13600.0
117.90	1287.0
122.00	696.0
122.90	1501.0
123.90	672.0
125.00	492.0
126.20	410.0
127.00	33112.0
128.00	2714.0
129.00	14447.0
130.10	1358.0
131.10	383.0
133.10	504.0
134.90	1189.0
135.90	332.0
136.90	810.0
141.00	2327.0
142.10	411.0
143.00	811.0
146.00	434.0
146.90	1508.0
147.90	4107.0
149.10	1117.0
153.00	603.0
154.10	915.0
155.10	702.0
155.90	1241.0
157.20	454.0
157.90	629.0
159.70	799.0
161.00	731.0
165.00	1076.0
165.80	392.0
167.00	4686.0
168.00	2955.0
172.10	531.0
173.00	370.0
174.10	1111.0
175.00	2167.0
176.00	645.0
176.90	1263.0
178.10	375.0
179.00	4282.0
180.00	2080.0
181.00	812.0
184.90	2617.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

186.00	10970.0
186.90	3550.0
188.60	351.0
189.10	881.0
191.00	579.0
191.90	962.0
193.10	1314.0
195.90	2709.0
196.70	411.0
197.10	320.0
197.90	66096.0
198.90	3020.0
201.80	509.0
202.90	665.0
203.90	2802.0
205.00	4896.0
206.00	20944.0
207.00	3727.0
208.10	708.0
208.90	442.0
209.90	574.0
210.90	927.0
214.90	345.0
215.90	443.0
216.90	7515.0
218.00	1127.0
221.00	3058.0
222.00	1074.0
223.00	1175.0
224.00	12757.0
225.00	3303.0
227.00	6212.0
228.00	908.0
228.90	890.0
231.00	761.0
234.00	458.0
235.10	653.0
236.10	357.0
236.80	500.0
238.80	359.0
239.80	363.0
242.10	731.0
243.00	685.0
244.00	9410.0
245.00	1334.0
245.90	2492.0
246.90	485.0
255.00	50728.0
256.00	6388.0
256.90	707.0
257.90	3426.0
259.10	472.0
264.80	1603.0
272.90	1907.0
274.00	3638.0
275.00	21784.0
276.10	2544.0
277.00	2290.0
277.90	525.0
281.00	646.0
283.00	365.0
292.80	381.0
295.90	6847.0
297.10	860.0
303.00	685.0
314.90	1138.0
323.00	2117.0
323.90	326.0
326.80	303.0
327.90	365.0
333.90	655.0
345.90	592.0
351.90	668.0
354.00	728.0
364.90	3373.0
366.00	432.0
372.00	1246.0
372.80	317.0
382.80	502.0
402.90	679.0
403.80	314.0
421.00	482.0
421.90	508.0
423.10	2706.0
424.10	808.0
441.00	8468.0
442.10	53952.0
443.00	11728.0
444.10	723.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

m/z	Abundance
40.00	627.0
44.10	358.0
72.90	626.0
207.10	1373.0
208.00	656.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03