

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041918\
 Data File : BM014747.D
 Acq On : 19 Apr 2018 23:17
 Operator : SJ/JU
 Sample : J2434-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB9

Quant Time: Apr 20 01:29:23 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 20 01:26:25 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.55	152	341405	20.00	ng/ul	0.00
18) Naphthalene-d8	11.39	136	1437861	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.14	164	762736	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.86	188	1579004	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1511166	20.00	ng/ul	0.00
83) Perylene-d12	24.44	264	1564466	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.68	96	38775	4.96	ng/uL	0.00
5) Phenol-d5	7.66	99	687096	26.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.85	67	467183	27.60	ng/ul	0.00
9) 2-Chlorophenol-d4	8.06	132	592397	26.83	ng/ul	0.00
13) 4-Methylphenol-d8	9.24	113	572171	27.18	ng/ul	0.00
19) Nitrobenzene-d5	9.73	128	272998	26.26	ng/ul	0.00
22) 2-Nitrophenol-d4	10.46	143	269611	26.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.99	165	539719	25.66	ng/ul	0.00
29) 4-Chloroaniline-d4	11.51	131	729246	35.12	ng/ul	0.00
43) Dimethylphthalate-d6	14.53	166	1597111	26.82	ng/ul	0.00
46) Acenaphthylene-d8	14.84	160	2059252	28.01	ng/ul	0.00
51) 4-Nitrophenol-d4	15.30	143	199108	18.02	ng/ul	0.00
57) Fluorene-d10	16.12	176	1384155	26.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.22	200	137810	16.13	ng/ul	0.00
70) Anthracene-d10	17.95	188	2031800	27.61	ng/ul	0.00
76) Pyrene-d10	20.19	212	2100837	29.38	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.28	264	2045313	26.61	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.58	163	218553	3.797	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041918\
Data File : BM014747.D
Acq On : 19 Apr 2018 23:17
Operator : SJ/JU
Sample : J2434-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB9

Quant Time: Apr 20 01:29:23 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 20 01:26:25 2018
Response via : Initial Calibration

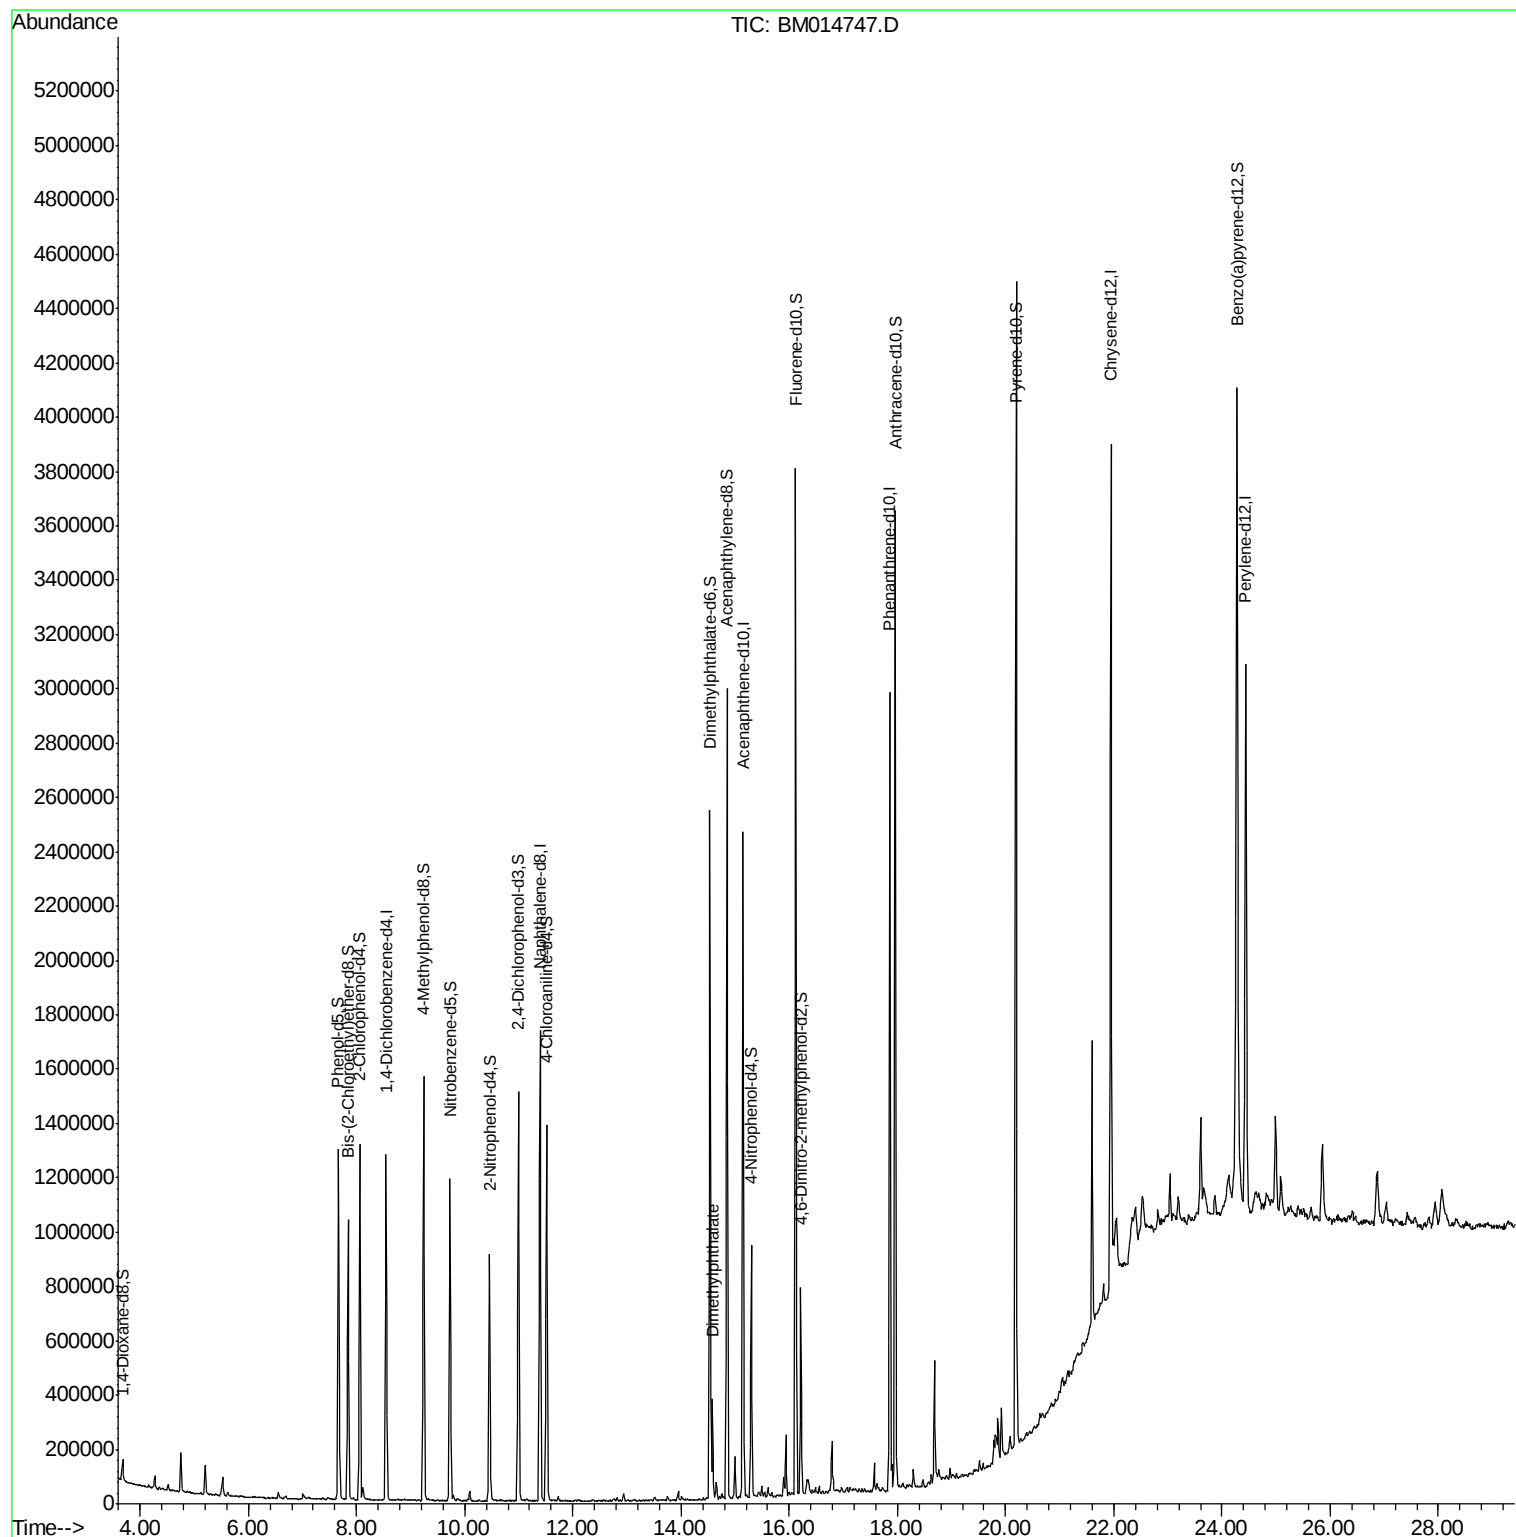

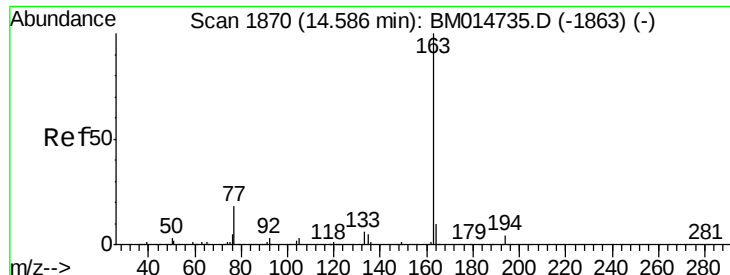

#44

Dimethylphthalate

Concen: 3.797 ng/ul

RT: 14.58 min Scan# 1869

Delta R.T. -0.01 min

Lab File: BM014747.D

Acq: 19 Apr 2018 23:17

Instrument :

BNA_M

ClientSampleId :

C0AB9



Tot Ion:163 Resp: 218553

Ion Ratio Lower Upper

163 100

194 3.7 3.5 5.3

164 9.5 8.2 12.4

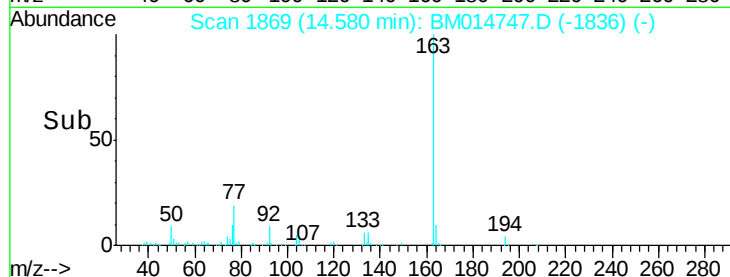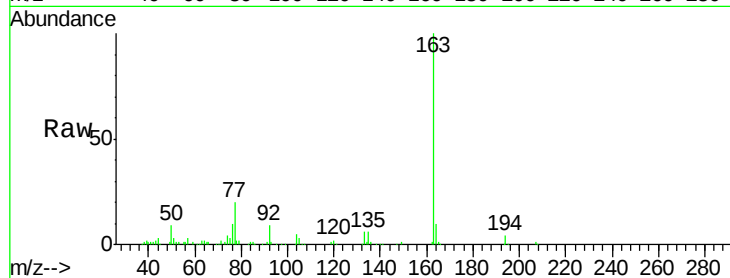

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

