
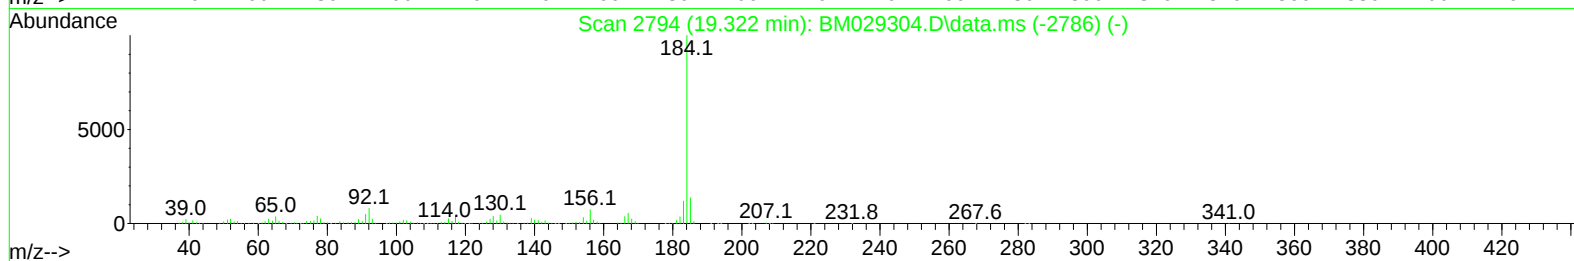
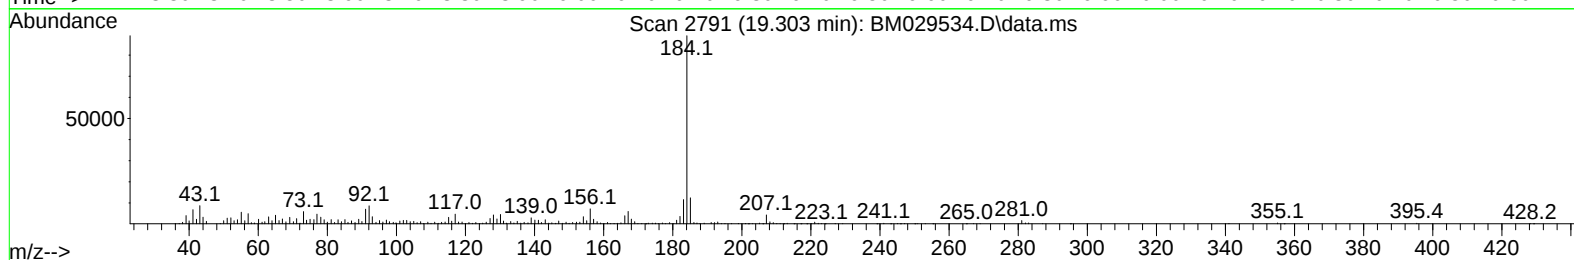


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041921\
Data File : BM029534.D
Acq On : 19 Apr 2021 10:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 11:37:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 11:56:50 2021
Response via : Initial Calibration

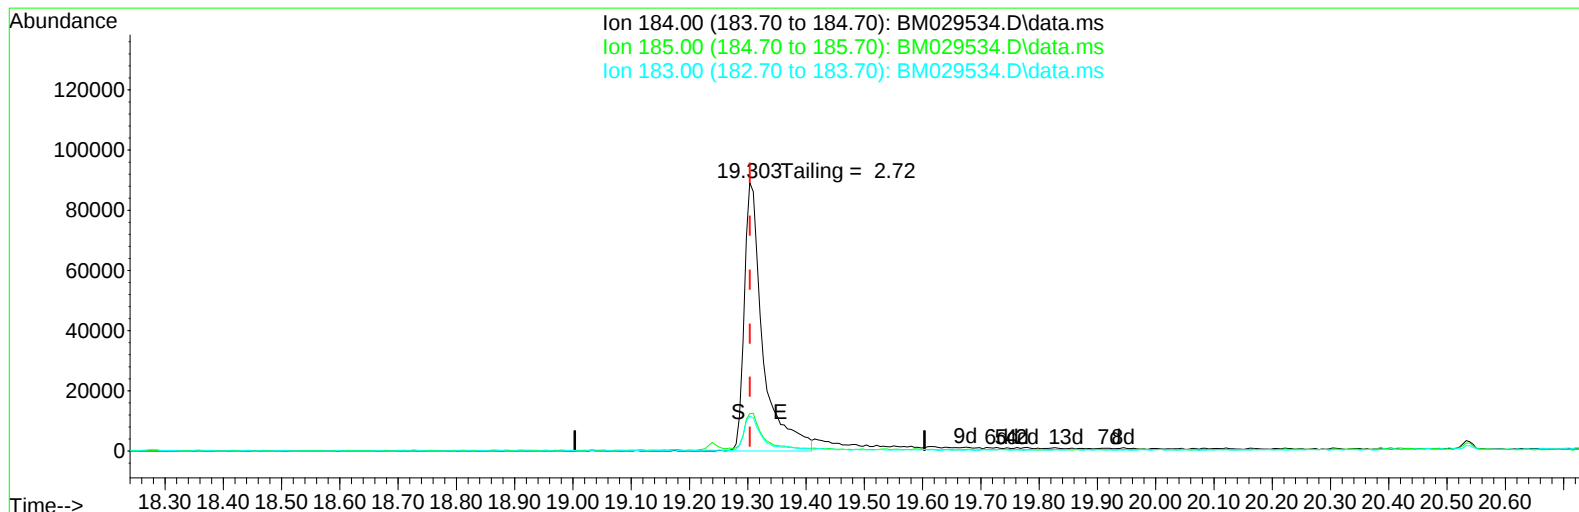

TIC: BM029534.D\data.ms

(77) Benzidine




19.303min (-0.000) 13531.06 ng m

response 230401

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.91
183.00	12.20	13.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041921\
Data File : BM029534.D
Acq On : 19 Apr 2021 10:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 11:37:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 11:56:50 2021
Response via : Initial Calibration

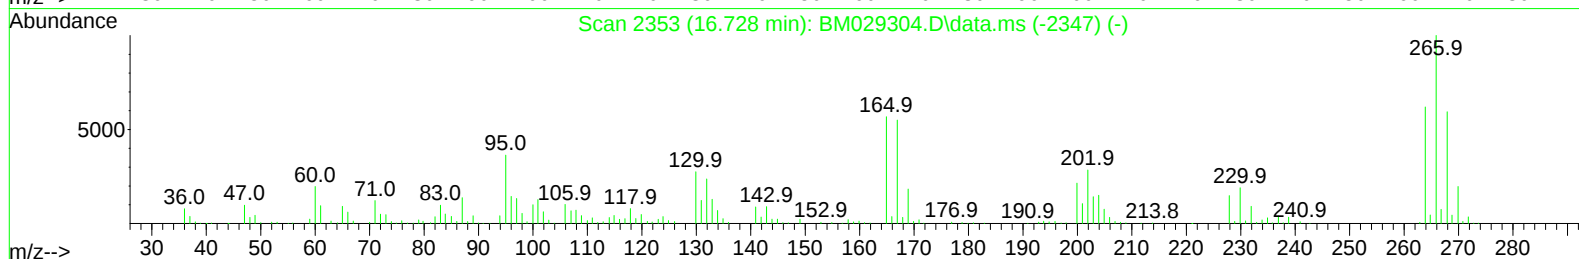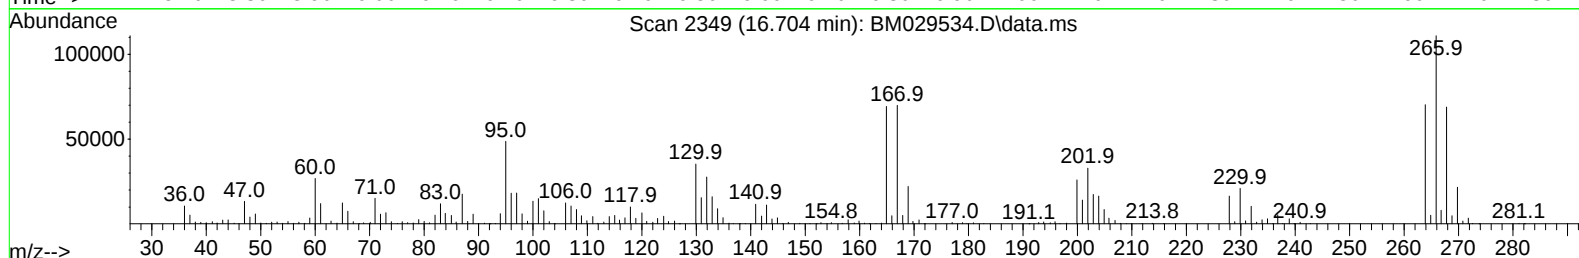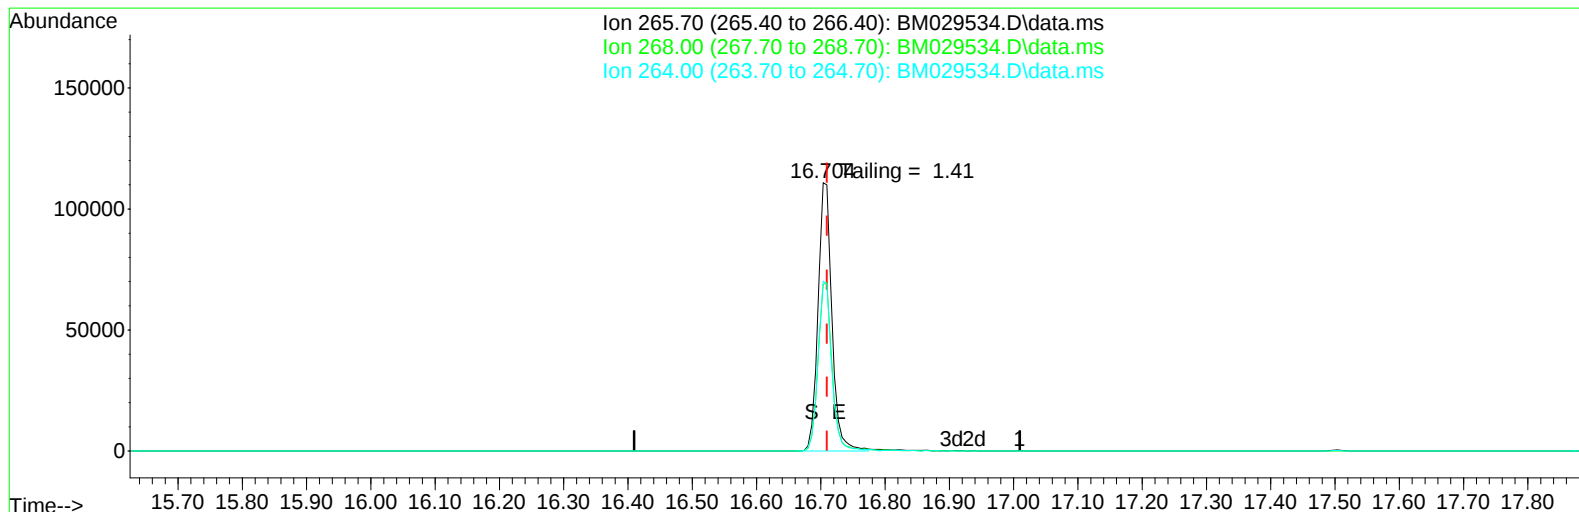

TIC: BM029534.D\data.ms

(70) Pentachlorophenol (C)

16.704min (-0.006) 22473.17 ng m

response 169192

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	62.07
264.00	63.60	63.33
0.00	0.00	0.00