
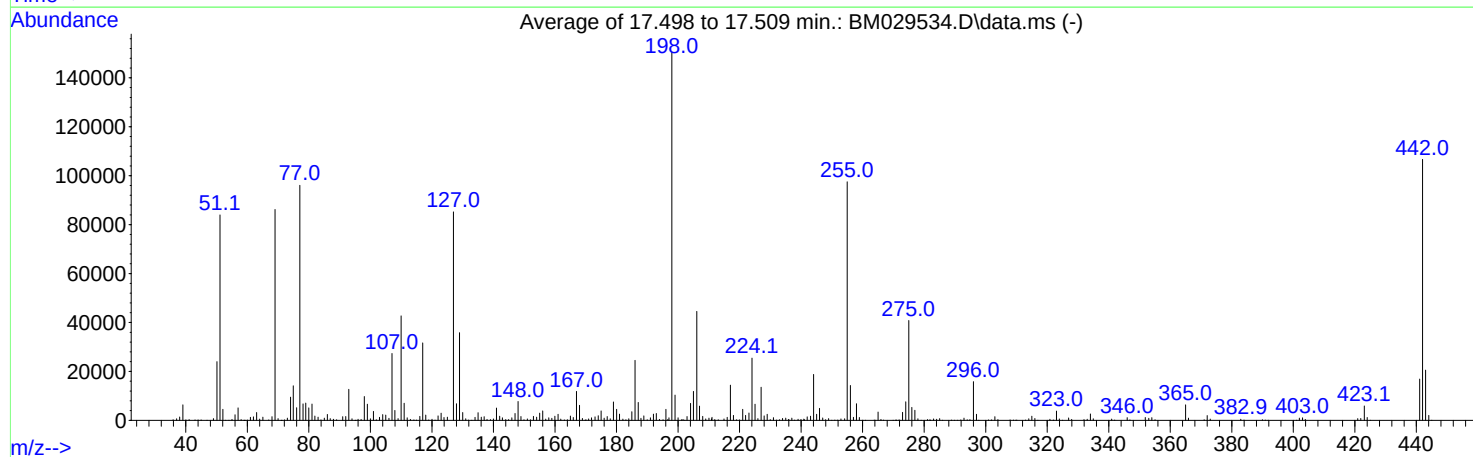


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041921\
 Data File : BM029534.D
 Acq On : 19 Apr 2021 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 11:56:50 2021

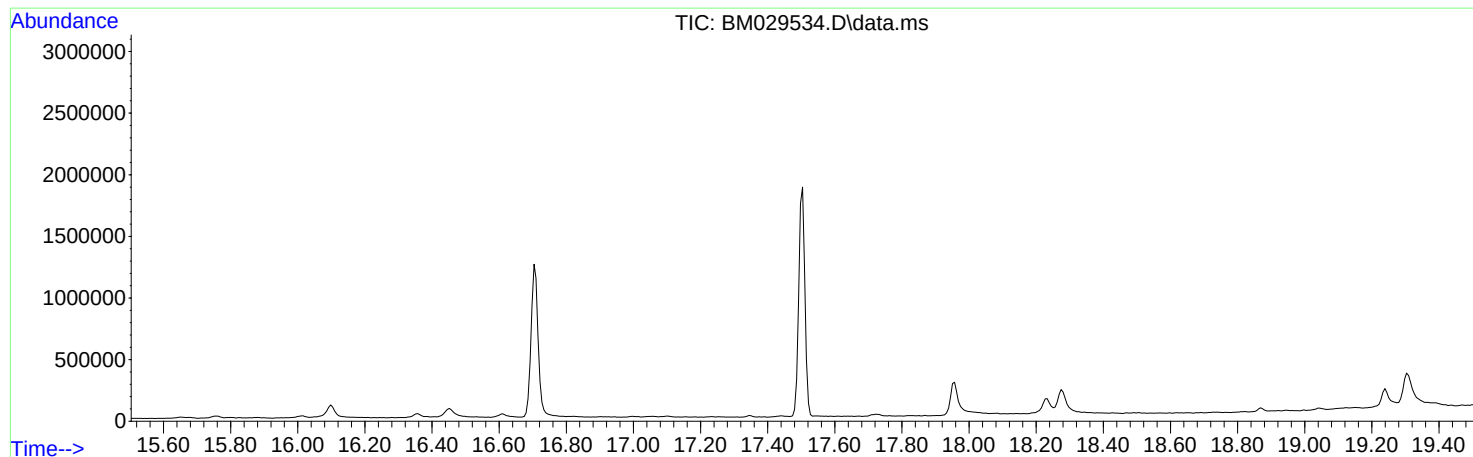




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	83989	PASS
68	69	0.00	2	1.8	1529	PASS
69	198	0.00	100	57.3	86225	PASS
70	69	0.00	2	0.8	732	PASS
127	198	10	80	56.7	85243	PASS
197	198	0.00	2	0.7	1076	PASS
198	198	100	100	100.0	150357	PASS
199	198	5	9	6.9	10315	PASS
275	198	10	60	27.2	40824	PASS
365	198	1	100	4.2	6333	PASS
441	198	0.01	100	11.2	16853	PASS
442	442	50	100	100.0	106645	PASS
443	442	15	24	19.3	20547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041921\
Data File : BM029534.D
Acq On : 19 Apr 2021 10:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 19 11:37:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 11:56:50 2021
Response via : Initial Calibration

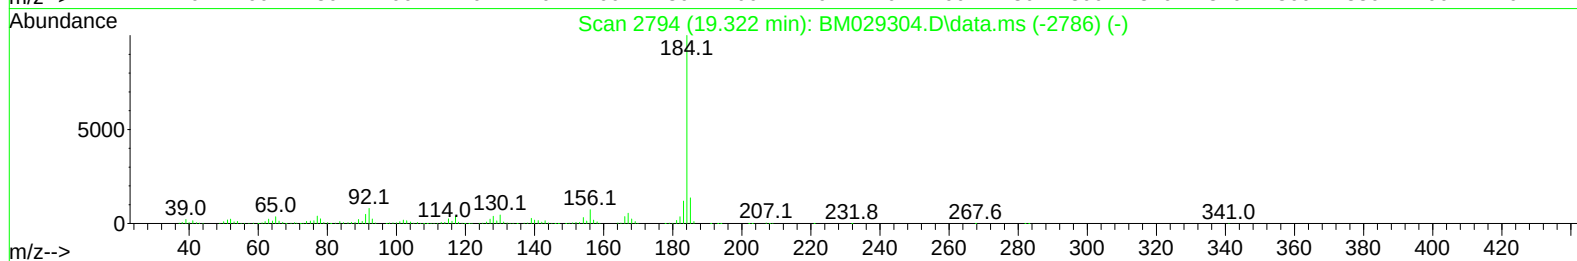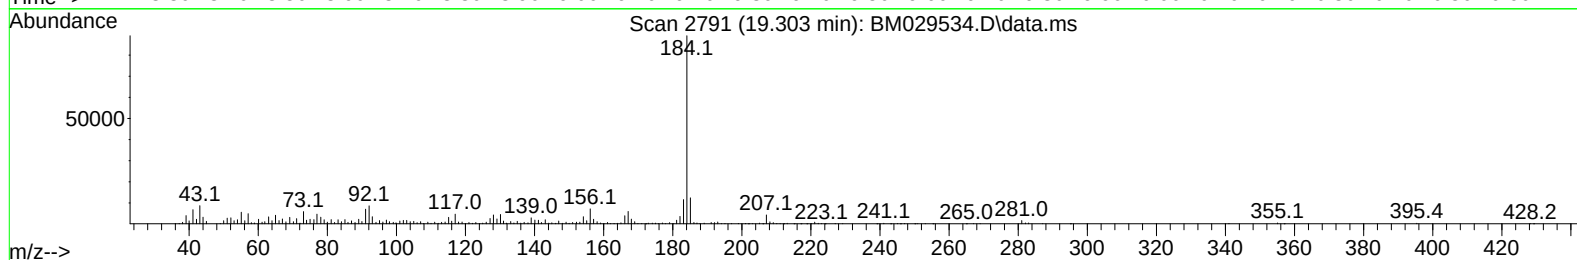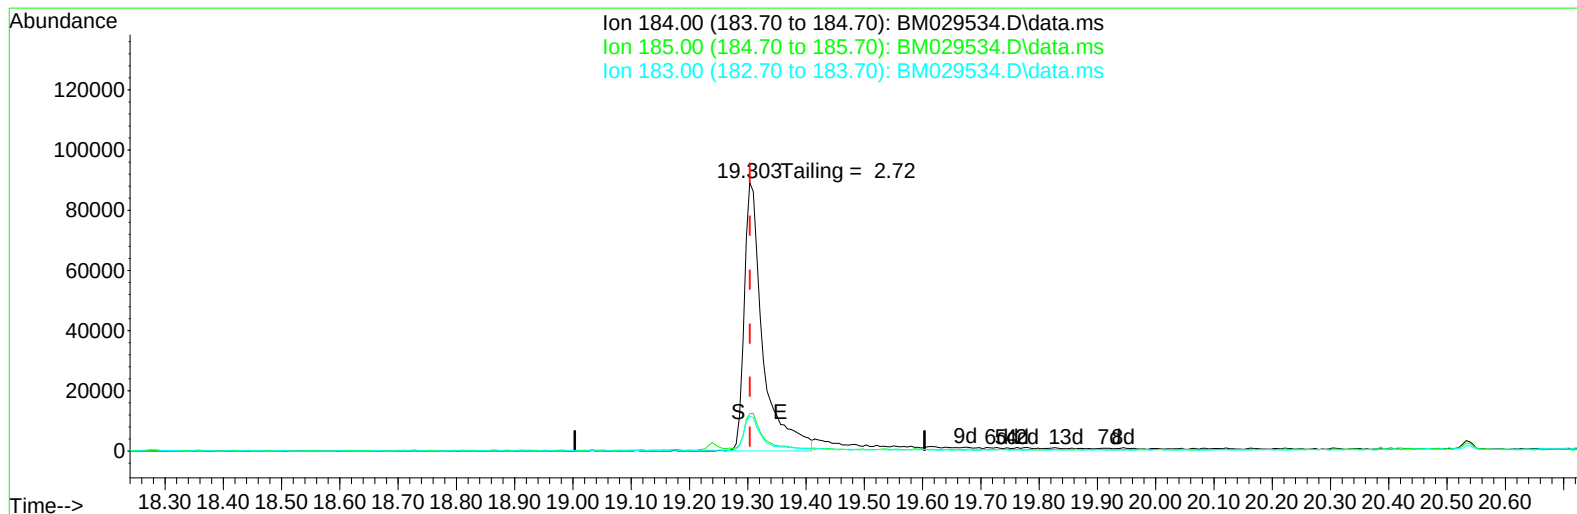

TIC: BM029534.D\data.ms

(77) Benzidine

19.303min (-0.000) 13531.06 ng m




response 230401

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.91
183.00	12.20	13.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041921\
Data File : BM029534.D
Acq On : 19 Apr 2021 10:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 19 11:37:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 11:56:50 2021
Response via : Initial Calibration

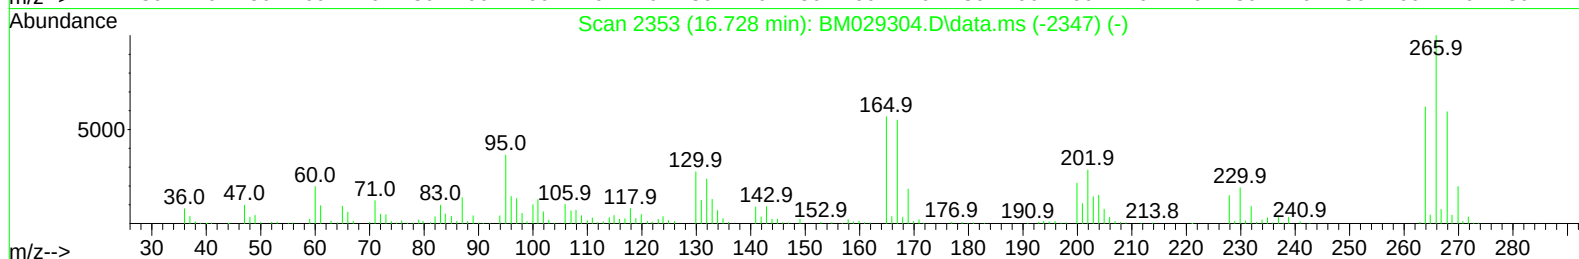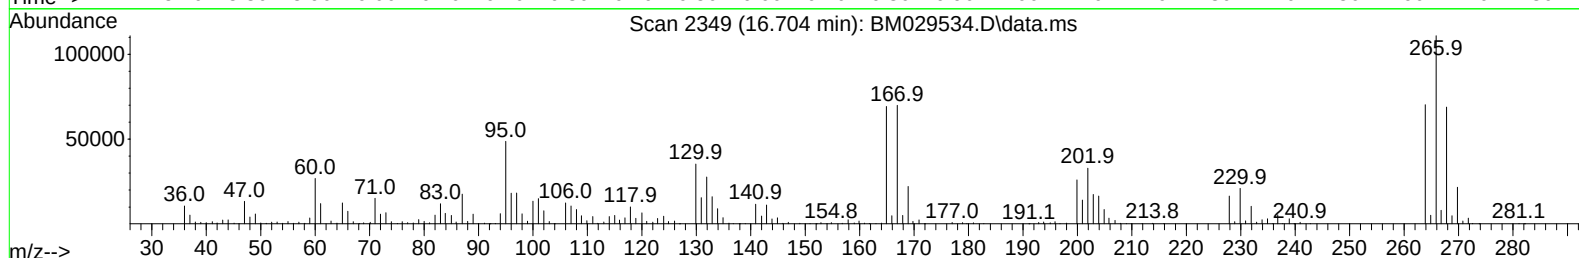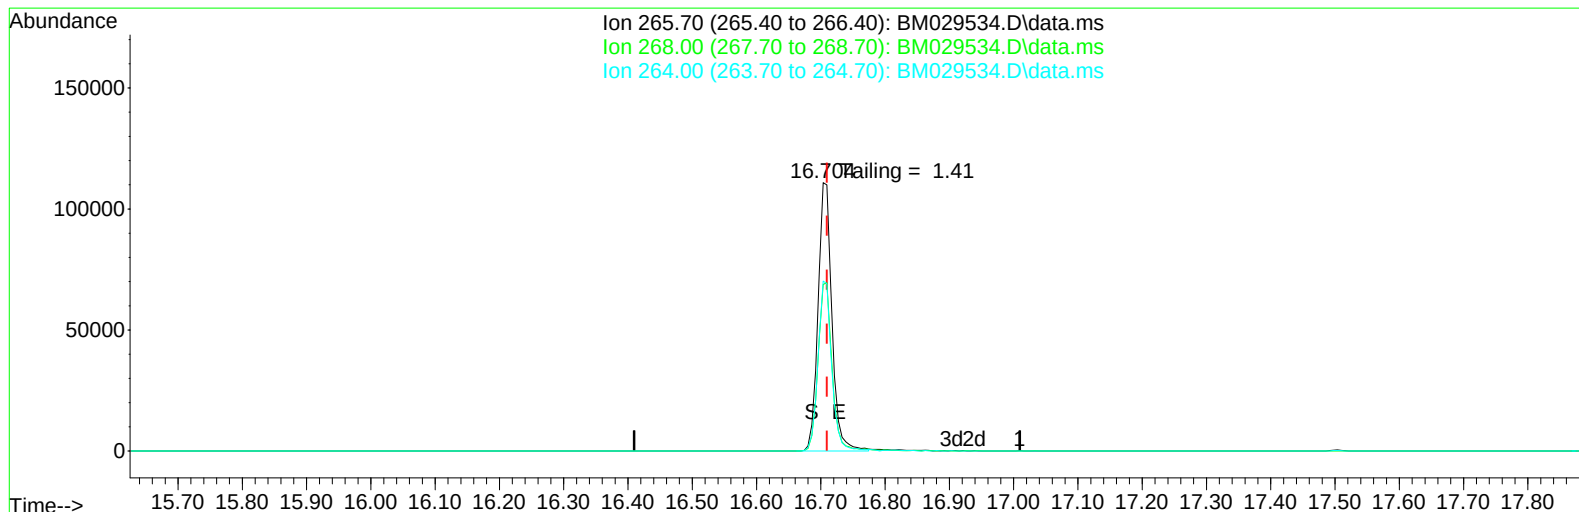

TIC: BM029534.D\data.ms

(70) Pentachlorophenol (C)

16.704min (-0.006) 22473.17 ng m

response 169192

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	62.07
264.00	63.60	63.33
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/19/2021	BNA_M	<u>BM029534.D</u>
Compound Name	Response	Retention Time
DDT	532986	20.53
DDD	10240	20.22
DDE	819	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11059	544045	2.03

Instrument :
BNA_M
ClientSampleId :
DFTPP