

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042015\
 Data File : BM001069.D
 Acq On : 20 Apr 2015 17:14
 Operator : TP/IZ
 Sample : PB82819BL
 Misc : SBLK52
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Apr 21 03:30:32 2015
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM01.2-EPA-BM041515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 21 03:16:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	231012	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	925874	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	489367	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	1054155	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	1234941	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	1216359	20.00	ng/ul	0.00


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.92	96	254	0.05	ng/uL	-0.11
5) Phenol-d5	6.75	99	617921	34.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	397767	35.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	515296	35.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	475790	33.46	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	244172	39.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	269480	38.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	452899	33.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	81619	6.16	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	1314146	40.30	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	1623143	34.78	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	255577	40.32	ng/ul	0.00
57) Fluorene-d10	15.23	176	1165432	35.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	214124	37.41	ng/ul	0.00
70) Anthracene-d10	17.08	188	1735472	36.36	ng/ul	0.00
76) Pyrene-d10	19.39	212	1946211	33.95	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.22	264	1869117	34.33	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.66	165	7067	1.04	ng/ul#	41

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042015\
Data File : BM001069.D
Acq On : 20 Apr 2015 17:14
Operator : TP/IZ
Sample : PB82819BL
Misc : SBLK52
ALS Vial : 4 Sample Multiplier: 1


Quant Time: Apr 21 03:30:32 2015
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM01.2-EPA-BM041515.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 21 03:16:42 2015
Response via : Initial Calibration

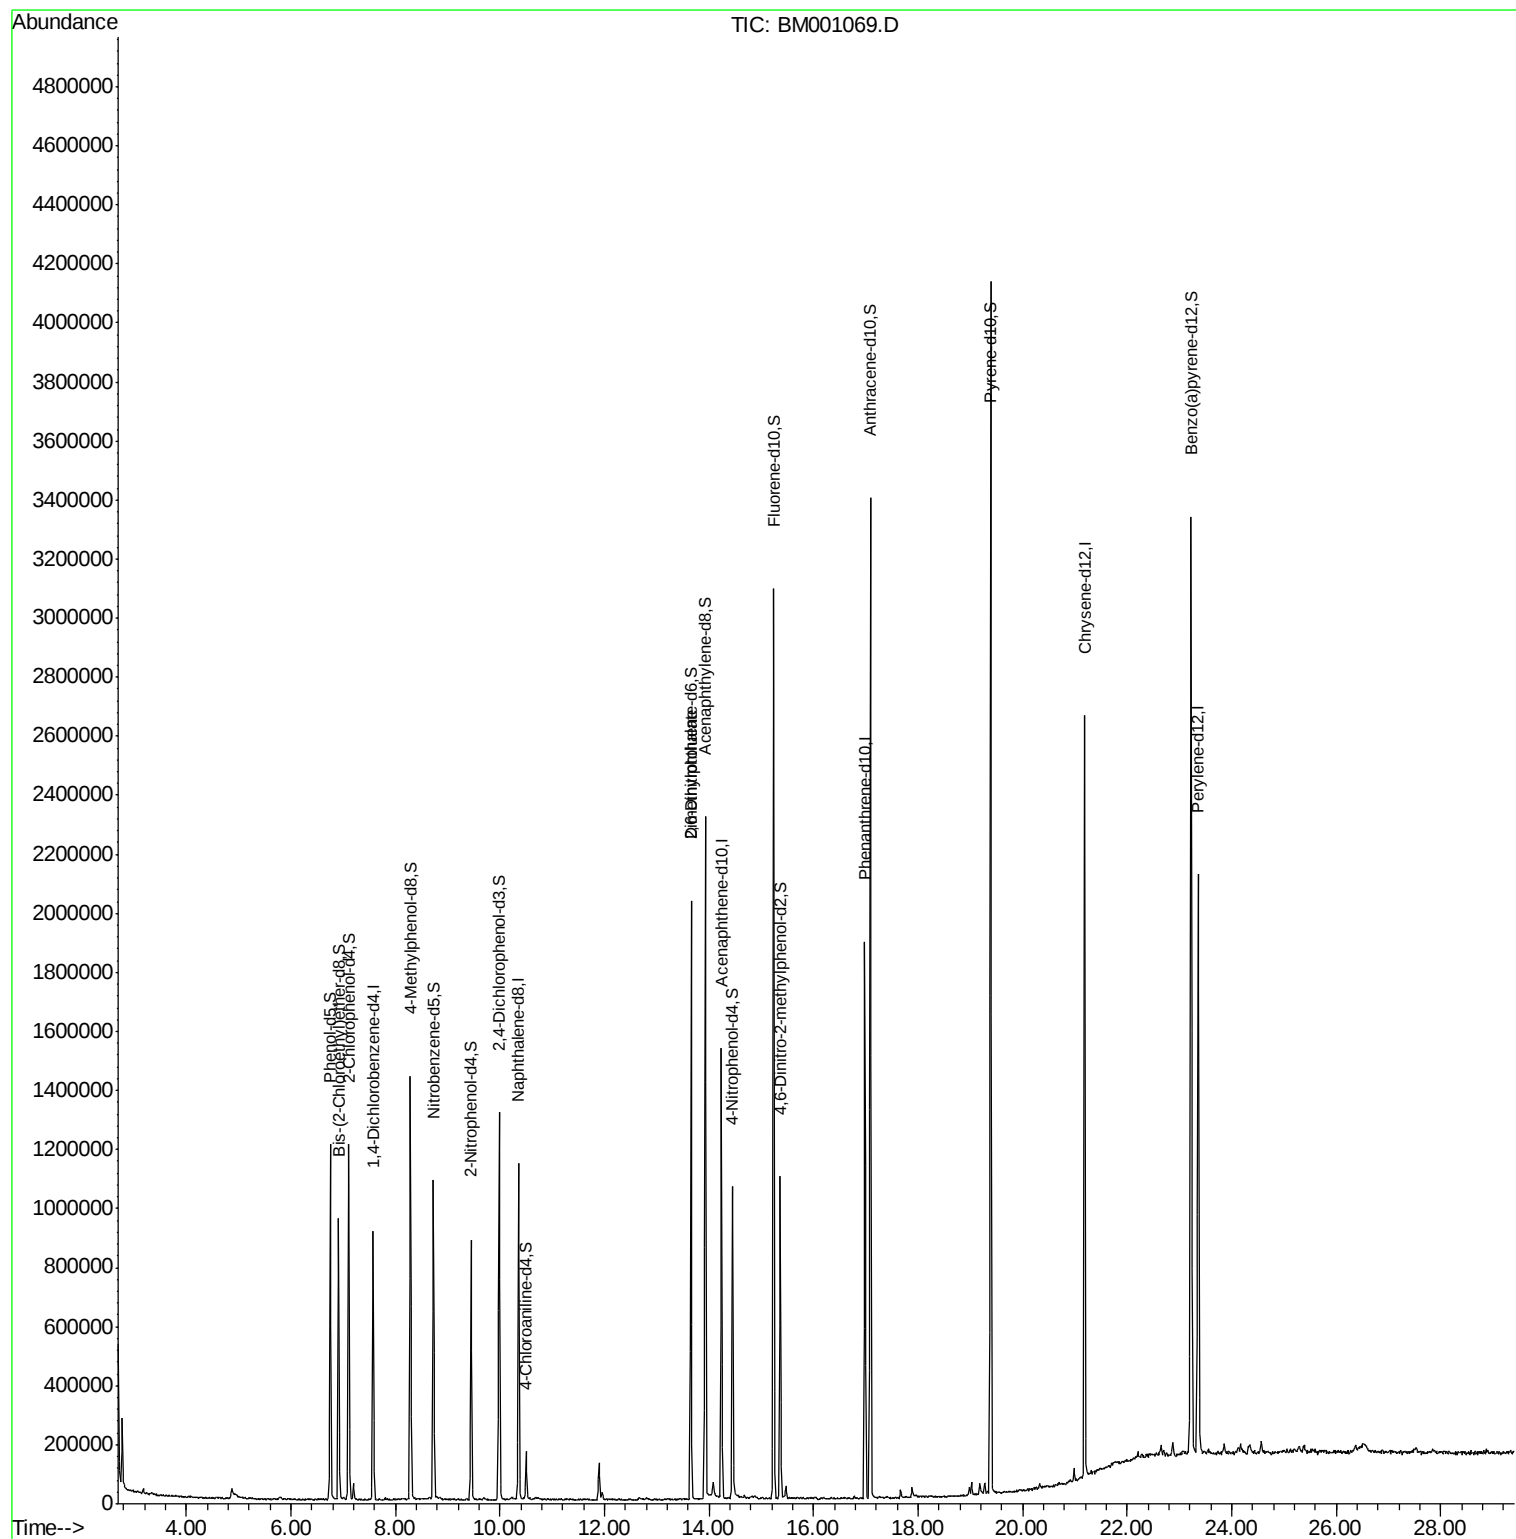

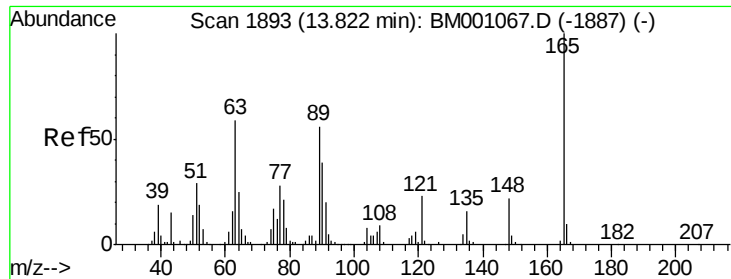

#45
 2,6-Dinitrotoluene
 Concen: 1.04 ng/ul
 RT: 13.66 min Scan# 1865
 Delta R.T. -0.16 min
 Lab File: BM001069.D
 Acq: 20 Apr 2015 17:14

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	47.4	71.2#
121	24.6	17.8	26.6

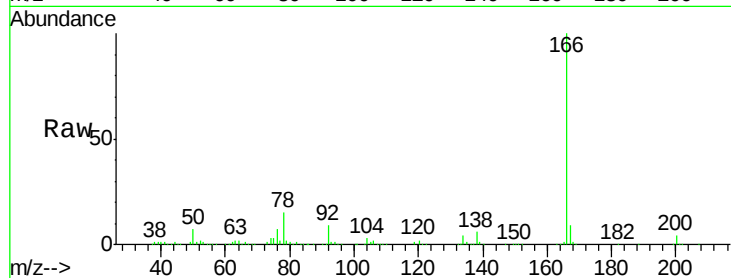

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

