

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042015\
 Data File : BM001085.D
 Acq On : 21 Apr 2015 03:24
 Operator : TP/IZ
 Sample : G1859-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Apr 21 04:55:18 2015
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM01.2-EPA-BM041515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 21 04:18:14 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	206396	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	881041	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	488783	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	1021013	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	1081367	20.00	ng/ul	0.01
83) Perylene-d12	23.39	264	1075752	20.00	ng/ul	0.04


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.05	96	128	0.03	ng/uL	0.02
5) Phenol-d5	6.75	99	420207	26.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	275960	27.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	354696	27.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	320544	25.23	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	165744	27.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	179446	27.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	321936	24.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	283411	22.49	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	933849	28.67	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	1162641	24.94	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	128043	20.22	ng/ul	0.00
57) Fluorene-d10	15.23	176	793121	24.50	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	30579	5.52	ng/ul	0.00
70) Anthracene-d10	17.08	188	1152174	24.93	ng/ul	0.00
76) Pyrene-d10	19.39	212	1238544	24.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	1079689	22.42	ng/ul	0.04


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.69	163	132768	3.64	ng/ul	99
77) Pyrene	19.42	202	77442	1.13	ng/ul#	84
81) Bis(2-ethylhexyl)phthalate	21.12	149	2455434	65.06	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042015\
 Data File : BM001085.D
 Acq On : 21 Apr 2015 03:24
 Operator : TP/IZ
 Sample : G1859-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1





Quant Time: Apr 21 04:55:18 2015
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM01.2-EPA-BM041515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 21 04:18:14 2015
 Response via : Initial Calibration

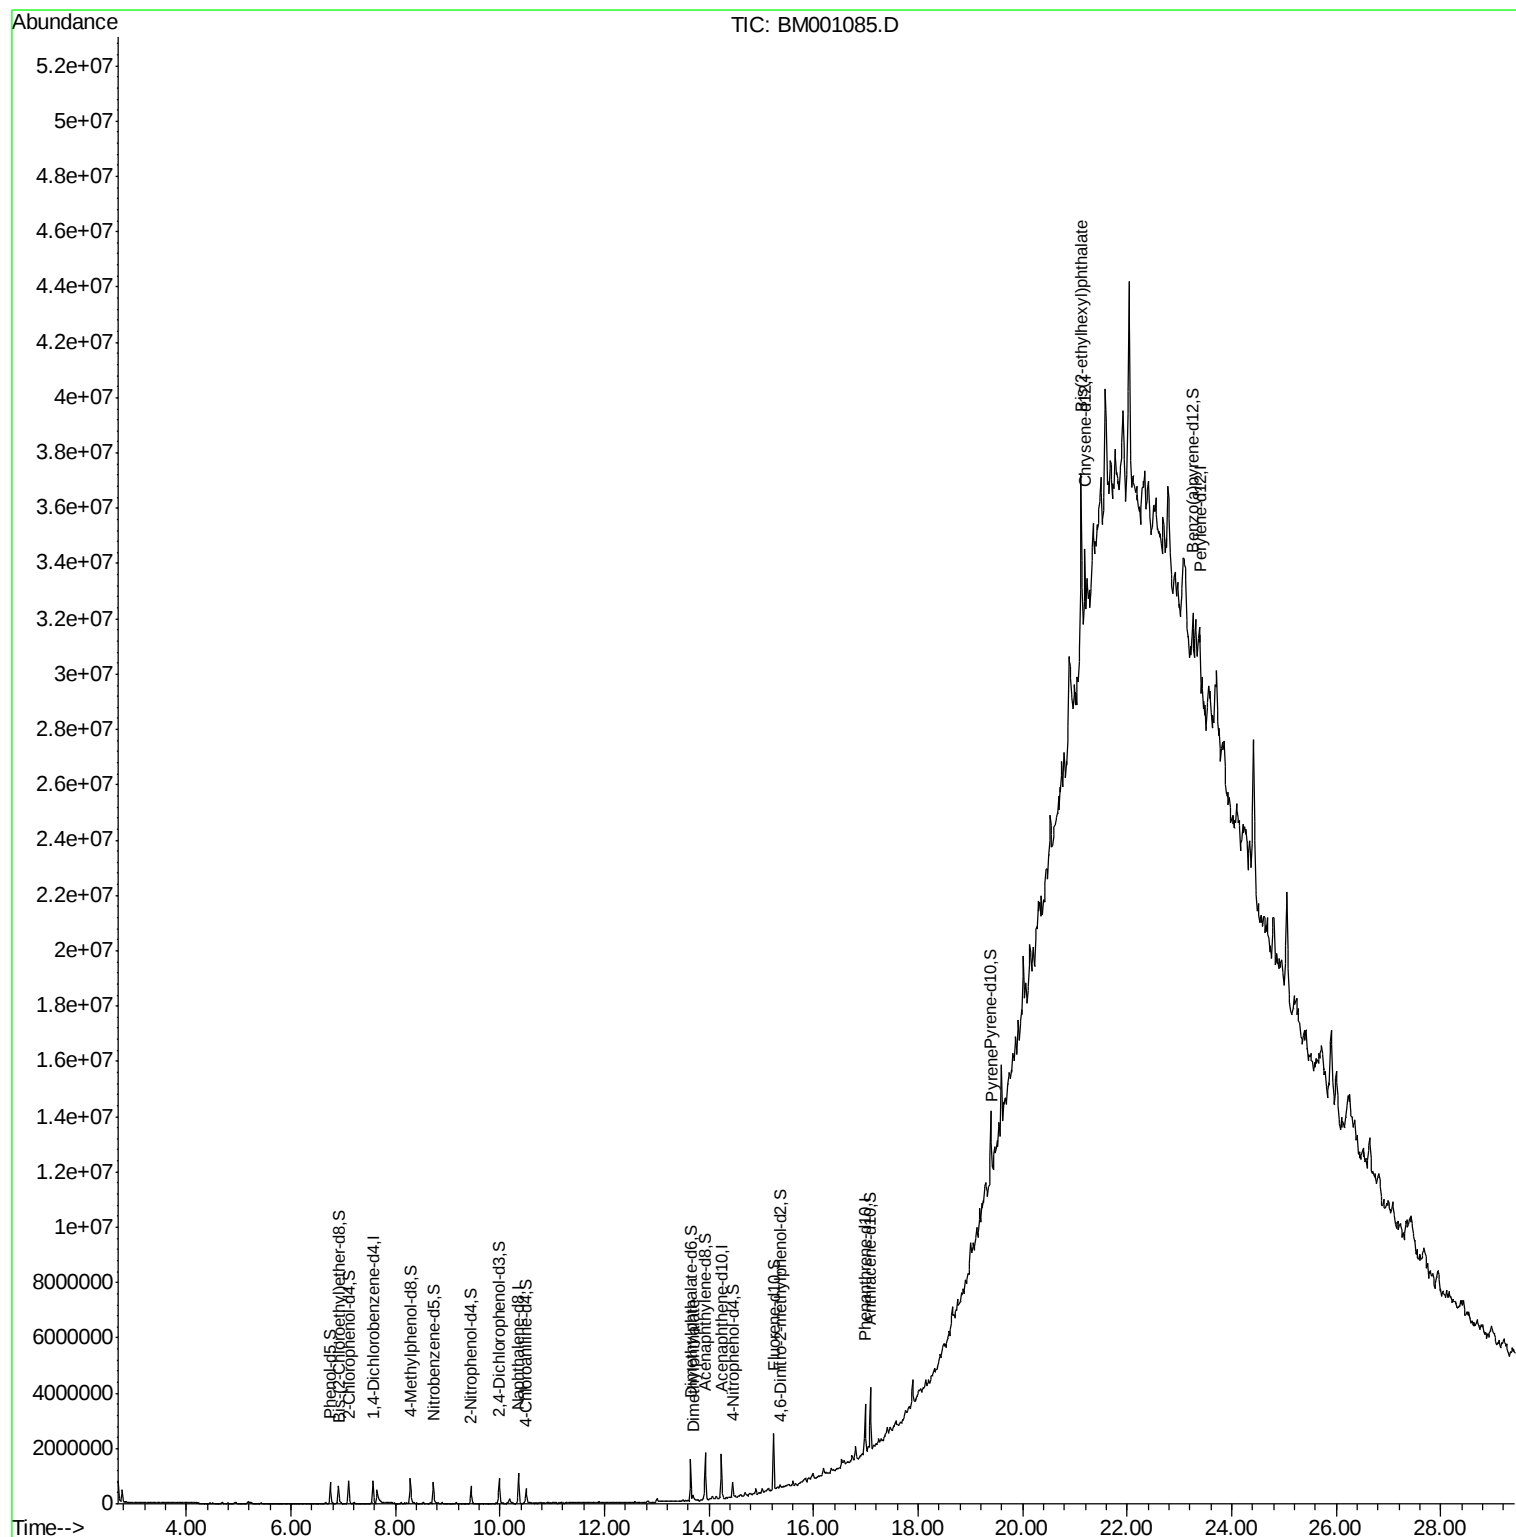

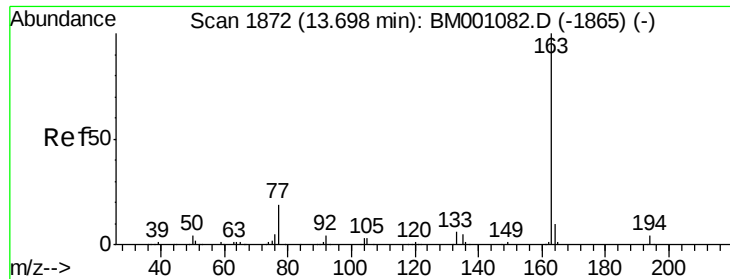




#44
Dimethylphthalate
Concen: 3.64 ng/ul
RT: 13.69 min Scan# 1871
Delta R.T. -0.01 min
Lab File: BM001085.D
Acq: 21 Apr 2015 03:24


Tgt Ion:163 Resp: 132768
Ion Ratio Lower Upper
163 100
194 4.2 3.0 4.4
164 10.1 8.2 12.4

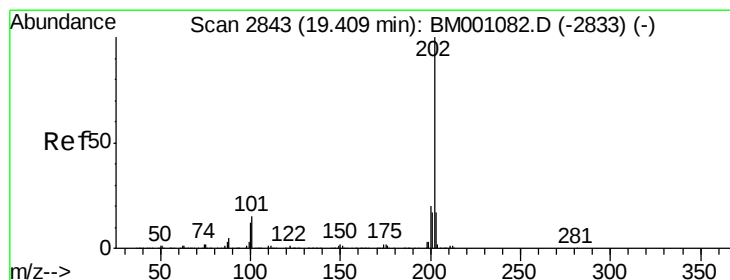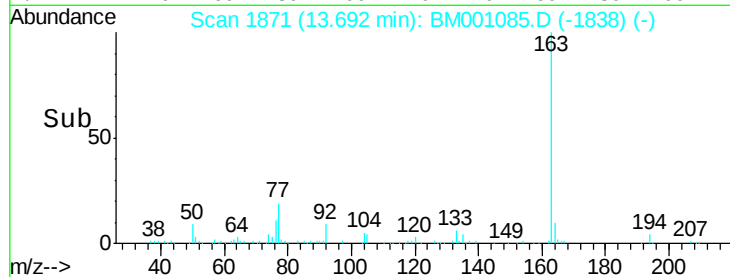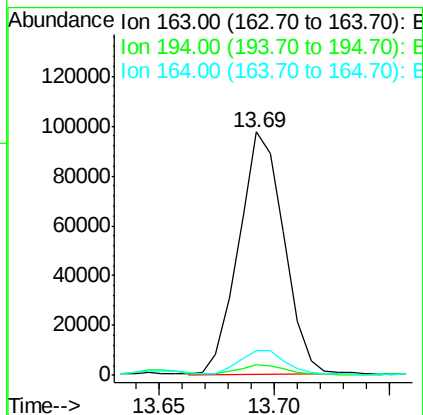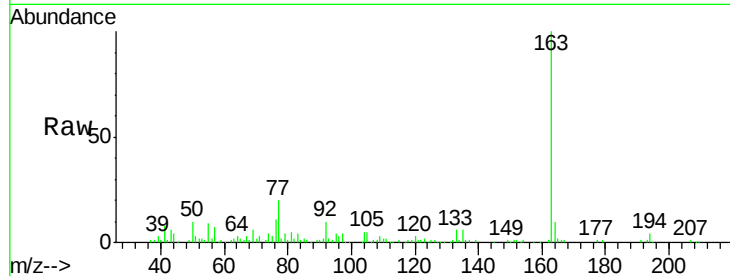

#77
Pyrene
Concen: 1.13 ng/ul
RT: 19.42 min Scan# 2844
Delta R.T. 0.01 min
Lab File: BM001085.D
Acq: 21 Apr 2015 03:24

Tgt Ion:202 Resp: 77442
Ion Ratio Lower Upper
202 100
101 18.4 11.4 17.2#
100 21.1 9.8 14.6#

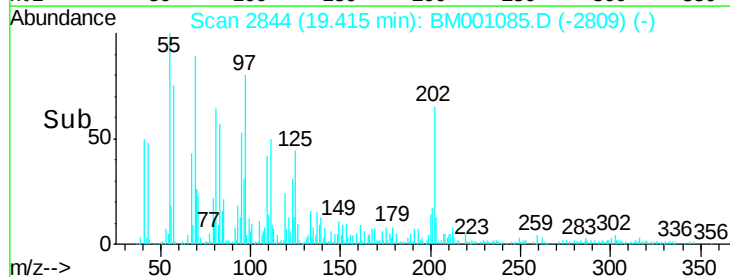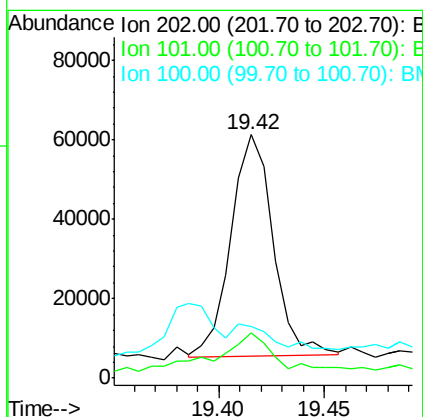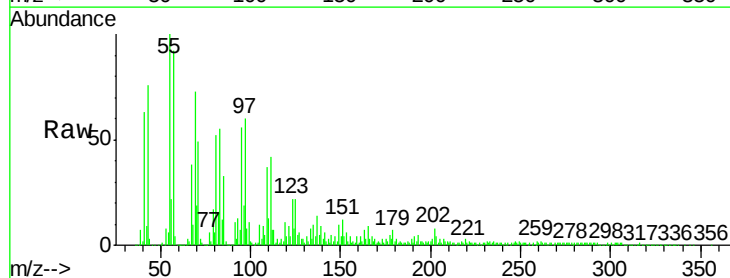

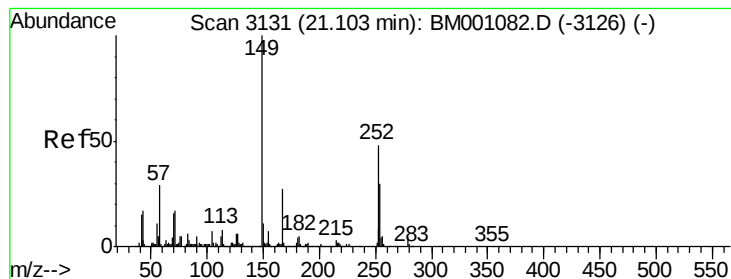

#81

Bis(2-ethylhexyl)phthalate

Concen: 65.06 ng/ul

RT: 21.12 min Scan# 3133

Delta R.T. 0.01 min

Lab File: BM001085.D

Acq: 21 Apr 2015 03:24


Tgt Ion:149 Resp: 2455434

Ion Ratio Lower Upper

149 100

167 30.2 22.3 33.5

279 4.1 3.3 4.9

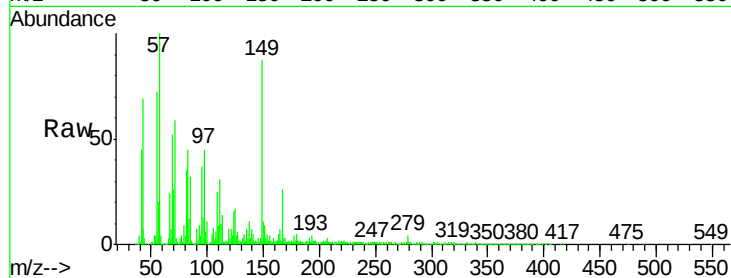

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

