

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042015\
 Data File : BM001086.D
 Acq On : 21 Apr 2015 03:59
 Operator : TP/IZ
 Sample : G1859-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 21 04:59:36 2015
 Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM01.2-EPA-BM041515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 21 04:18:14 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	204571	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	806710	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	420730	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.99	188	857081	20.00	ng/ul	0.00
75) Chrysene-d12	21.18	240	911502	20.00	ng/ul	0.00
83) Perylene-d12	23.35	264	922141	20.00	ng/ul	0.00


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.04	96	364	0.08	ng/uL	0.00
5) Phenol-d5	6.76	99	414558	25.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	263770	26.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	340497	26.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	285334	22.66	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	158242	29.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	168981	27.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	289367	24.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	213085	18.47	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	821836	29.32	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	922985	23.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	130579	23.96	ng/ul	0.00
57) Fluorene-d10	15.23	176	553703	19.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	68342	14.68	ng/ul	0.00
70) Anthracene-d10	17.08	188	756774	19.50	ng/ul	0.00
76) Pyrene-d10	19.39	212	689677	16.30	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.21	264	549907	13.32	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.69	163	115741	3.69	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042015\
Data File : BM001086.D
Acq On : 21 Apr 2015 03:59
Operator : TP/IZ
Sample : G1859-04
Misc :
ALS Vial : 20 Sample Multiplier: 1


Quant Time: Apr 21 04:59:36 2015
Quant Method : Z:\HPCHEM1\BNA_M\Methods\SOM01.2-EPA-BM041515.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 21 04:18:14 2015
Response via : Initial Calibration

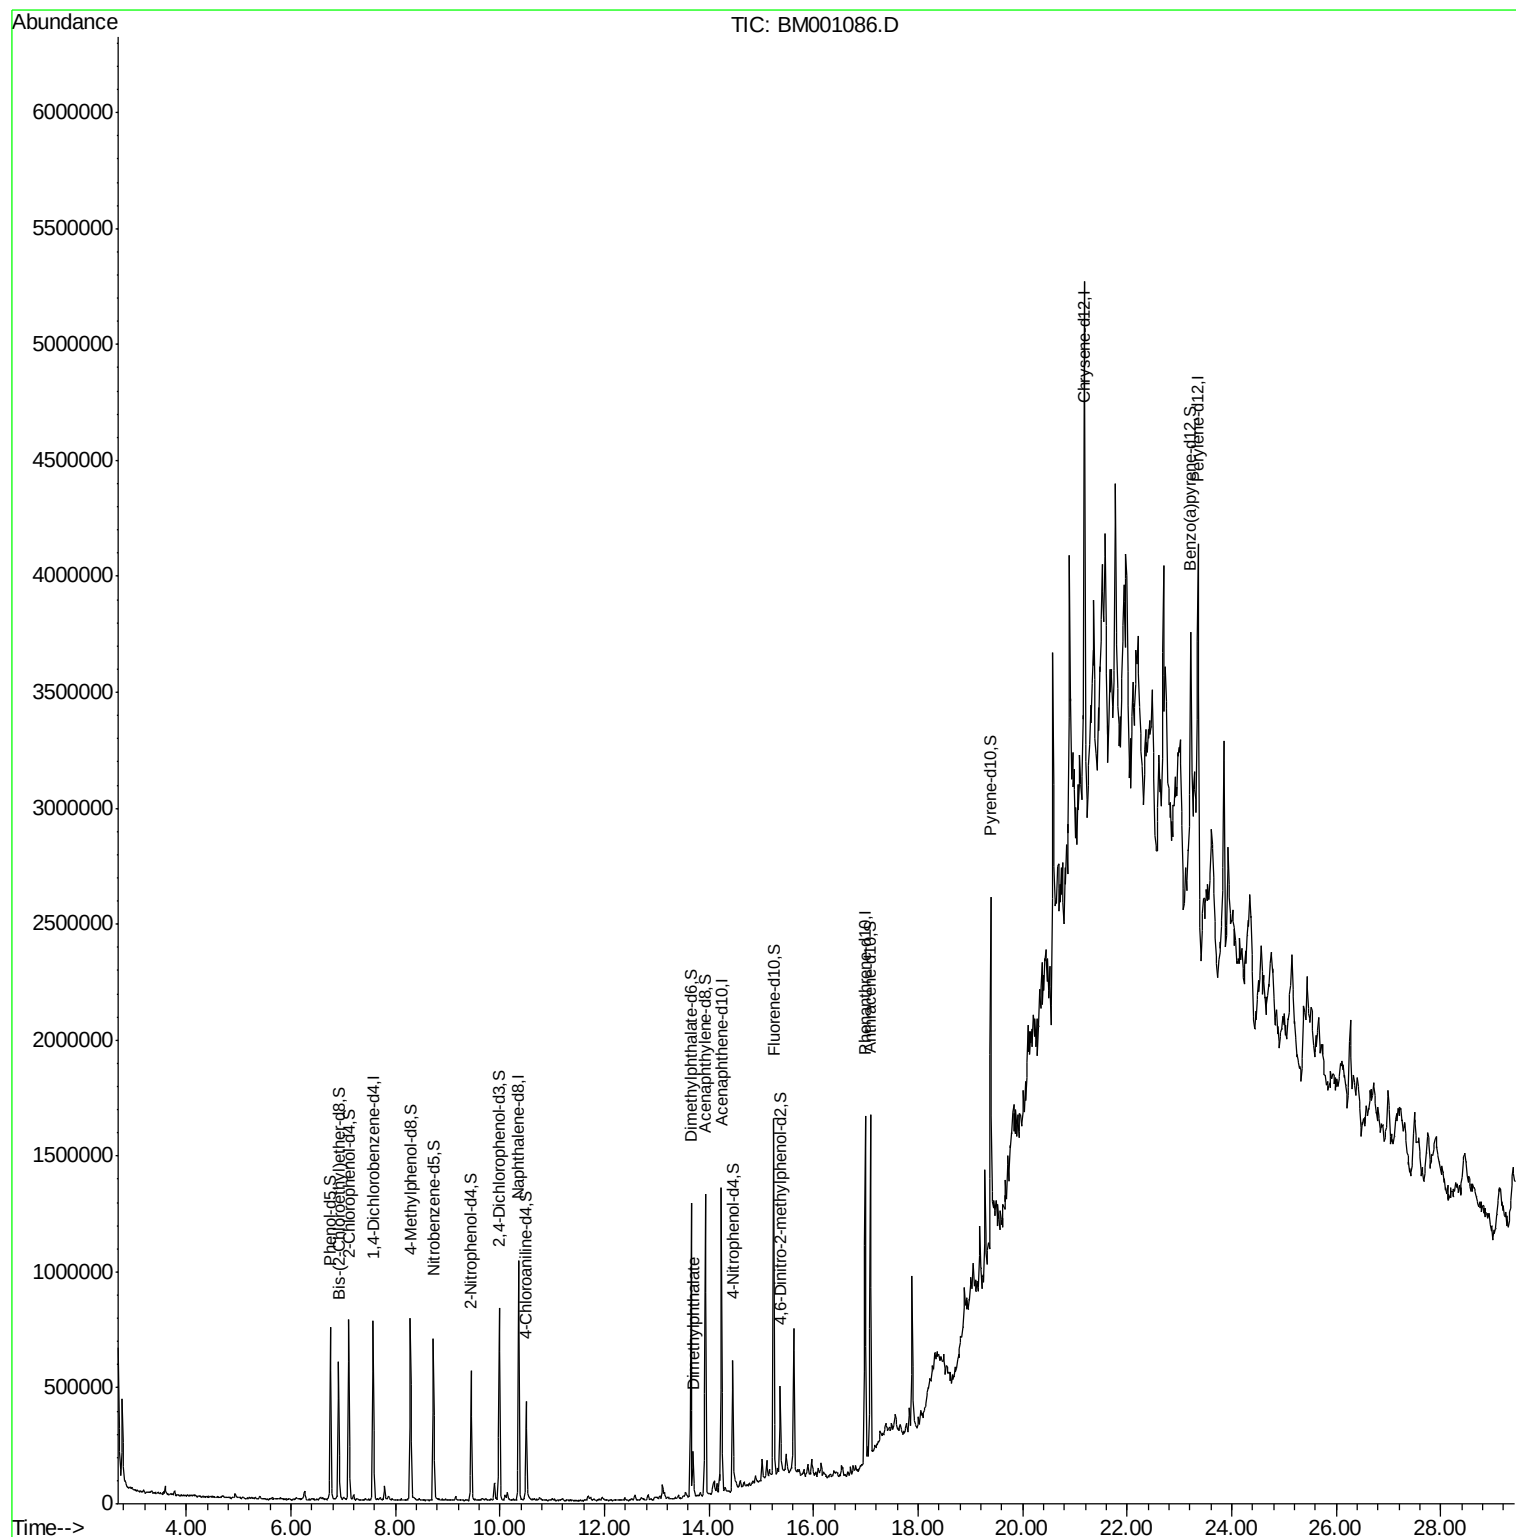

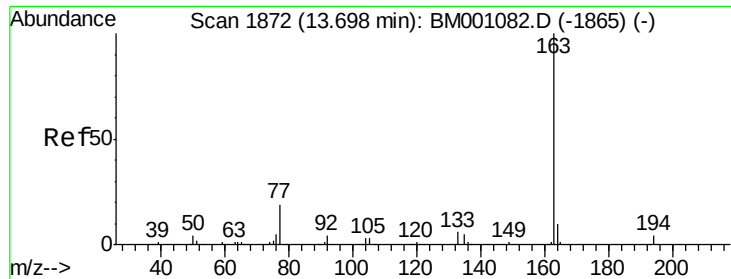

#44
 Dimethylphthalate
 Concen: 3.69 ng/ul
 RT: 13.69 min Scan# 1871
 Delta R.T. -0.01 min
 Lab File: BM001086.D
 Acq: 21 Apr 2015 03:59

Tgt Ion:163	Resp:	115741
Ion Ratio	Lower	Upper
163	100	
194	3.5	3.0 4.4
164	10.4	8.2 12.4

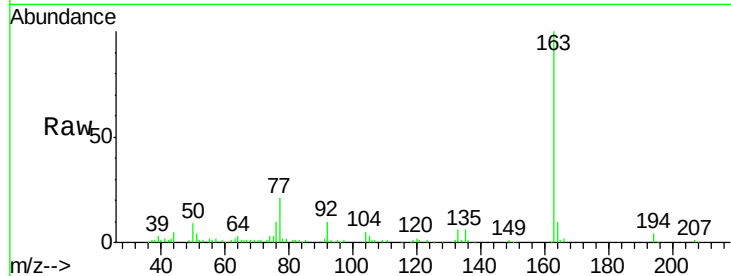

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

