


Data Path : Z:\HPCHEM1\BNA_M\Data\BM042015\
Data File : BM001066.D
Acq On : 20 Apr 2015 15:11
Operator : TP/IZ
Sample : DFTPP50
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\Methods\SOM01.2-EPA-BM041515.M
Title : SVOA CALIBRATION
Last Update : Thu Apr 16 05:47:45 2015

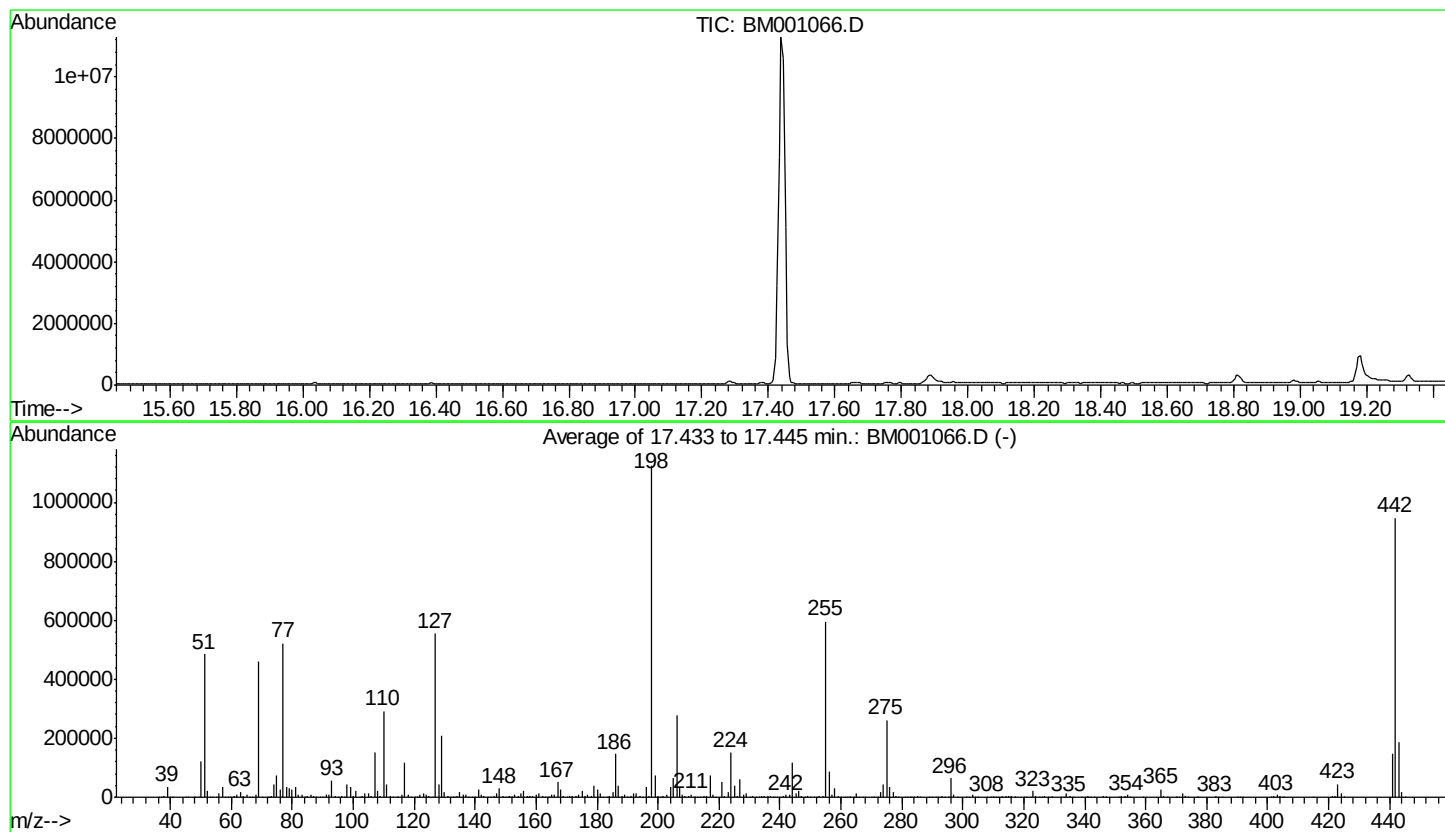

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	485779	PASS
68	69	0.00	2	1.5	6894	PASS
69	198	0.00	100	41.0	461108	PASS
70	69	0.00	2	0.5	2127	PASS
127	198	10	80	49.4	554730	PASS
197	198	0.00	2	0.5	5572	PASS
198	198	100	100	100.0	1123754	PASS
199	198	5	9	6.7	75648	PASS
275	198	10	60	23.3	261290	PASS
365	198	1	100	2.4	26600	PASS
441	443	0.01	100	78.1	145621	PASS
442	198	50	100	84.3	947136	PASS
443	442	15	24	19.7	186490	PASS