

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042015\
 Data File : BM001096.D
 Acq On : 21 Apr 2015 09:58
 Operator : TP/IZ
 Sample : G1859-14
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Apr 21 19:12:46 2015
 Quant Method : Z:\HPCHEM1\BNA M\Methods\SOM01.2-EPA-BM041515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 16 05:47:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	220764	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	870270	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.23	164	462841	20.00	ng/ul	-0.01
61) Phenanthrene-d10	16.99	188	970520	20.00	ng/ul	0.00
75) Chrysene-d12	21.19	240	1041961	20.00	ng/ul	0.00
83) Perylene-d12	23.36	264	1040738	20.00	ng/ul	-0.01


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	297	0.06	ng/uL	0.11
5) Phenol-d5	6.76	99	430691	25.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	266252	24.81	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	358345	25.59	ng/ul	-0.01
13) 4-Methylphenol-d8	8.29	113	307908	22.66	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	164409	28.02	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.45	143	176432	26.93	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.99	165	302403	23.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	395799	31.79	ng/ul	-0.01
43) Dimethylphthalate-d6	13.65	166	864255	28.02	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	1033718	23.42	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.46	143	127183	21.21	ng/ul	0.00
57) Fluorene-d10	15.23	176	653602	21.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	59435	11.28	ng/ul	0.00
70) Anthracene-d10	17.08	188	946914	21.55	ng/ul	-0.01
76) Pyrene-d10	19.39	212	909628	18.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.21	264	734718	15.77	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.70	163	121828	3.53	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042015\
Data File : BM001096.D
Acq On : 21 Apr 2015 09:58
Operator : TP/IZ
Sample : G1859-14
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Apr 21 19:12:46 2015
Quant Method : Z:\HPCHEM1\BNA M\Methods\SOM01.2-EPA-BM041515.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 05:47:45 2015
Response via : Initial Calibration

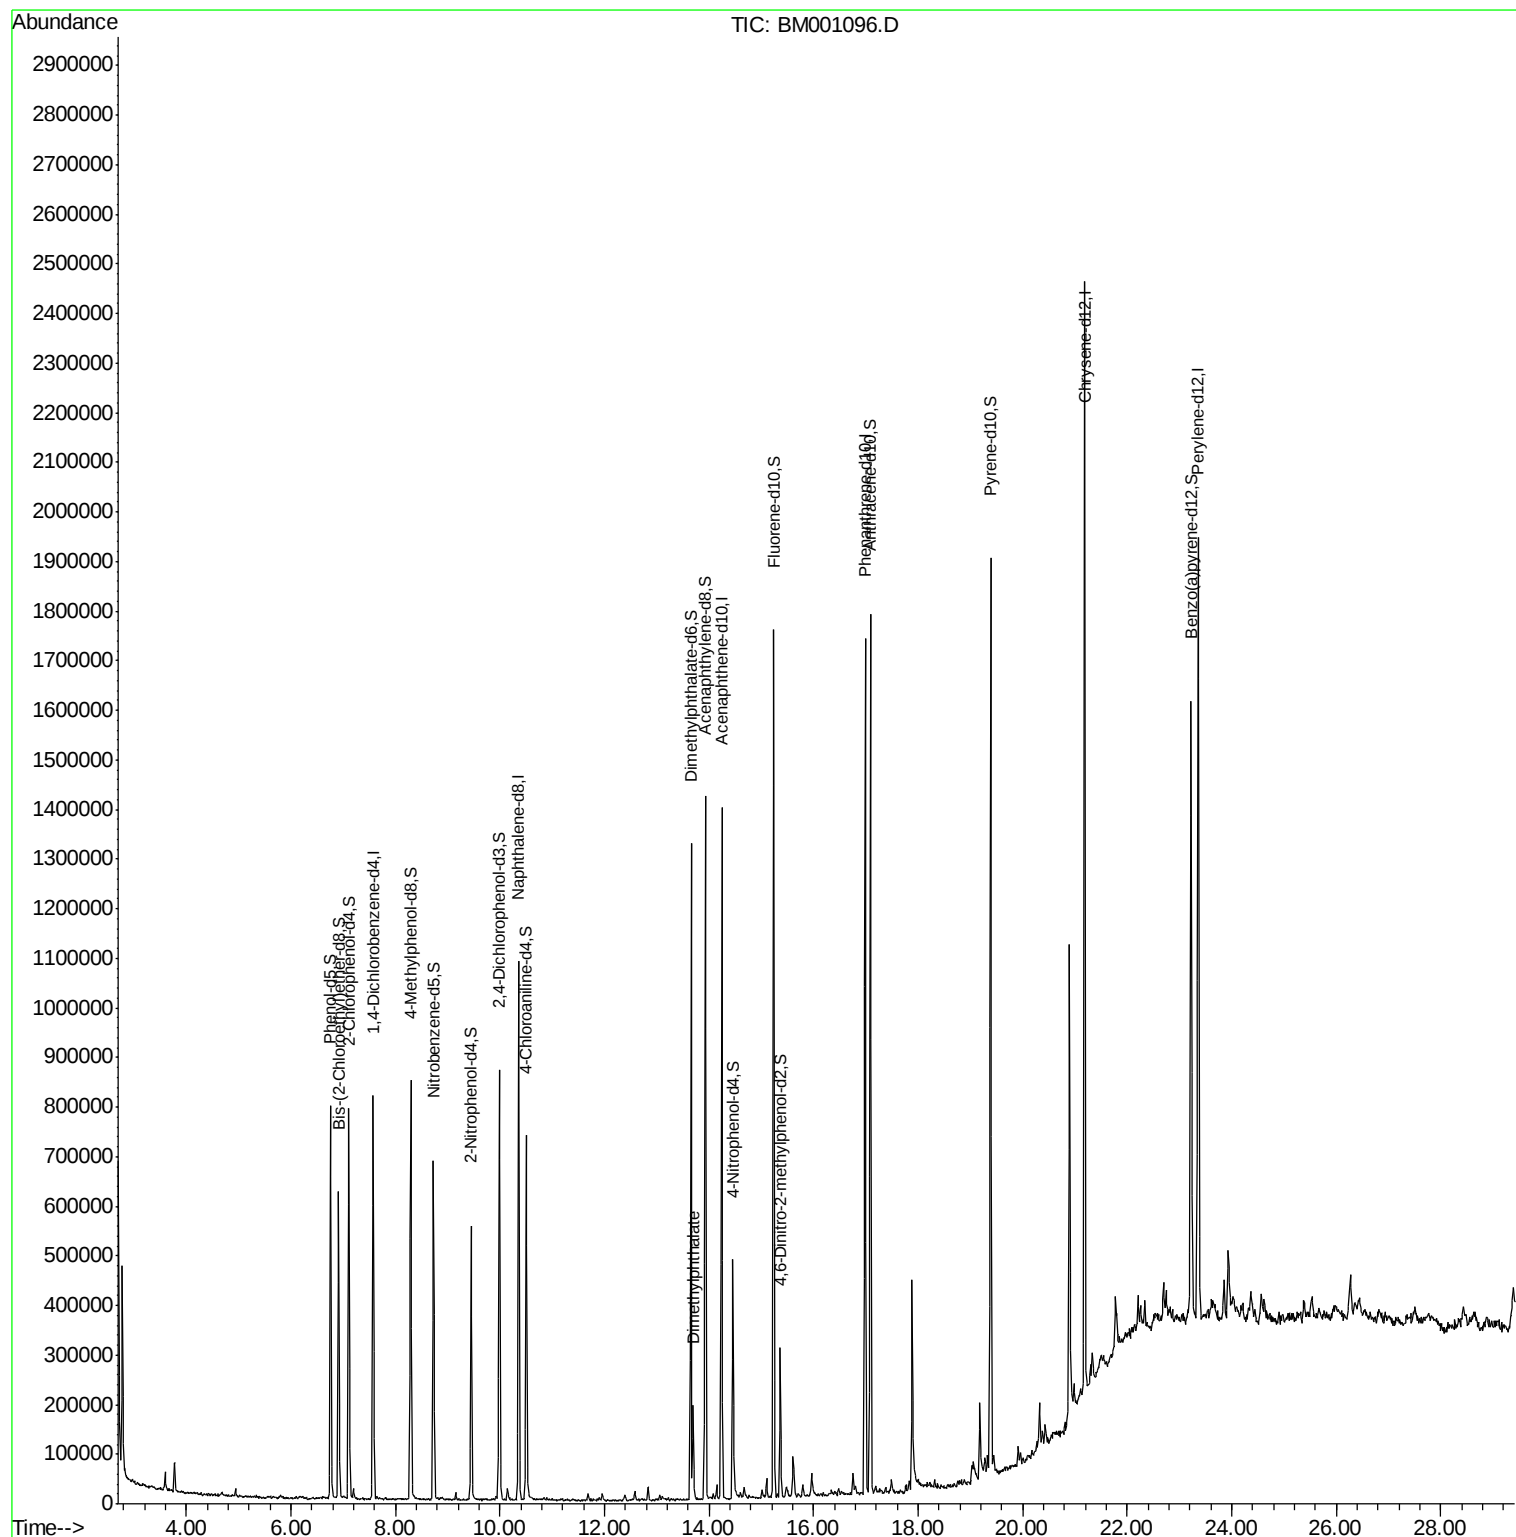

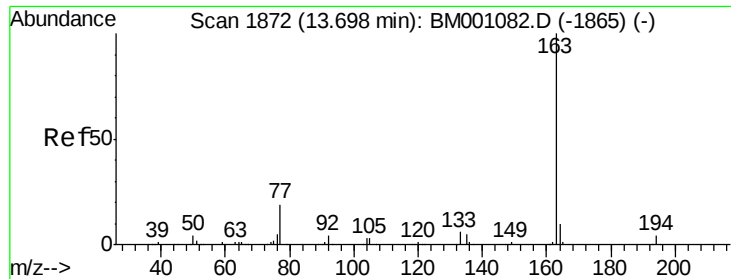

#44
 Dimethylphthalate
 Concen: 3.53 ng/ul
 RT: 13.70 min Scan# 1872
 Delta R.T. -0.01 min
 Lab File: BM001096.D
 Acq: 21 Apr 2015 09:58

Tot Ion:163	Resp: 121828
Ion Ratio	Lower Upper
163 100	
194 4.2	3.0 4.4
164 9.9	8.2 12.4

