

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
 Data File : BM004998.D
 Acq On : 20 Apr 2016 19:39
 Operator : UM/SJ
 Sample : H2621-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H2TR4

Quant Time: Apr 21 10:20:55 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 15 22:59:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	48555	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	209227	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	118195	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	259857	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	297190	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	282421	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	1733	1.91	ng/uL	0.00
5) Phenol-d5	6.98	99	40334	11.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	23735	11.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	33409	11.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	32859	11.48	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	14809	10.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	16087	10.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	31236	11.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.74	131	35925	11.26	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	99761	12.41	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	123553	12.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	9114	6.64	ng/ul	0.00
57) Fluorene-d10	15.44	176	90831	13.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	9670	8.60	ng/ul	0.00
70) Anthracene-d10	17.29	188	137157	13.28	ng/ul	0.00
76) Pyrene-d10	19.59	212	157371	12.71	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	148259	13.63	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.90	163	26817	3.35	ng/ul	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM004998.D
Acq On : 20 Apr 2016 19:39
Operator : UM/SJ
Sample : H2621-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H2TR4

Quant Time: Apr 21 10:20:55 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 15 22:59:24 2016
Response via : Initial Calibration

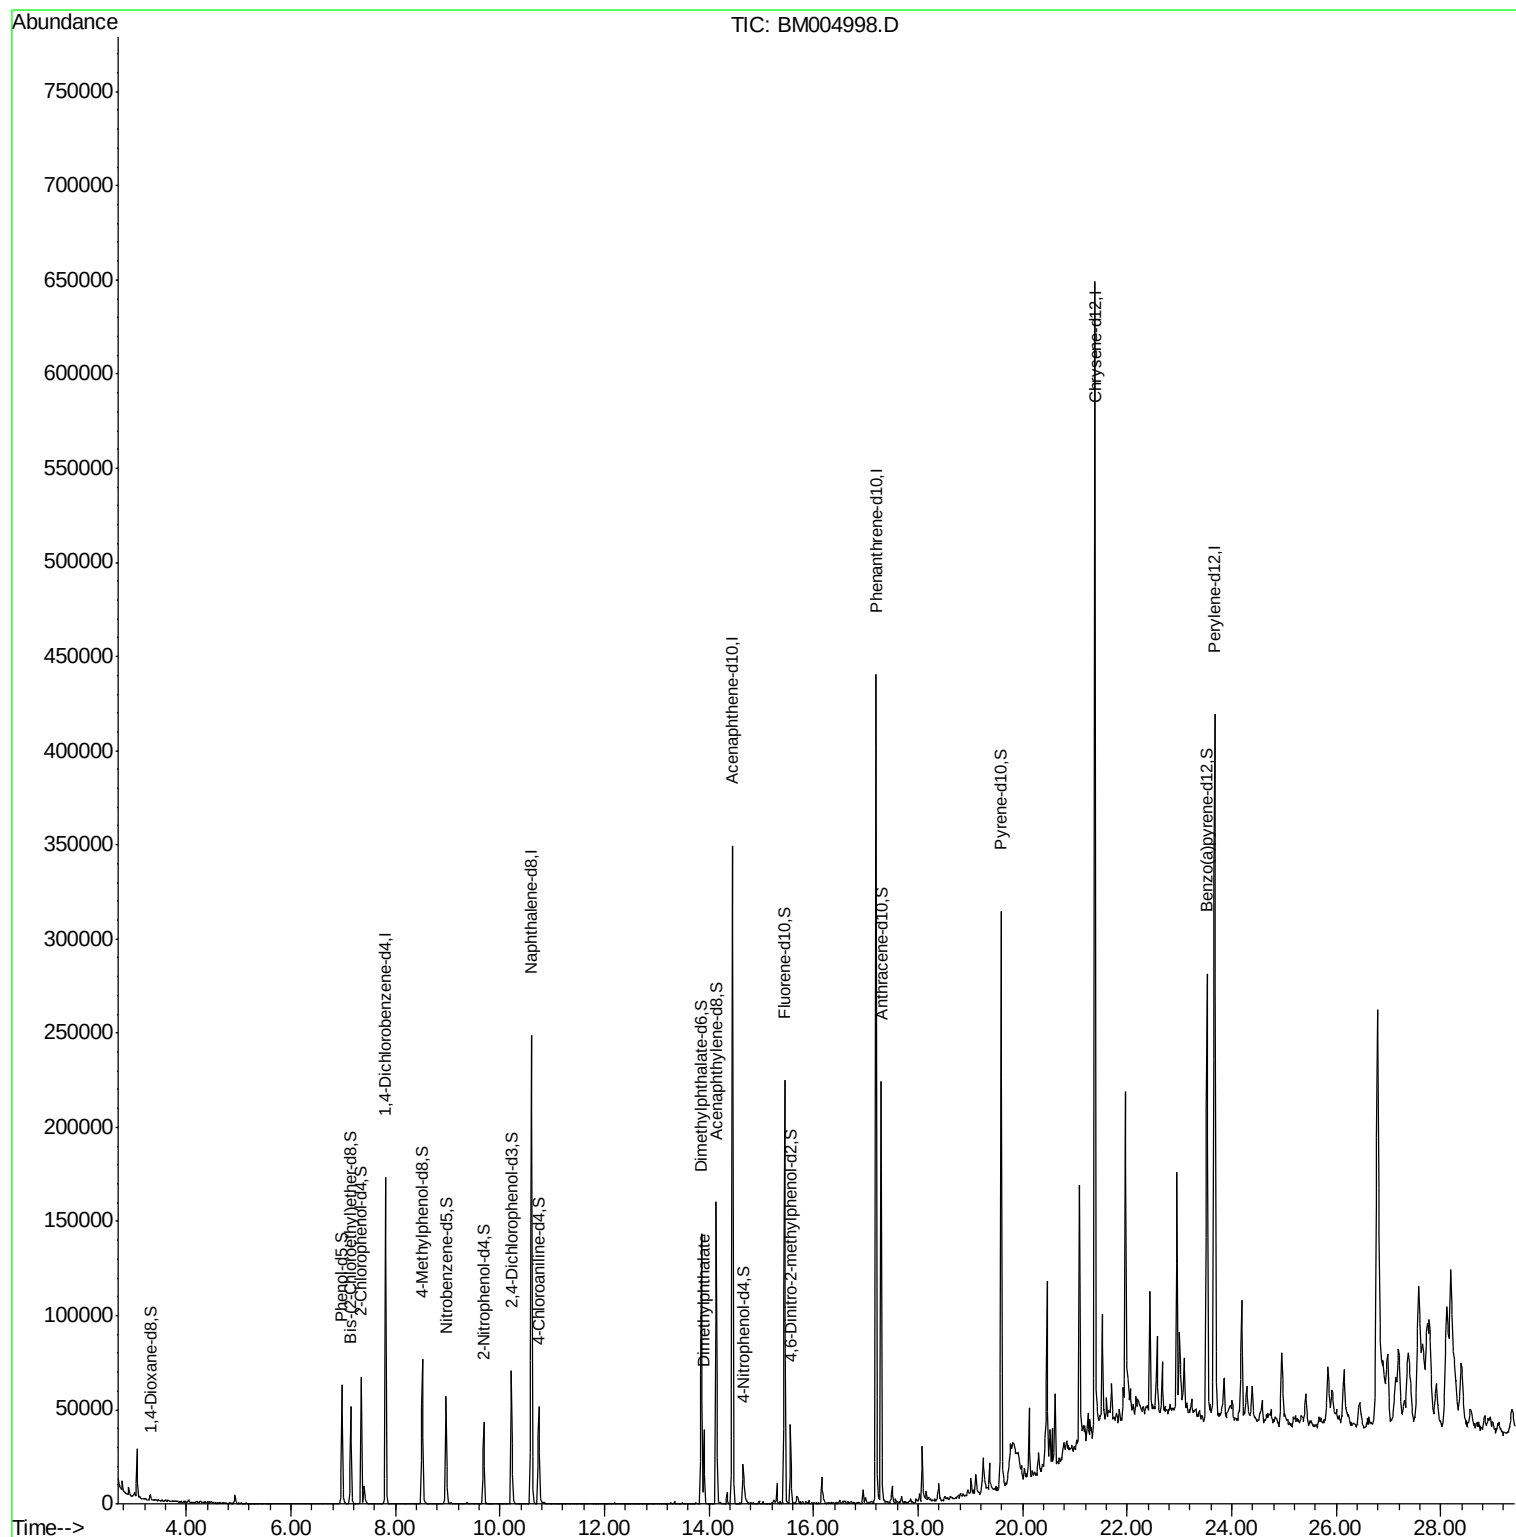

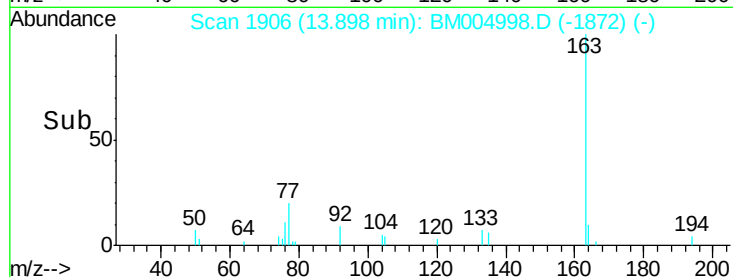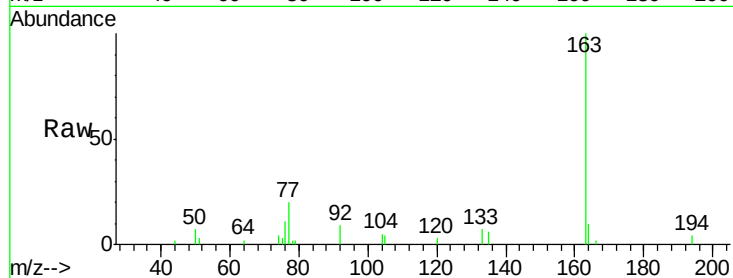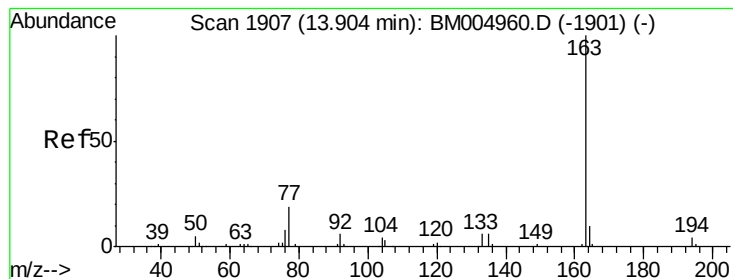

#44

Dimethylphthalate

Concen: 3.35 ng/ul

RT: 13.90 min Scan# 1906

Delta R.T. 0.00 min

Lab File: BM004998.D

Acq: 20 Apr 2016 19:39

Instrument :

BNA_M

ClientSampleId :

H2TR4

Tgt Ion:163 Resp: 26817

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.2 8.2 12.2

