

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
 Data File : BM005005.D
 Acq On : 20 Apr 2016 23:55
 Operator : UM/SJ
 Sample : H2567-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7L0

Quant Time: Apr 21 10:21:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 15 22:59:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	47269	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	201590	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	115848	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	258847	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	303011	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	292170	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	5190	5.88	ng/uL	0.00
5) Phenol-d5	6.97	99	96310	28.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	60178	31.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	80388	28.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	75678	27.15	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	37020	27.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	41248	27.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	74176	27.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	102600	33.37	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	245160	31.11	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	303150	31.37	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	29786	22.15	ng/ul	0.00
57) Fluorene-d10	15.44	176	220347	32.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	29675	26.50	ng/ul	0.00
70) Anthracene-d10	17.29	188	340442	33.10	ng/ul	0.00
76) Pyrene-d10	19.59	212	386982	30.65	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	386720	34.37	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.90	163	73188	9.33	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005005.D
Acq On : 20 Apr 2016 23:55
Operator : UM/SJ
Sample : H2567-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7L0

Quant Time: Apr 21 10:21:36 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 15 22:59:24 2016
Response via : Initial Calibration

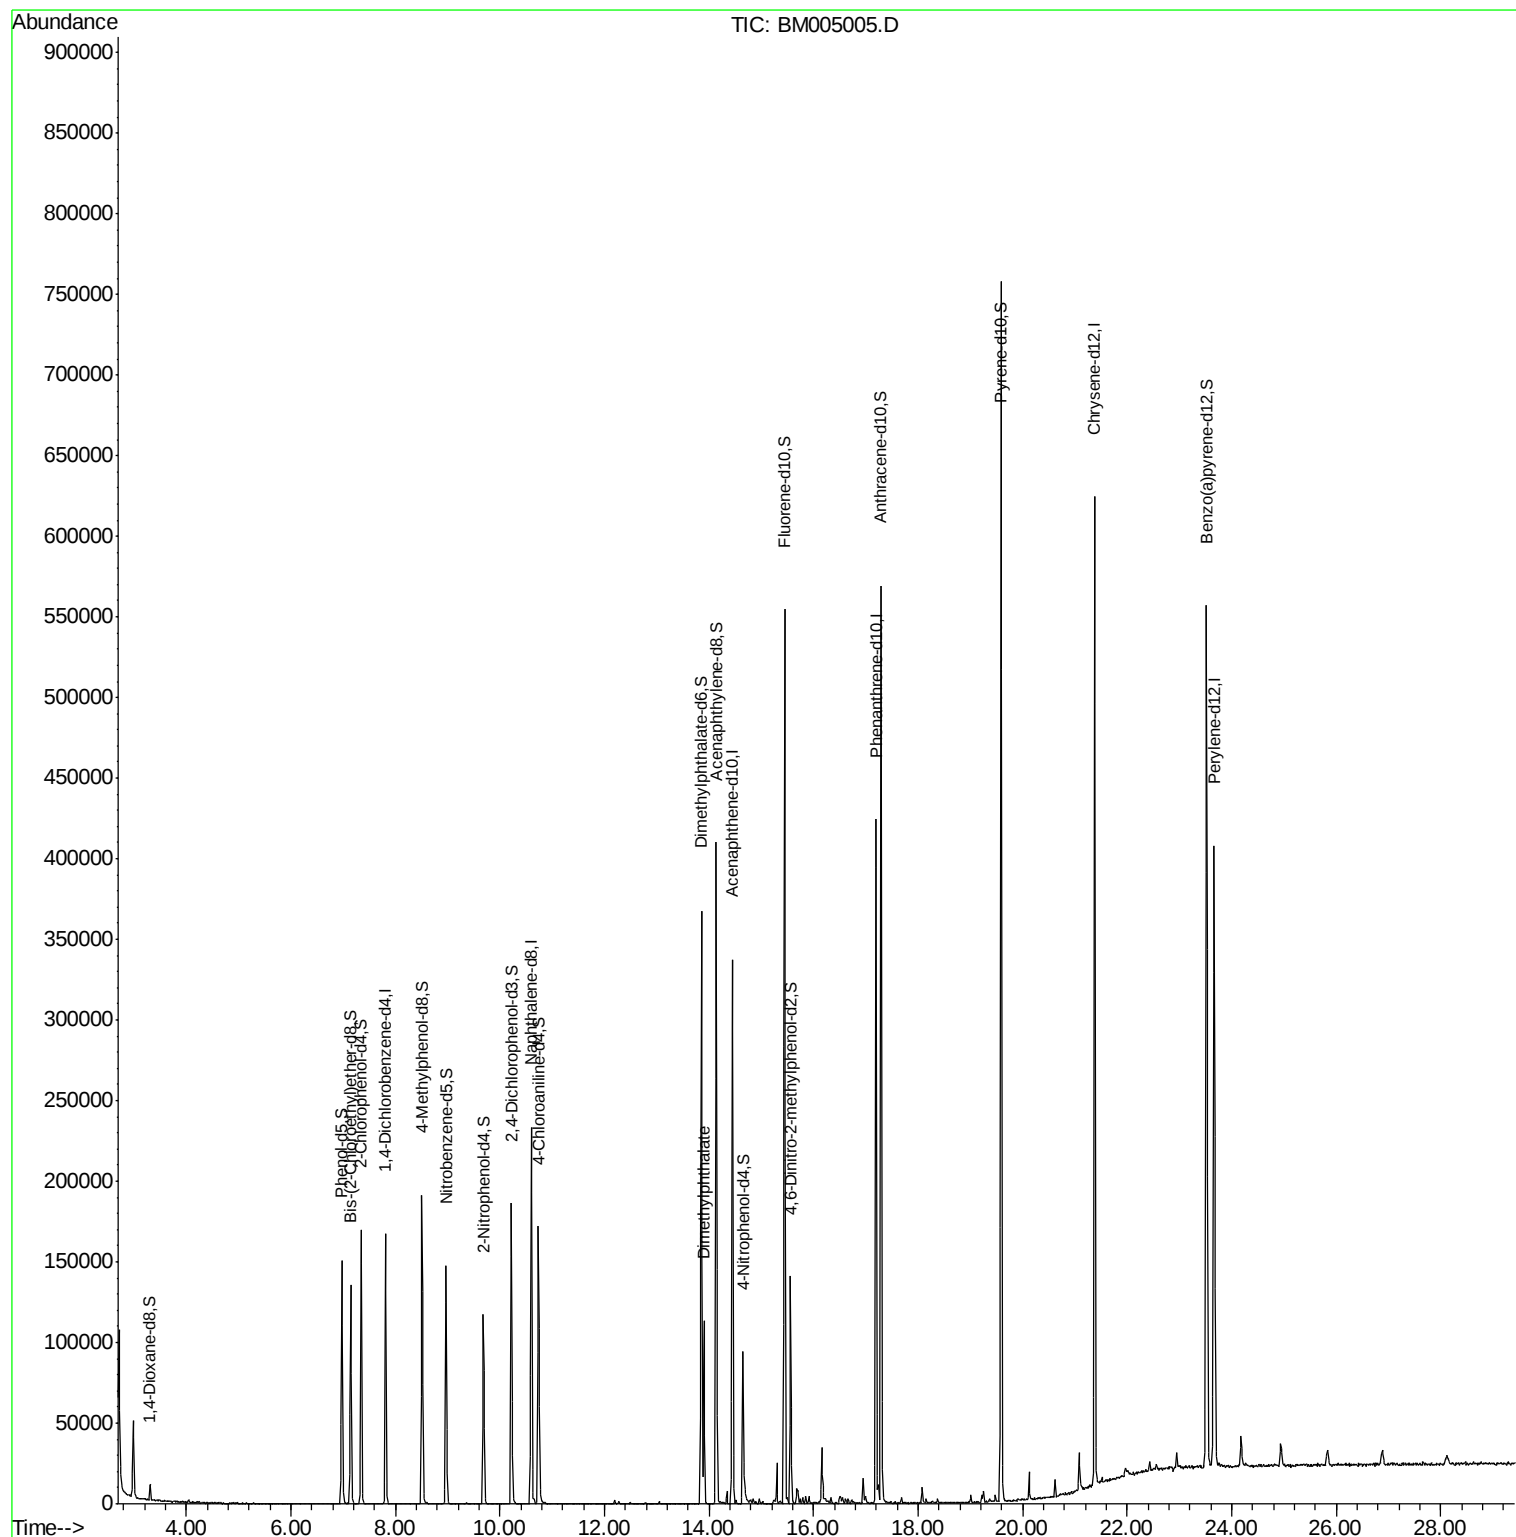

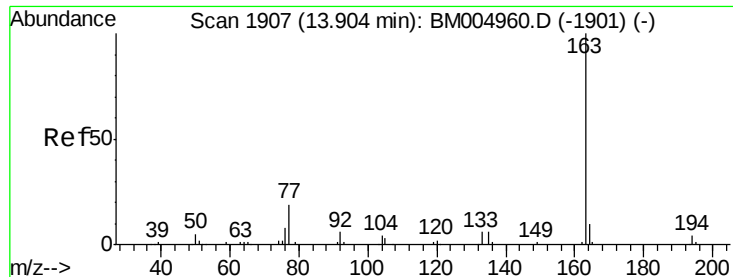

#44

Dimethylphthalate

Concen: 9.33 ng/ul

RT: 13.90 min Scan# 1906

Delta R.T. -0.00 min

Lab File: BM005005.D

Acq: 20 Apr 2016 23:55

Instrument :

BNA_M

ClientSampleId :

BC7L0


Tgt Ion:163 Resp: 73188

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.1 8.2 12.2

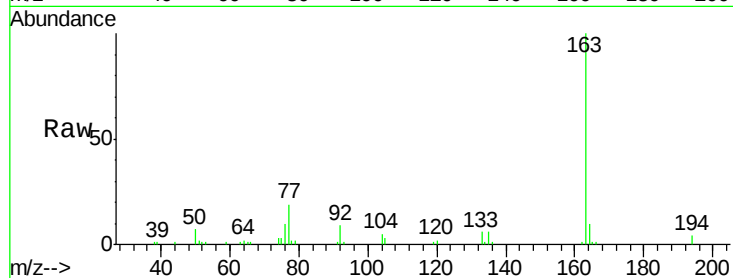

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

