

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
 Data File : BM005009.D
 Acq On : 21 Apr 2016 02:57
 Operator : UM/SJ
 Sample : H2567-23
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7R1

Quant Time: Apr 21 11:10:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 15 22:59:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	52667	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	225508	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	131164	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	293896	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	341082	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	328757	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	1456	1.48	ng/uL	0.00
5) Phenol-d5	6.97	99	31252	8.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	75052	34.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	87666	27.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	59626	19.20	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	52175	34.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	57893	34.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	101306	33.19	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.85	166	342477	38.38	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	411374	37.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	9837	6.46	ng/ul	0.00
57) Fluorene-d10	15.44	176	295417	38.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	50315	39.58	ng/ul	0.00
70) Anthracene-d10	17.29	188	452830	38.78	ng/ul	0.00
76) Pyrene-d10	19.58	212	511562	35.99	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	502525	39.69	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
81) Bis(2-ethylhexyl)phthalate	21.28	149	23290	2.44	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005009.D
Acq On : 21 Apr 2016 02:57
Operator : UM/SJ
Sample : H2567-23
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7R1

Quant Time: Apr 21 11:10:19 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 15 22:59:24 2016
Response via : Initial Calibration

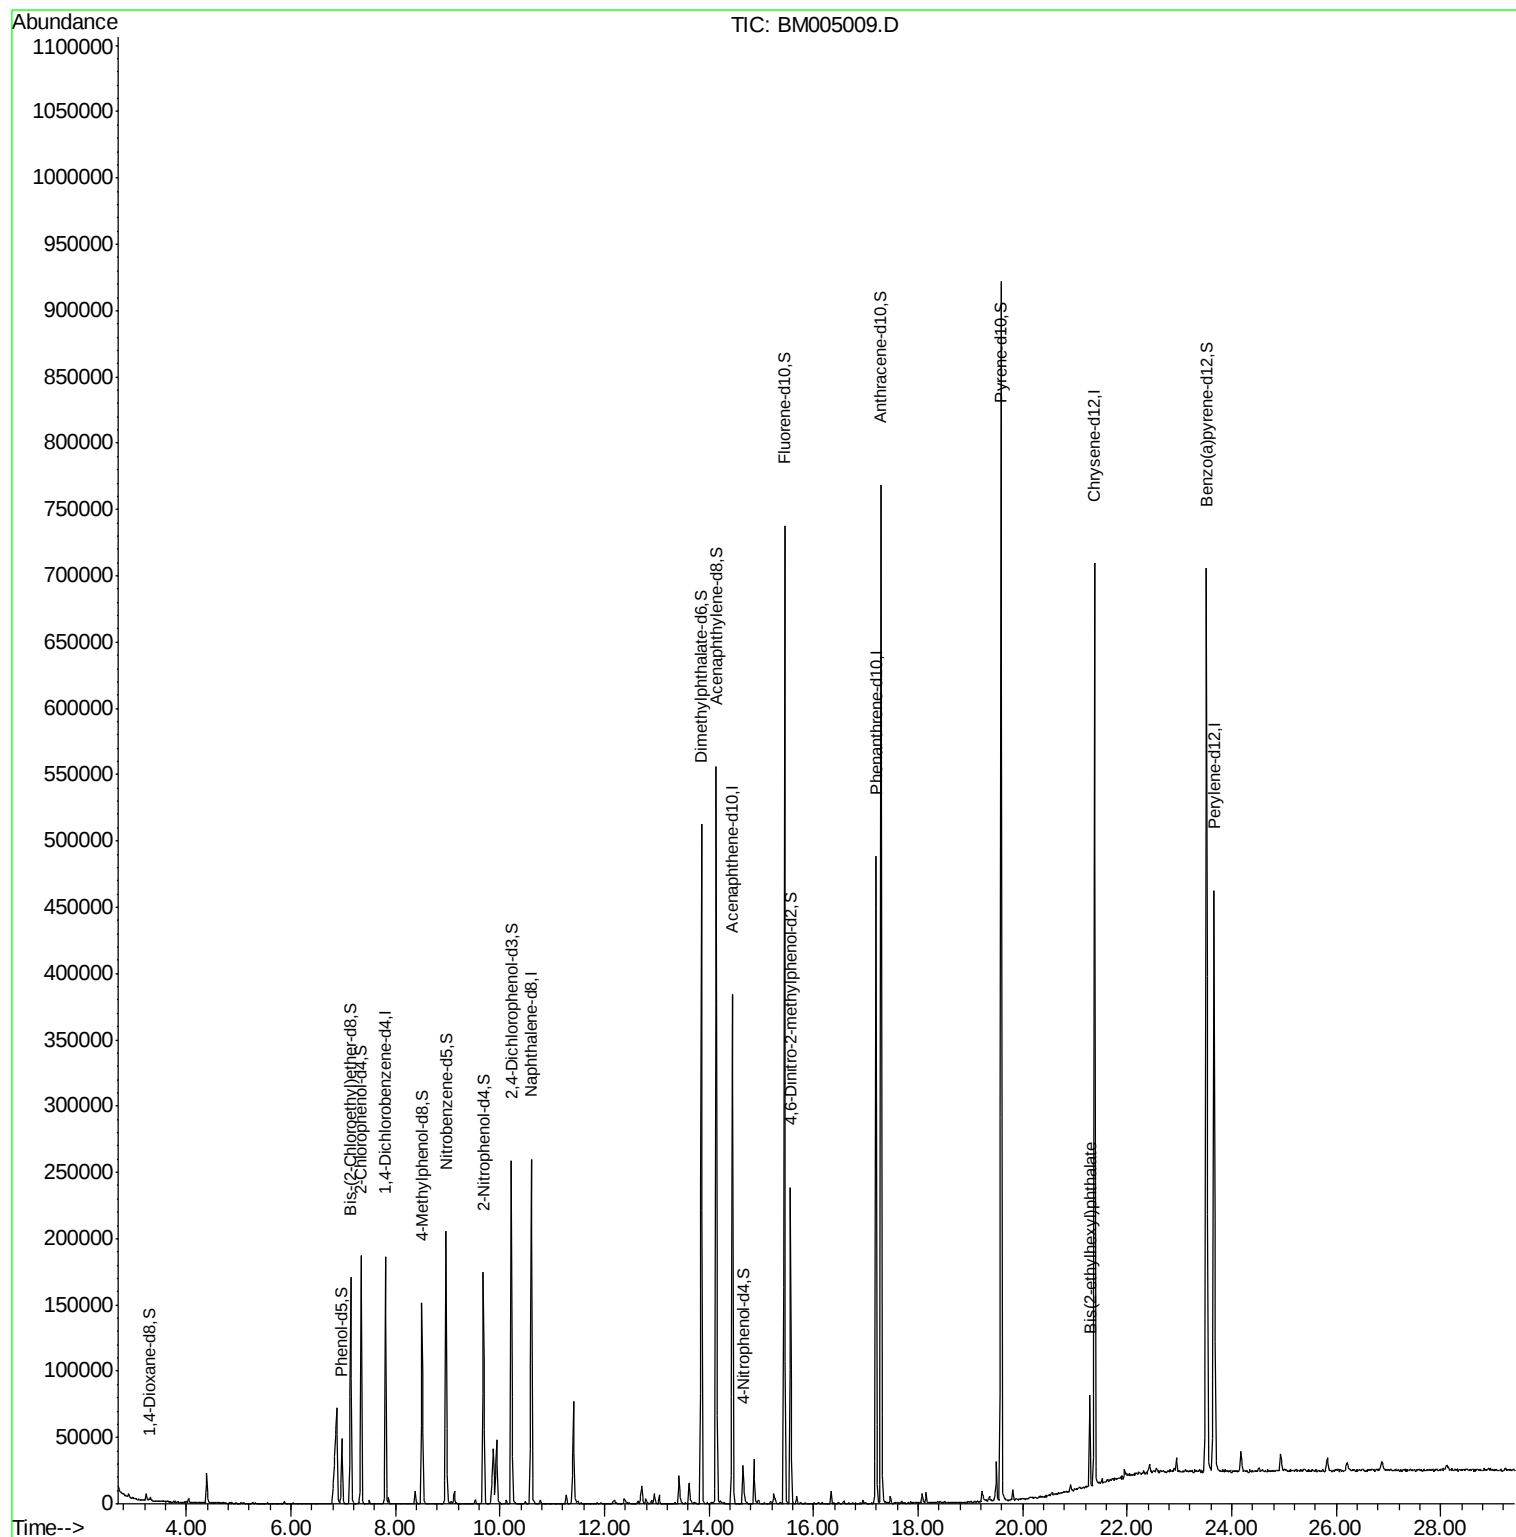

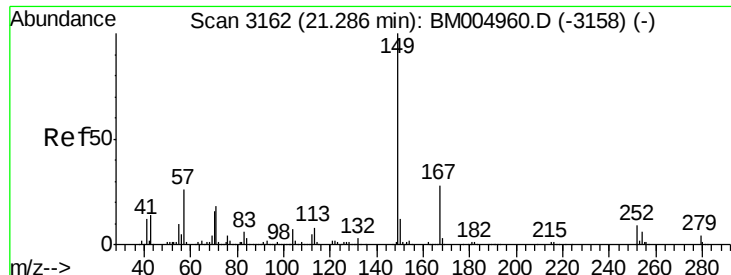

#81
 Bis(2-ethylhexyl)phthalate
 Concen: 2.44 ng/ul
 RT: 21.28 min Scan# 3161
 Delta R.T. -0.01 min
 Lab File: BM005009.D
 Acq: 21 Apr 2016 02:57

Instrument :
 BNA_M
 ClientSampleId :
 BC7R1

Tgt Ion	Ratio	Lower	Upper
149	100		
167	28.5	22.7	34.1
279	4.7	3.4	5.0

