

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
 Data File : BM005012.D
 Acq On : 21 Apr 2016 04:45
 Operator : UM/SJ
 Sample : H2567-26
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7R4

Quant Time: Apr 21 11:14:36 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 15 22:59:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	51325	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	220386	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	128123	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	295735	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	346459	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	335169	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	2174	2.27	ng/uL	0.00
5) Phenol-d5	6.97	99	40870	11.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	79433	37.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	96267	31.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	63130	20.86	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	54851	37.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	62618	38.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	104867	35.15	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.85	166	340041	39.02	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	409467	38.31	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	14708	9.89	ng/ul	0.00
57) Fluorene-d10	15.44	176	292420	38.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	49872	38.99	ng/ul	0.00
70) Anthracene-d10	17.29	188	448670	38.18	ng/ul	0.00
76) Pyrene-d10	19.58	212	516443	35.77	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	500877	38.81	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.34	88	10545	6.03 ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005012.D
Acq On : 21 Apr 2016 04:45
Operator : UM/SJ
Sample : H2567-26
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7R4

Quant Time: Apr 21 11:14:36 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 15 22:59:24 2016
Response via : Initial Calibration

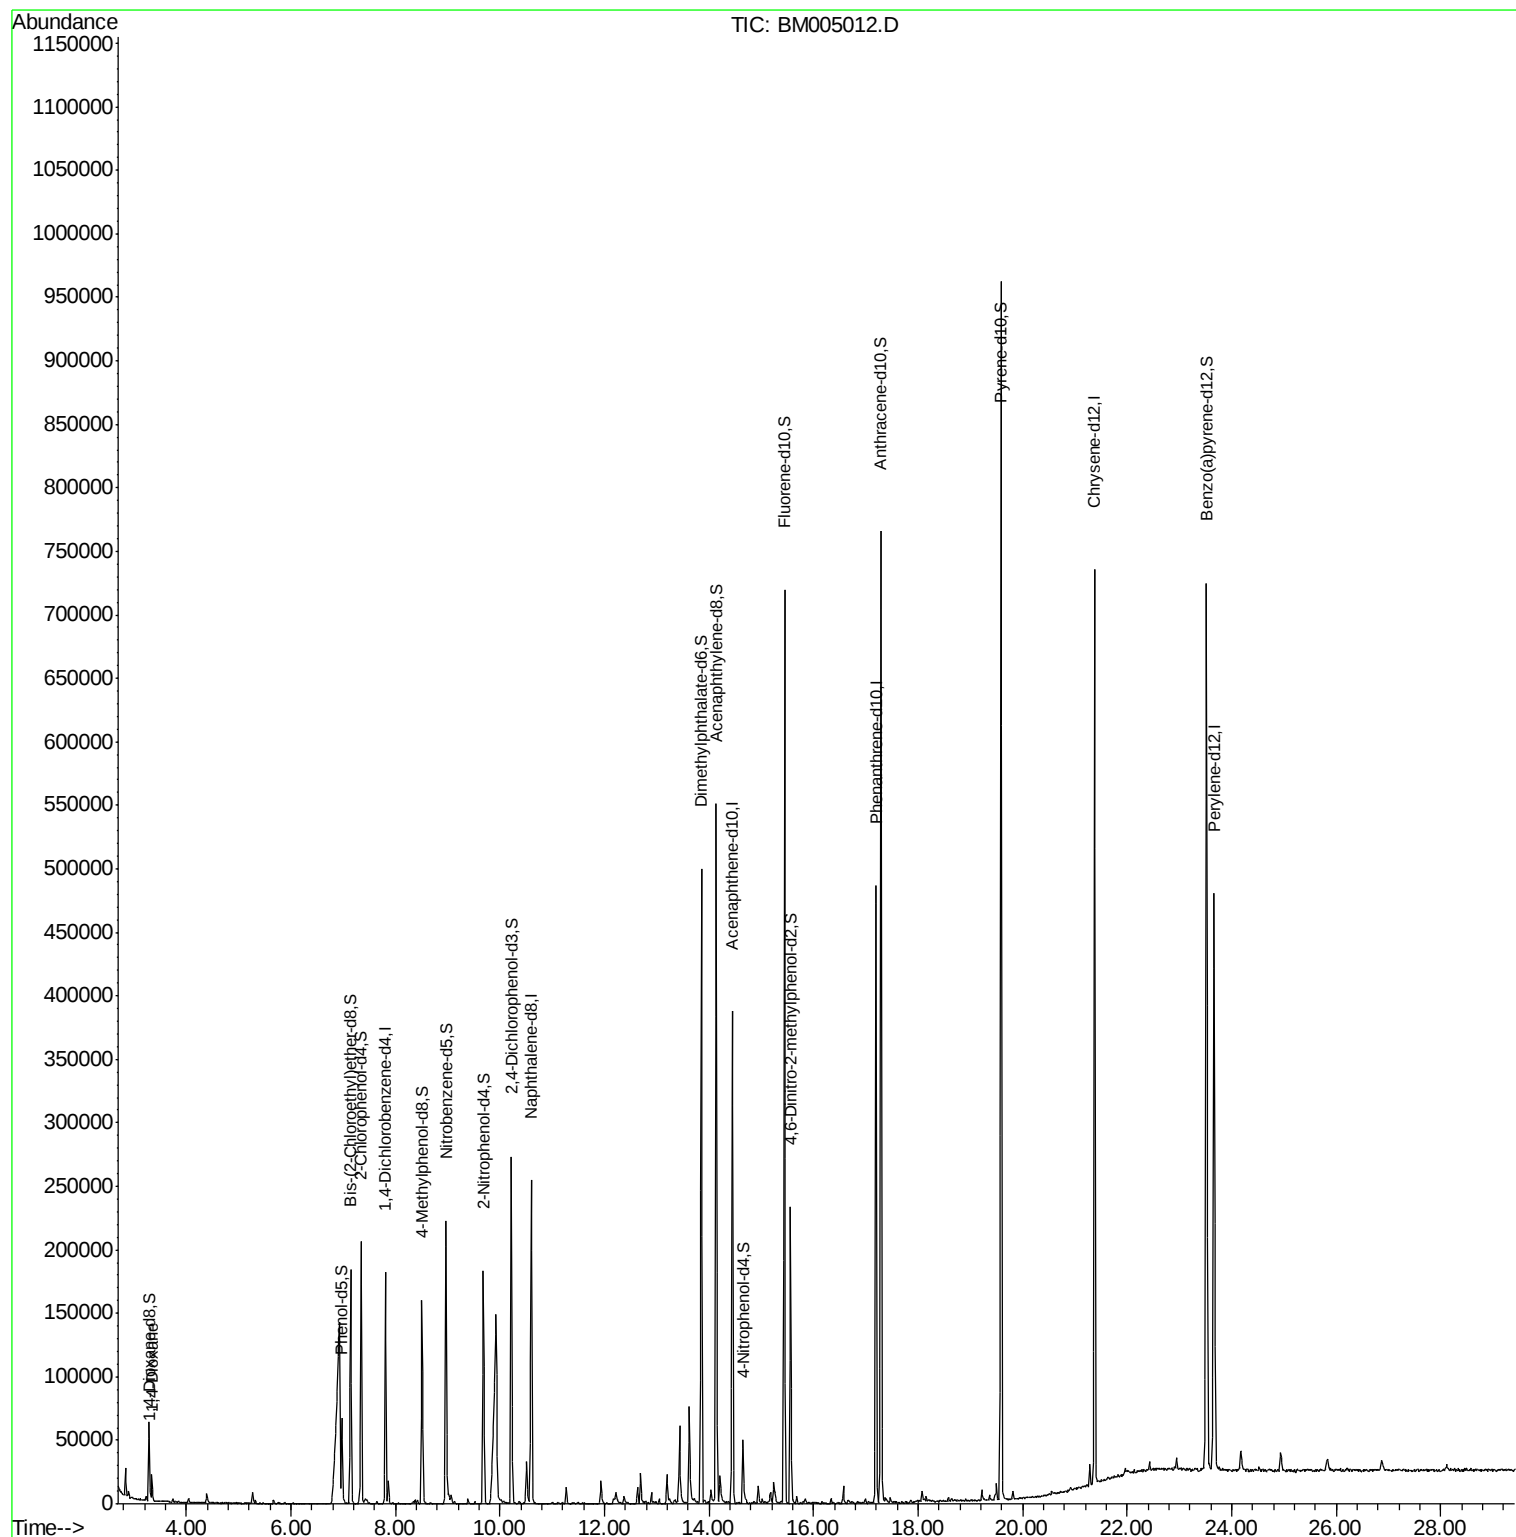

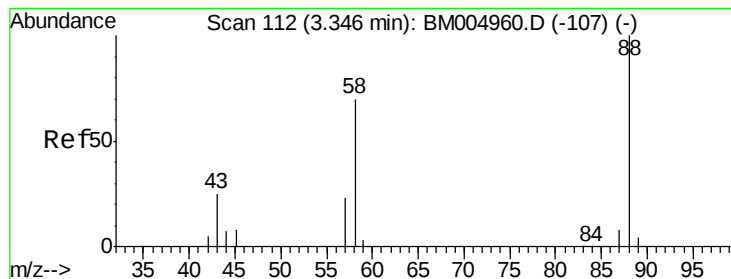

#2

1,4-Dioxane

Concen: 6.03 ng/uL

RT: 3.34 min Scan# 111

Delta R.T. 0.00 min

Lab File: BM005012.D

Acq: 21 Apr 2016 04:45

Instrument :

BNA_M

ClientSampleId :

BC7R4

Tgt Ion: 88 Resp: 10545

Ion Ratio Lower Upper

88 100

43 25.5 23.0 34.4

58 71.8 55.4 83.2

