

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
 Data File : BM005023.D
 Acq On : 21 Apr 2016 14:24
 Operator : UM/SJ
 Sample : H2567-05DL2 250X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7M3DL2

Manual Integrations
 APPROVED

UMANGI
 4/21/2016 8:12:26 PM

Quant Time: Apr 21 15:38:17 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 15 22:59:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	73690m	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	315631m	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	187756m	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	428732m	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	495565m	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	472893m	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.44	176	896m	0.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.19	188	431052m	25.30	ng/ul	-0.10
76) Pyrene-d10	0.00	212	0	0.00	ng/ul	
87) Benzo(a)pyrene-d12	0.00	264	0	0.00	ng/ul	

Target Compounds					Qvalue
28) Naphthalene	10.65	128	35001m	2.49	ng/ul

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005023.D
Acq On : 21 Apr 2016 14:24
Operator : UM/SJ
Sample : H2567-05DL2 250X
Misc :
ALS Vial : 37 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
BC7M3DL2

Manual Integrations
APPROVED

UMANGI
4/21/2016 8:12:26 PM

Quant Time: Apr 21 15:38:17 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 15 22:59:24 2016
Response via : Initial Calibration

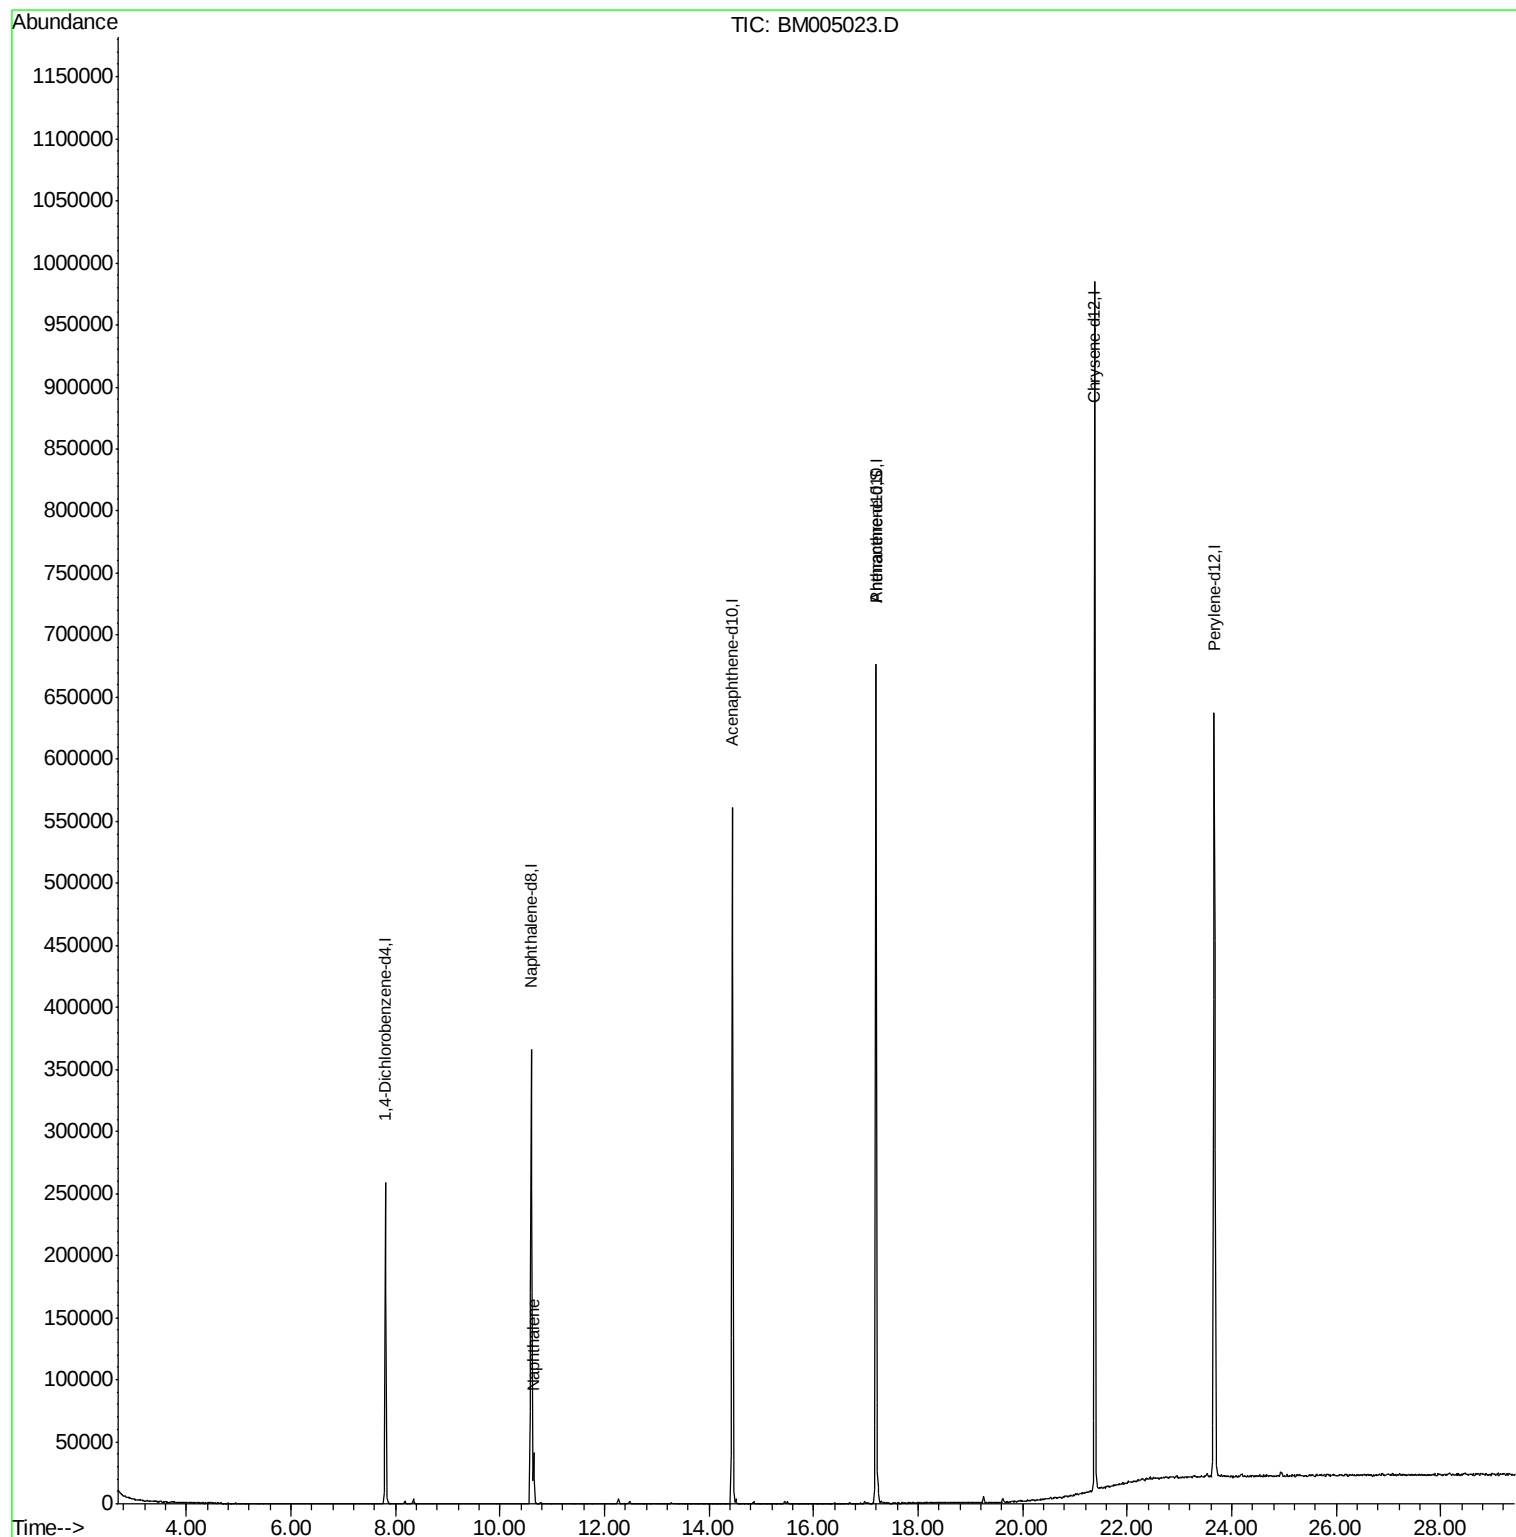

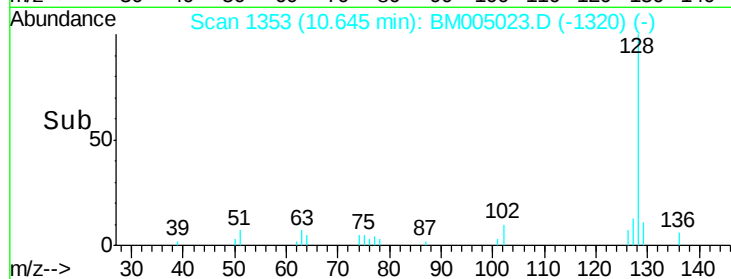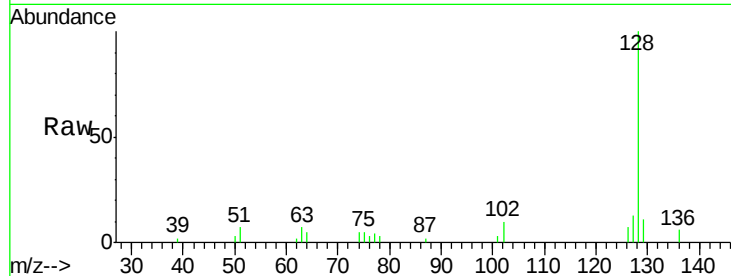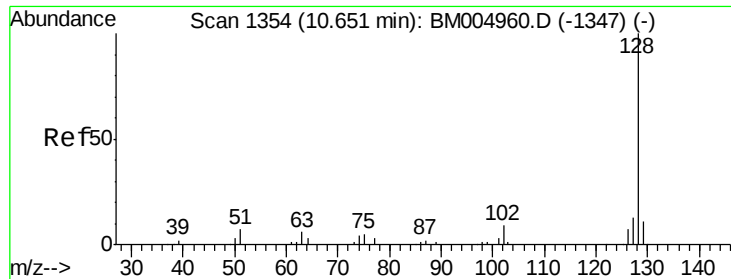

#28

Naphthalene

Concen: 2.49 ng/ul m

RT: 10.65 min Scan# 1353

Delta R.T. -0.01 min

Lab File: BM005023.D

Acq: 21 Apr 2016 14:24

Tgt Ion:	128	Resp:	35001
Ion Ratio	Lower	Upper	
128	100		
129	11.2	8.7	13.1
127	13.0	10.6	15.8

Instrument :

BNA_M

ClientSampleId :

BC7M3DL2

Manual Integrations
APPROVED

UMANGI
4/21/2016 8:12:26 PM

