

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
 Data File : BM005000.D
 Acq On : 20 Apr 2016 20:53
 Operator : UM/SJ
 Sample : PB89896BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.310	101	106	111	rVB	14368	18928	1.48%	0.149%
2	6.975	723	729	741	rBV	208457	335394	26.28%	2.637%
3	7.140	751	757	772	rBB	178747	280754	22.00%	2.207%
4	7.339	785	791	805	rBB	227426	360878	28.28%	2.837%
5	7.810	865	871	881	rBV	162827	258515	20.26%	2.032%
6	8.510	984	990	1003	rBV	263873	436037	34.17%	3.428%
7	8.963	1061	1067	1081	rBV	206367	337543	26.45%	2.654%
8	9.681	1184	1189	1200	rBB	163457	275972	21.62%	2.170%
9	10.216	1274	1280	1296	rBV	252558	428075	33.54%	3.366%
10	10.598	1338	1345	1354	rBV	226401	382763	29.99%	3.009%
11	10.733	1362	1368	1380	rBV	253230	439528	34.44%	3.456%
12	13.851	1892	1898	1910	rBV	479716	664108	52.04%	5.221%
13	14.139	1940	1947	1956	rBV	552089	802162	62.85%	6.307%
14	14.445	1993	1999	2007	rBV2	326456	504522	39.53%	3.967%
15	14.645	2027	2033	2048	rBV	144646	252925	19.82%	1.988%
16	15.439	2162	2168	2176	rBV	704042	1005628	78.80%	7.906%
17	15.557	2183	2188	2195	rBV	178365	244686	19.17%	1.924%
18	17.192	2460	2466	2473	rBV	411056	586783	45.98%	4.613%
19	17.292	2476	2483	2505	rVB	727386	1082061	84.78%	8.507%
20	19.586	2867	2873	2884	rBV	906661	1269653	99.48%	9.982%
21	21.374	3172	3177	3188	rBV	547877	736965	57.74%	5.794%
22	23.521	3534	3542	3555	rBV2	677022	1276246	100.00%	10.034%
23	23.662	3559	3566	3579	rVB2	370354	720832	56.48%	5.667%
24	24.185	3652	3655	3660	rVB3	11408	18459	1.45%	0.145%


Sum of corrected areas: 12719417

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005000.D
Acq On : 20 Apr 2016 20:53
Operator : UM/SJ
Sample : PB89896BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK96

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

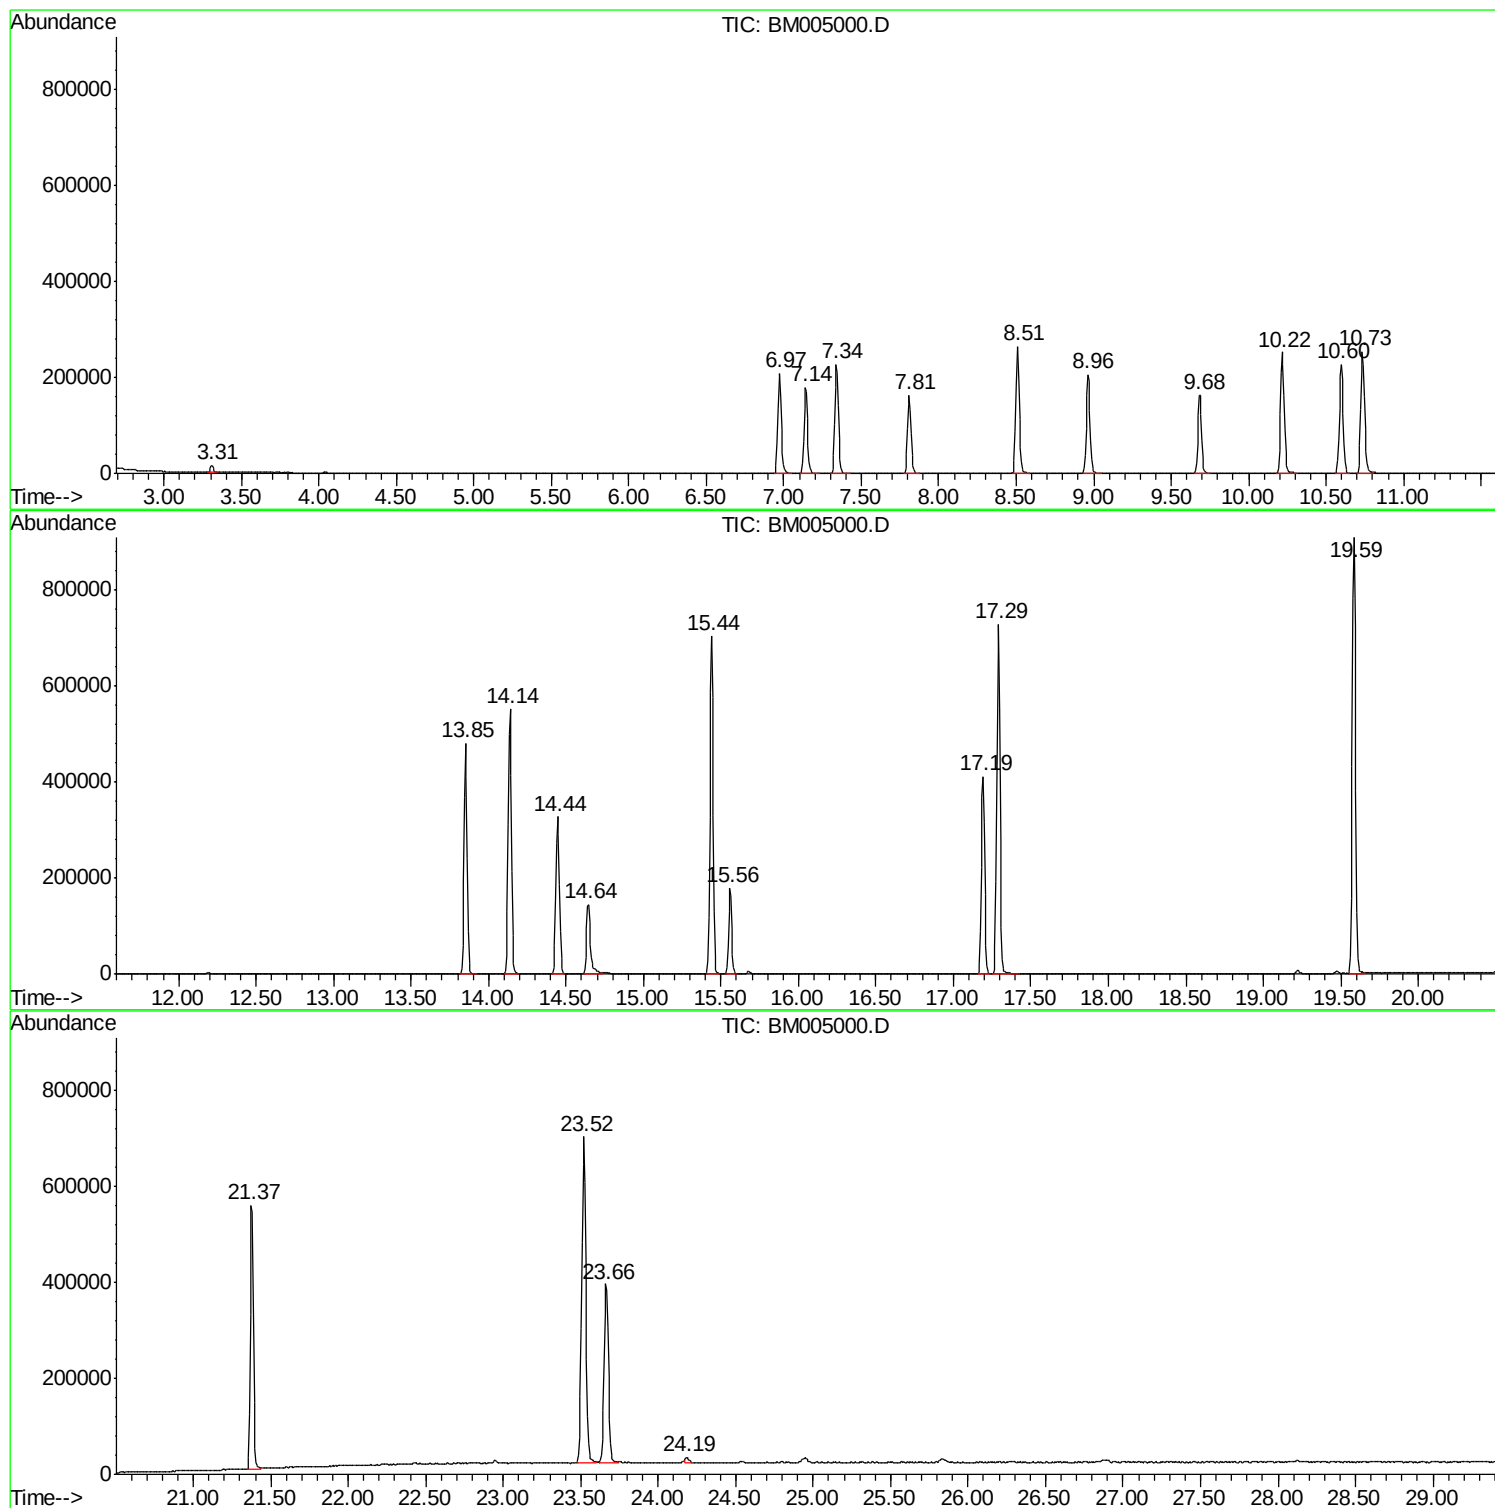

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005000.D
Acq On : 20 Apr 2016 20:53
Operator : UM/SJ
Sample : PB89896BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK96

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005000.D
Acq On : 20 Apr 2016 20:53
Operator : UM/SJ
Sample : PB89896BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK96

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc