

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
 Data File : BM005001.D
 Acq On : 20 Apr 2016 21:29
 Operator : UM/SJ
 Sample : PB89893BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	101	105	113	rVB	15161	19651	1.54%	0.151%
2	6.975	723	729	748	rBV	213176	344525	27.01%	2.648%
3	7.140	751	757	771	rVV	183201	287881	22.57%	2.213%
4	7.340	785	791	801	rBV	232252	369808	29.00%	2.842%
5	7.810	865	871	882	rBB	167162	264418	20.73%	2.032%
6	8.510	984	990	1001	rBV	276710	449877	35.27%	3.458%
7	8.963	1061	1067	1082	rBV	212427	347619	27.26%	2.672%
8	9.681	1184	1189	1201	rBB	167136	284117	22.28%	2.184%
9	10.216	1274	1280	1294	rBV	262777	443558	34.78%	3.409%
10	10.598	1338	1345	1354	rBV	237609	400201	31.38%	3.076%
11	10.734	1362	1368	1382	rBV	260407	460847	36.14%	3.542%
12	13.851	1892	1898	1907	rBV	497400	690392	54.13%	5.306%
13	14.139	1940	1947	1957	rBV	556585	839519	65.83%	6.452%
14	14.445	1991	1999	2009	rBV2	340563	528616	41.45%	4.063%
15	14.645	2027	2033	2055	rBV	148221	255848	20.06%	1.966%
16	15.439	2162	2168	2178	rBV	717403	1039415	81.50%	7.989%
17	15.557	2183	2188	2198	rVB	179953	242025	18.98%	1.860%
18	17.192	2460	2466	2476	rBV	422391	598398	46.92%	4.599%
19	17.292	2476	2483	2496	rVV	734514	1108386	86.91%	8.519%
20	19.586	2867	2873	2884	rBV2	896808	1267809	99.41%	9.744%
21	21.374	3172	3177	3187	rBV	546148	729046	57.16%	5.603%
22	23.521	3534	3542	3555	rBV2	663824	1275344	100.00%	9.802%
23	23.662	3558	3566	3577	rVB2	361434	710987	55.75%	5.464%
24	24.180	3650	3654	3661	rBV2	14858	23776	1.86%	0.183%
25	24.950	3779	3785	3792	rVB2	14107	29161	2.29%	0.224%


Sum of corrected areas: 13011224

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005001.D
Acq On : 20 Apr 2016 21:29
Operator : UM/SJ
Sample : PB89893BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK93

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

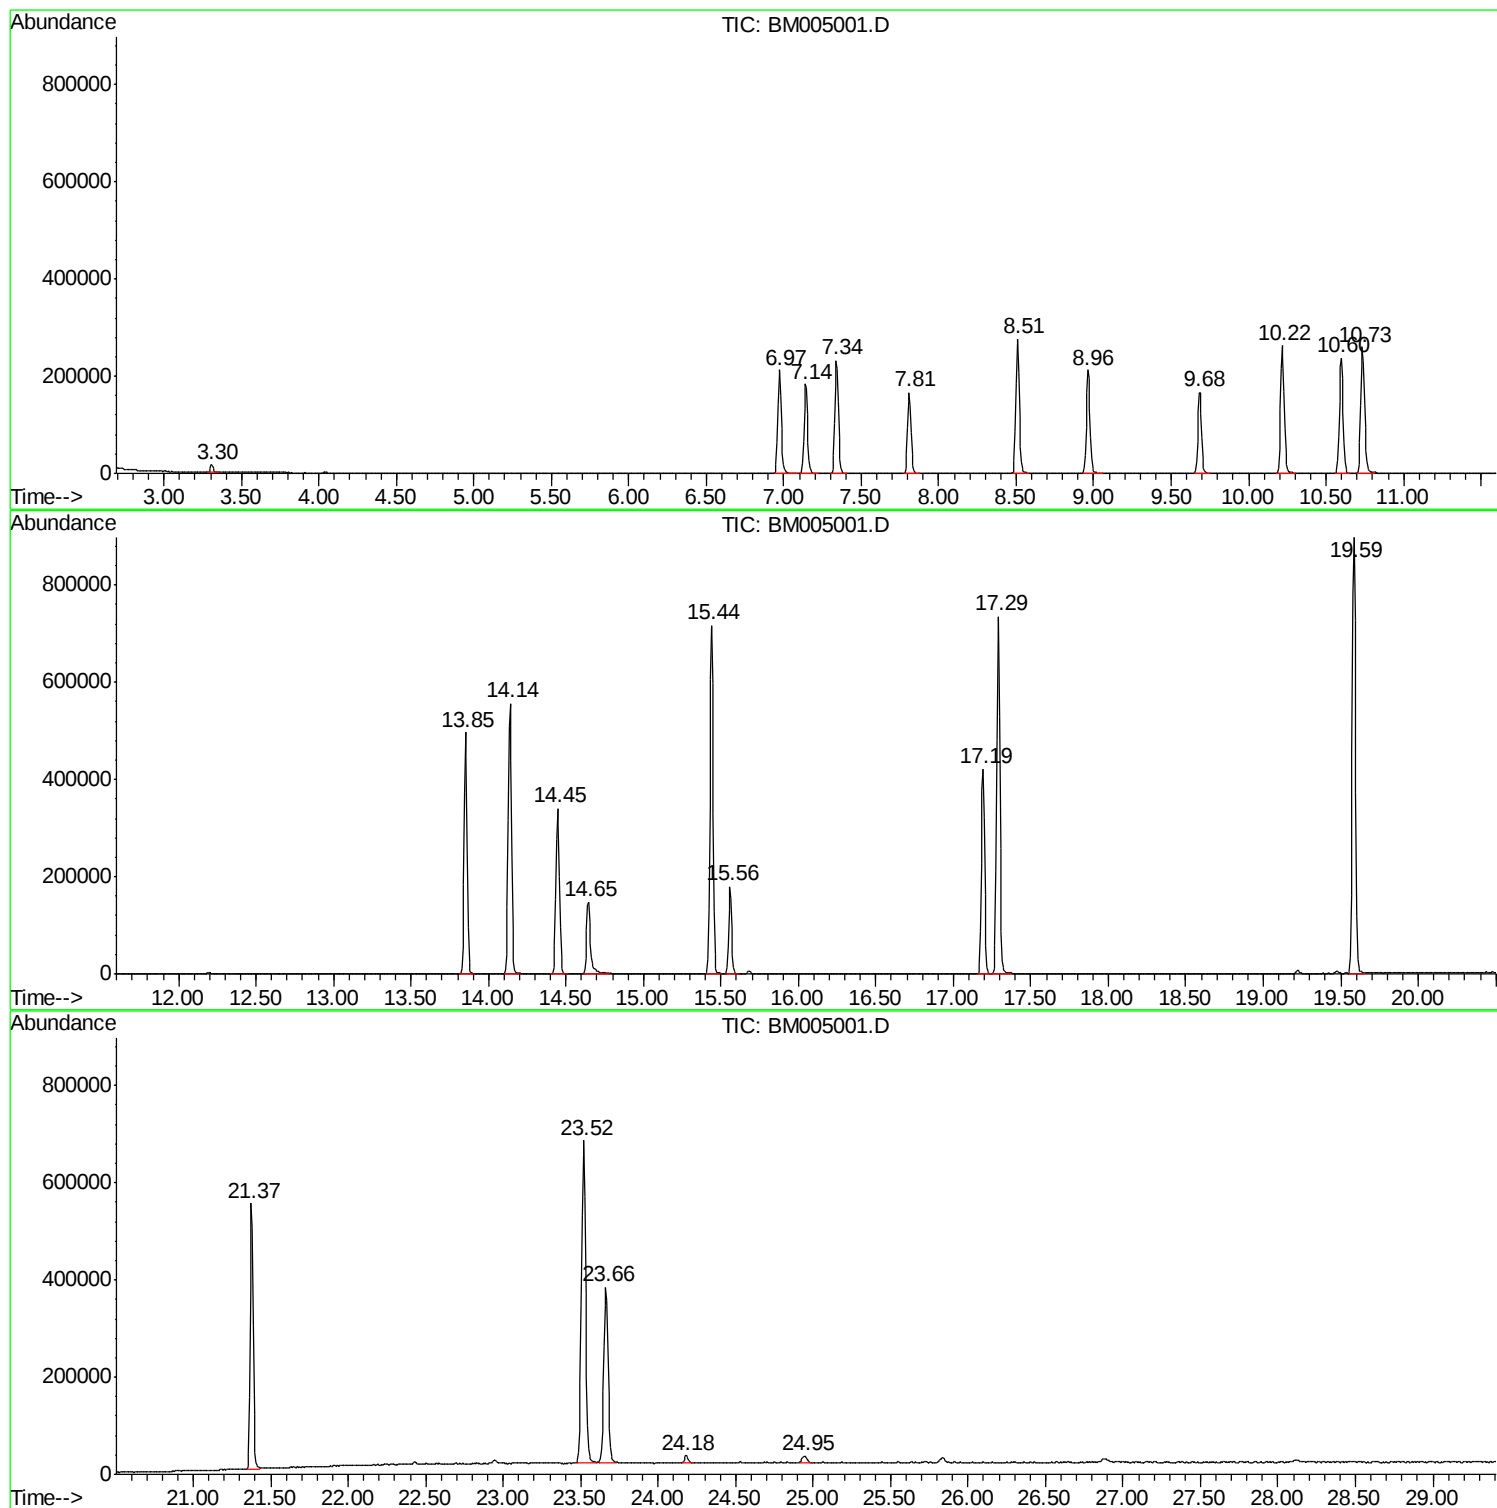

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005001.D
Acq On : 20 Apr 2016 21:29
Operator : UM/SJ
Sample : PB89893BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK93

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005001.D
Acq On : 20 Apr 2016 21:29
Operator : UM/SJ
Sample : PB89893BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK93

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc