

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
 Data File : BM005002.D
 Acq On : 20 Apr 2016 22:06
 Operator : UM/SJ
 Sample : PB89890BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.304	101	105	112	rVB	14191	18446	1.43%	0.146%
2	6.975	723	729	746	rBV	202064	324367	25.08%	2.569%
3	7.139	751	757	770	rBV	174266	272826	21.10%	2.160%
4	7.339	785	791	804	rBB	219300	348113	26.92%	2.757%
5	7.810	865	871	882	rBB	157836	250392	19.36%	1.983%
6	8.510	984	990	1005	rBV	251444	415880	32.16%	3.293%
7	8.963	1061	1067	1081	rBV	195221	321884	24.89%	2.549%
8	9.680	1184	1189	1201	rBB	156908	261913	20.25%	2.074%
9	10.216	1274	1280	1293	rBV	244965	406929	31.47%	3.222%
10	10.598	1338	1345	1353	rBV	222439	371749	28.75%	2.944%
11	10.733	1362	1368	1382	rBV	243465	429094	33.18%	3.398%
12	13.851	1892	1898	1912	rBV	465351	654195	50.59%	5.180%
13	14.139	1939	1947	1957	rBV	535298	786147	60.79%	6.225%
14	14.445	1992	1999	2008	rVB2	327088	496467	38.39%	3.931%
15	14.645	2027	2033	2058	rBV	143266	248804	19.24%	1.970%
16	15.439	2162	2168	2183	rVB	680042	999073	77.25%	7.911%
17	15.557	2183	2188	2196	rBV	174668	241868	18.70%	1.915%
18	17.192	2460	2466	2474	rBV	417551	588507	45.51%	4.660%
19	17.292	2476	2483	2497	rVB	729405	1087181	84.07%	8.609%
20	19.586	2867	2873	2887	rBV	923321	1286358	99.47%	10.186%
21	21.374	3172	3177	3187	rBV	586239	753598	58.27%	5.968%
22	23.515	3534	3541	3554	rBV2	666127	1293229	100.00%	10.241%
23	23.662	3558	3566	3578	rVB2	369386	726588	56.18%	5.754%
24	24.179	3650	3654	3660	rVB	12172	21422	1.66%	0.170%
25	24.938	3779	3783	3790	rVB2	11554	23305	1.80%	0.185%


Sum of corrected areas: 12628335

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005002.D
Acq On : 20 Apr 2016 22:06
Operator : UM/SJ
Sample : PB89890BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK90

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

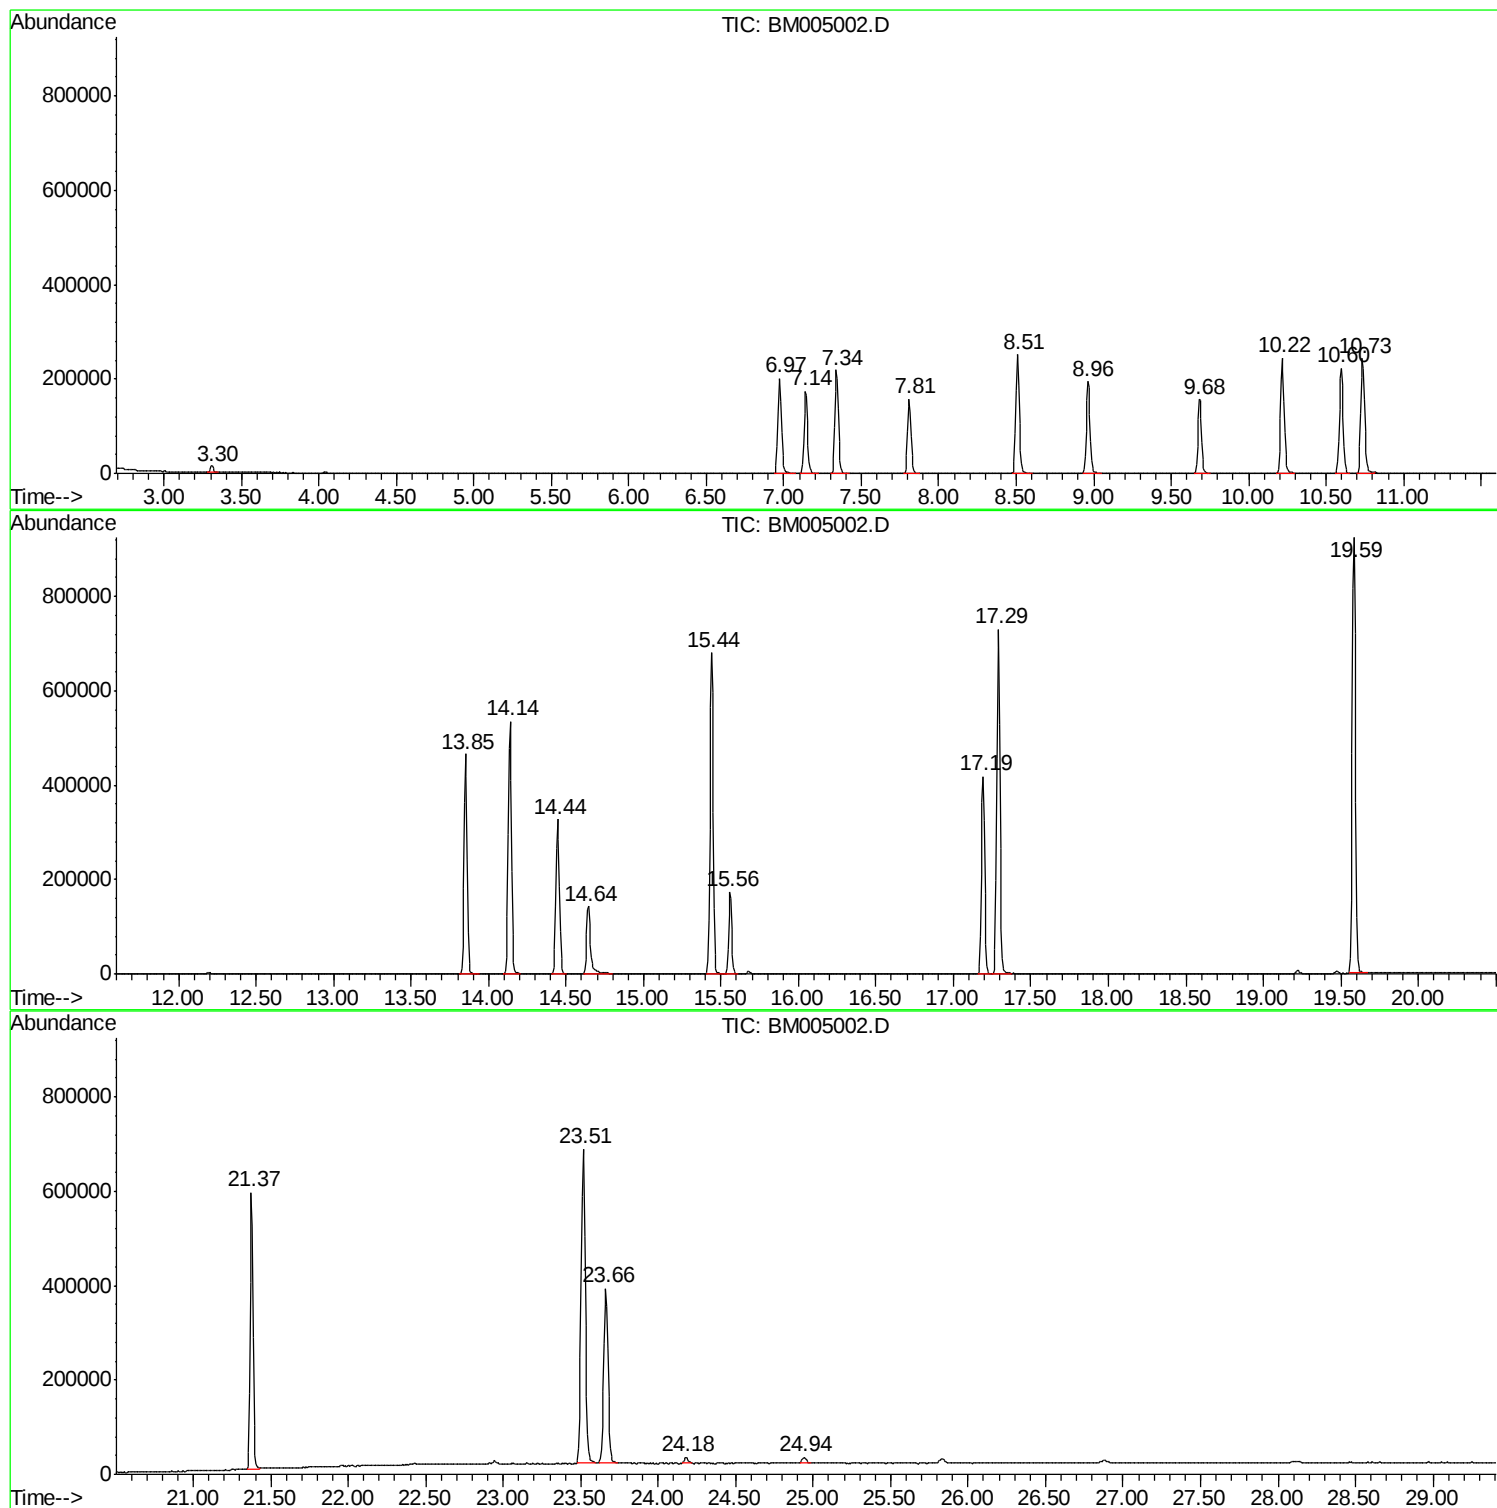

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005002.D
Acq On : 20 Apr 2016 22:06
Operator : UM/SJ
Sample : PB89890BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK90

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005002.D
Acq On : 20 Apr 2016 22:06
Operator : UM/SJ
Sample : PB89890BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK90

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc