

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
 Data File : BM005003.D
 Acq On : 20 Apr 2016 22:42
 Operator : UM/SJ
 Sample : PB89939BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK39

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.310	102	106	113	rVB	14042	18329	1.44%	0.146%
2	6.975	723	729	744	rBV	207502	331914	26.14%	2.643%
3	7.139	751	757	771	rBV	179757	282859	22.28%	2.252%
4	7.339	785	791	802	rBV	224723	356265	28.06%	2.836%
5	7.810	865	871	882	rBB	163465	256555	20.20%	2.043%
6	8.510	984	990	1003	rBV	258026	427290	33.65%	3.402%
7	8.963	1061	1067	1078	rBV	200453	329996	25.99%	2.627%
8	9.686	1184	1190	1202	rBB	161125	268280	21.13%	2.136%
9	10.216	1274	1280	1297	rBV	252450	421210	33.17%	3.353%
10	10.598	1338	1345	1358	rBB	227484	384322	30.27%	3.060%
11	10.733	1362	1368	1383	rBV	248301	436975	34.41%	3.479%
12	13.851	1892	1898	1909	rBV	473018	649998	51.19%	5.175%
13	14.139	1940	1947	1955	rBV	529206	796370	62.72%	6.340%
14	14.445	1993	1999	2007	rBB2	326748	502890	39.60%	4.004%
15	14.645	2028	2033	2054	rBV	136952	241337	19.01%	1.921%
16	15.439	2162	2168	2179	rBV	693160	993300	78.23%	7.908%
17	15.557	2184	2188	2196	rVV	170426	229290	18.06%	1.825%
18	17.192	2460	2466	2473	rBV2	396310	573766	45.19%	4.568%
19	17.292	2476	2483	2499	rVV2	708378	1064946	83.87%	8.479%
20	19.586	2866	2873	2884	rBV	893999	1239452	97.61%	9.868%
21	21.374	3172	3177	3189	rBV	559018	719788	56.69%	5.731%
22	23.515	3533	3541	3552	rBV2	660842	1269764	100.00%	10.109%
23	23.656	3558	3565	3580	rVB2	364960	708619	55.81%	5.642%
24	24.174	3649	3653	3662	rVB3	15586	28305	2.23%	0.225%
25	24.938	3778	3783	3789	rVB4	13965	28683	2.26%	0.228%


Sum of corrected areas: 12560503

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005003.D
Acq On : 20 Apr 2016 22:42
Operator : UM/SJ
Sample : PB89939BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK39

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

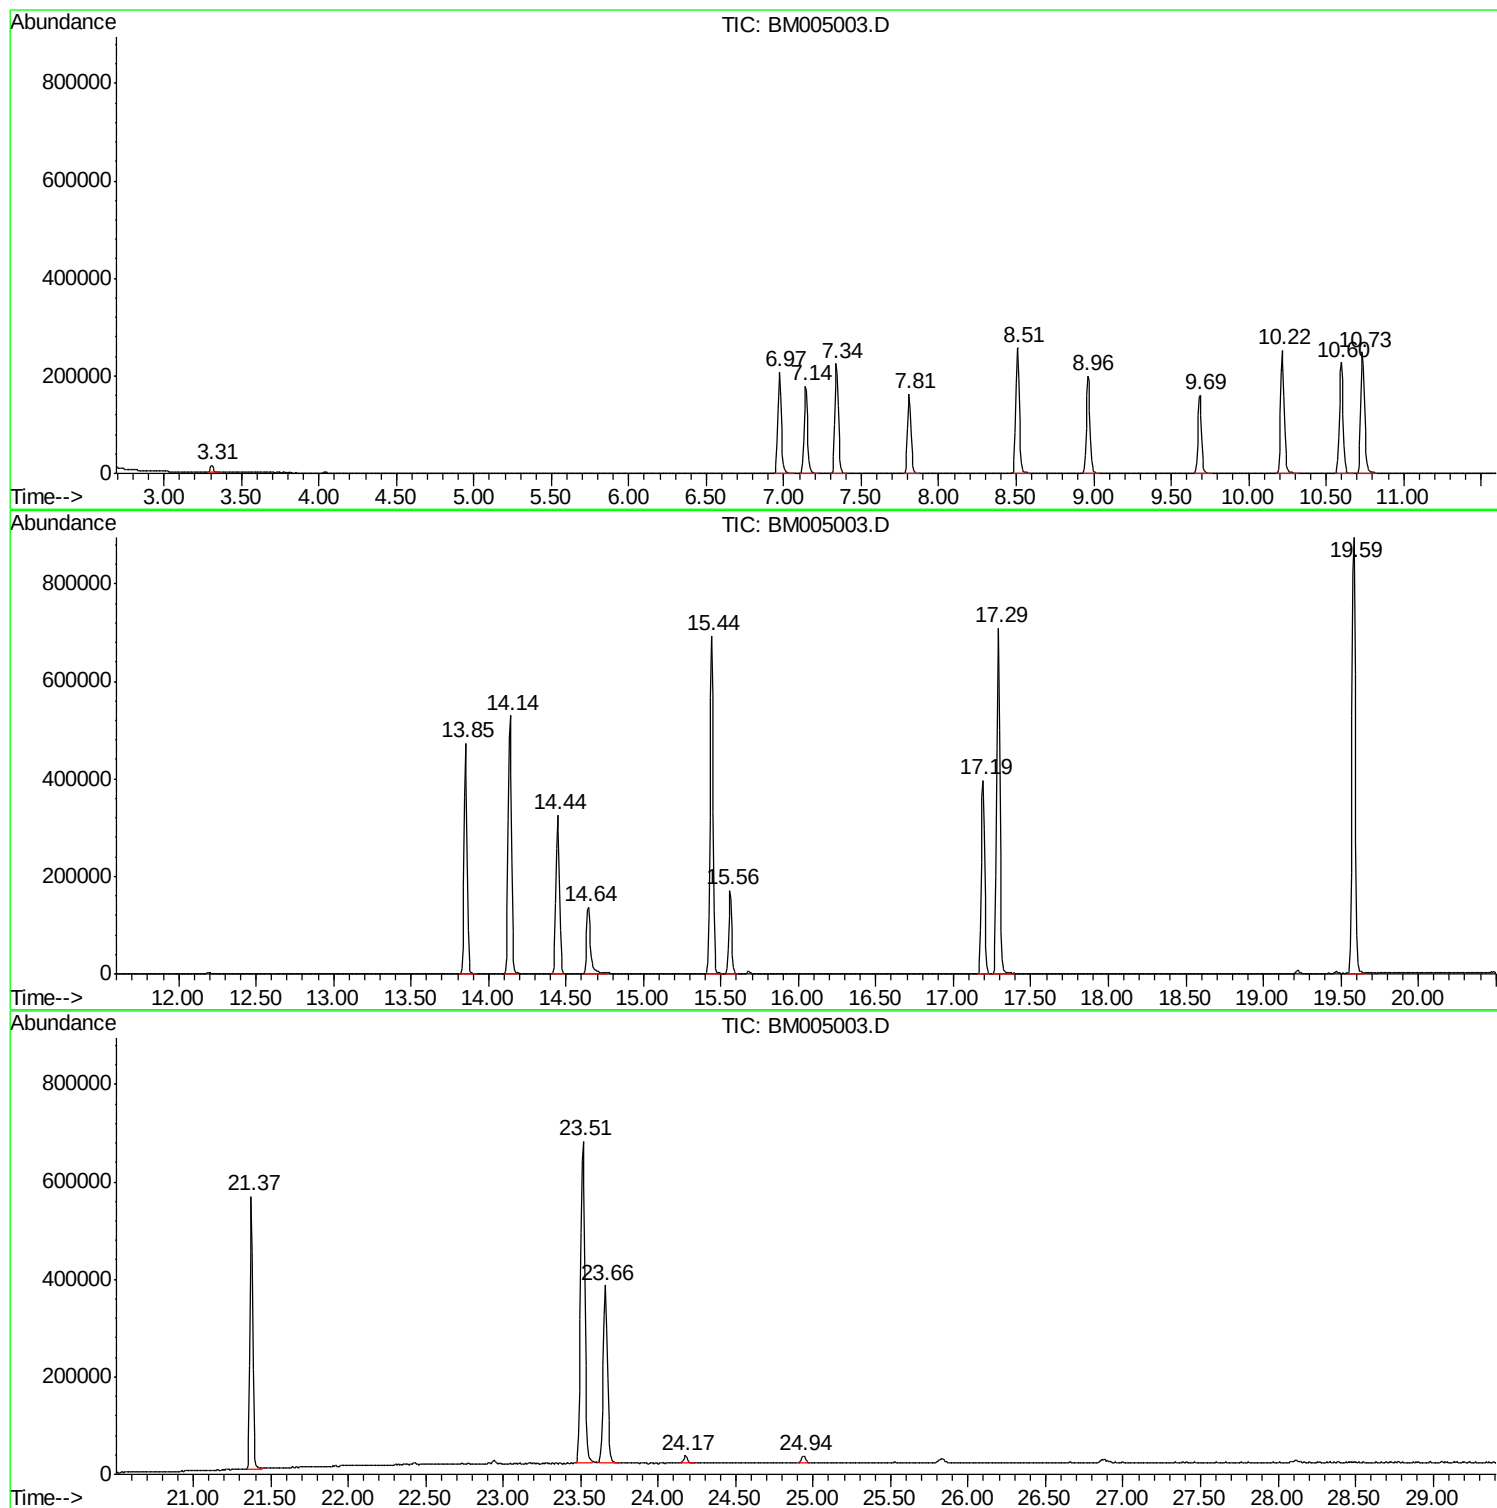

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005003.D
Acq On : 20 Apr 2016 22:42
Operator : UM/SJ
Sample : PB89939BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK39

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042016\
Data File : BM005003.D
Acq On : 20 Apr 2016 22:42
Operator : UM/SJ
Sample : PB89939BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK39

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc