

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042022\
 Data File : BM034722.D
 Acq On : 20 Apr 2022 09:37
 Operator : CG/JU
 Sample : SSTD00518
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD005018

Quant Time: Apr 20 12:49:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 12:46:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	228102	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	862982	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.580	164	558737	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.321	188	1137749	20.000	ng/u1	0.00
79) Chrysene-d12	21.497	240	1134716	20.000	ng/u1	0.00
88) Perylene-d12	23.897	264	1147270	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	8626	1.349	ng/uL	0.00
4) Pyridine-d5	3.804	84	47735	3.516	ng/u1	0.00
7) Phenol-d5	7.104	99	71366	3.622	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	37709	2.852	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	64101	4.239	ng/u1	0.00
15) 4-Methylphenol-d8	8.651	113	59138	3.802	ng/u1	0.00
21) Nitrobenzene-d5	9.104	128	24383	3.758	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	22430	3.183	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	66685	5.250	ng/u1	0.00
31) 4-Chloroaniline-d4	10.886	131	84901	4.962	ng/u1	0.00
46) Dimethylphthalate-d6	13.992	166	201764	4.890	ng/u1	0.00
49) Acenaphthylene-d8	14.274	160	248049	4.683	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	18730	3.166	ng/u1	0.00
60) Fluorene-d10	15.568	176	174652	5.006	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	14062	2.164	ng/u1	0.00
73) Anthracene-d10	17.421	188	258487	4.742	ng/u1	0.00
81) Pyrene-d10	19.703	212	287925	4.527	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.744	264	263042	4.526	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	9082	1.390	ng/uL	97
5) Pyridine	3.822	79	53115	3.373	ng/u1#	85
6) Benzaldehyde	7.081	77	46843	4.466	ng/u1	95
8) Phenol	7.134	94	70047	3.559	ng/u1	96
10) Bis(2-Chloroethyl)ether	7.369	93	54003	3.368	ng/u1	99
12) 2-Chlorophenol	7.510	128	64814	4.208	ng/u1	99
13) 2-Methylphenol	8.392	108	54140	3.654	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.481	45	63717	2.484	ng/u1#	90
16) Acetophenone	8.775	105	95108	3.879	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.757	70	40871	3.103	ng/u1	93
18) 4-Methylphenol	8.716	108	58386	3.669	ng/u1	99
19) Hexachloroethane	9.039	117	26978	3.914	ng/u1	91
22) Nitrobenzene	9.145	77	53896	3.146	ng/u1	96
23) Isophorone	9.681	82	113074	3.598	ng/u1	99
25) 2-Nitrophenol	9.863	139	24315	3.274	ng/u1	94
26) 2,4-Dimethylphenol	9.922	107	67840	4.199	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.163	93	71192	3.842	ng/u1	98
29) 2,4-Dichlorophenol	10.398	162	63200	5.157	ng/u1	98
30) Naphthalene	10.804	128	210704	4.625	ng/u1	99
32) 4-Chloroaniline	10.904	127	82839	4.766	ng/u1	99
33) Hexachlorobutadiene	11.104	225	54205	6.393	ng/u1	97
34) Caprolactam	11.669	113	12297	4.496	ng/u1	99
35) 4-Chloro-3-methylphenol	12.027	107	58088	4.326	ng/u1	96
36) 2-Methylnaphthalene	12.410	142	147562	4.989	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042022\
 Data File : BM034722.D
 Acq On : 20 Apr 2022 09:37
 Operator : CG/JU
 Sample : SST00518
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST005018


Quant Time: Apr 20 12:49:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 20 12:46:21 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.633	142	149623	4.947	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.780	216	99159	6.060	ng/ul	98
40) Hexachlorocyclopentadiene	12.769	237	53954	5.234	ng/ul	95
41) 2,4,6-Trichlorophenol	13.016	196	50013	4.936	ng/ul	97
42) 2,4,5-Trichlorophenol	13.080	196	53281	5.251	ng/ul	98
43) 1,1'-Biphenyl	13.421	154	206025	4.794	ng/ul	99
44) 2-Chloronaphthalene	13.457	162	160760	4.899	ng/ul	99
45) 2-Nitroaniline	13.651	65	20317	2.109	ng/ul	94
47) Dimethylphthalate	14.039	163	192397	4.793	ng/ul	99
48) 2,6-Dinitrotoluene	14.145	165	23712	3.023	ng/ul	98
50) Acenaphthylene	14.304	152	247484	4.629	ng/ul	100
51) 3-Nitroaniline	14.474	138	22148	3.738	ng/ul#	91
52) Acenaphthene	14.645	153	163675	4.592	ng/ul	98
53) 2,4-Dinitrophenol	14.674	184	9139	2.736	ng/ul#	84
55) 4-Nitrophenol	14.768	109	14746	2.869	ng/ul#	70
56) Dibenzofuran	14.980	168	242421	4.986	ng/ul	94
57) 2,4-Dinitrotoluene	14.927	165	31655	2.949	ng/ul#	98
58) 2,3,4,6-Tetrachlorophenol	15.204	232	43027	4.977	ng/ul	92
59) Diethylphthalate	15.404	149	178413	4.330	ng/ul	96
61) Fluorene	15.627	166	192483	4.721	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.621	204	107540	5.547	ng/ul	98
63) 4-Nitroaniline	15.627	138	22975	4.632	ng/ul	90
66) 4,6-Dinitro-2-methylph...	15.692	198	13889	2.189	ng/ul#	98
67) N-Nitrosodiphenylamine	15.833	169	159256	4.567	ng/ul	98
68) 4-Bromophenyl-phenylether	16.515	248	65348	5.540	ng/ul	98
69) Hexachlorobenzene	16.633	284	79208	5.651	ng/ul#	94
70) Atrazine	16.780	200	54808	4.258	ng/ul	99
71) Pentachlorophenol	16.968	266	33206	4.982	ng/ul	97
72) Phenanthrene	17.362	178	294285	4.569	ng/ul	99
74) Anthracene	17.451	178	293607	4.680	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.386	216	101478	5.661	ng/ul	99
76) Pentachlorobenzene	14.898	250	97208	5.767	ng/ul	99
77) Carbazole	17.715	167	241782	4.571	ng/ul	99
78) Di-n-butylphthalate	18.298	149	249119	3.626	ng/ul	100
80) Fluoranthene	19.374	202	332262	4.547	ng/ul	100
82) Pyrene	19.733	202	346249	4.505	ng/ul	98
83) Butylbenzylphthalate	20.639	149	90607	2.935	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.409	252	96233	4.781	ng/ul	99
85) Benzo(a)anthracene	21.480	228	330419	4.953	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.427	149	148037	3.225	ng/ul	97
87) Chrysene	21.533	228	322196	4.539	ng/ul	99
89) Di-n-octyl phthalate	22.356	149	235212	2.902	ng/ul	100
90) Benzo(b)fluoranthene	23.168	252	330212	4.762	ng/ul	99
91) Benzo(k)fluoranthene	23.215	252	311704	4.444	ng/ul#	98
93) Benzo(a)pyrene	23.791	252	310819	4.499	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.391	276	367344	4.860	ng/ul	98
95) Dibenzo(a,h)anthracene	26.409	278	313637	5.288	ng/ul	99
96) Benzo(g,h,i)perylene	27.150	276	319048	4.665	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
BNA_M
ClientSampleId :
SSTD005018

Quant Time: Apr 20 12:49:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM042022.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 20 12:46:21 2022
Response via : Initial Calibration




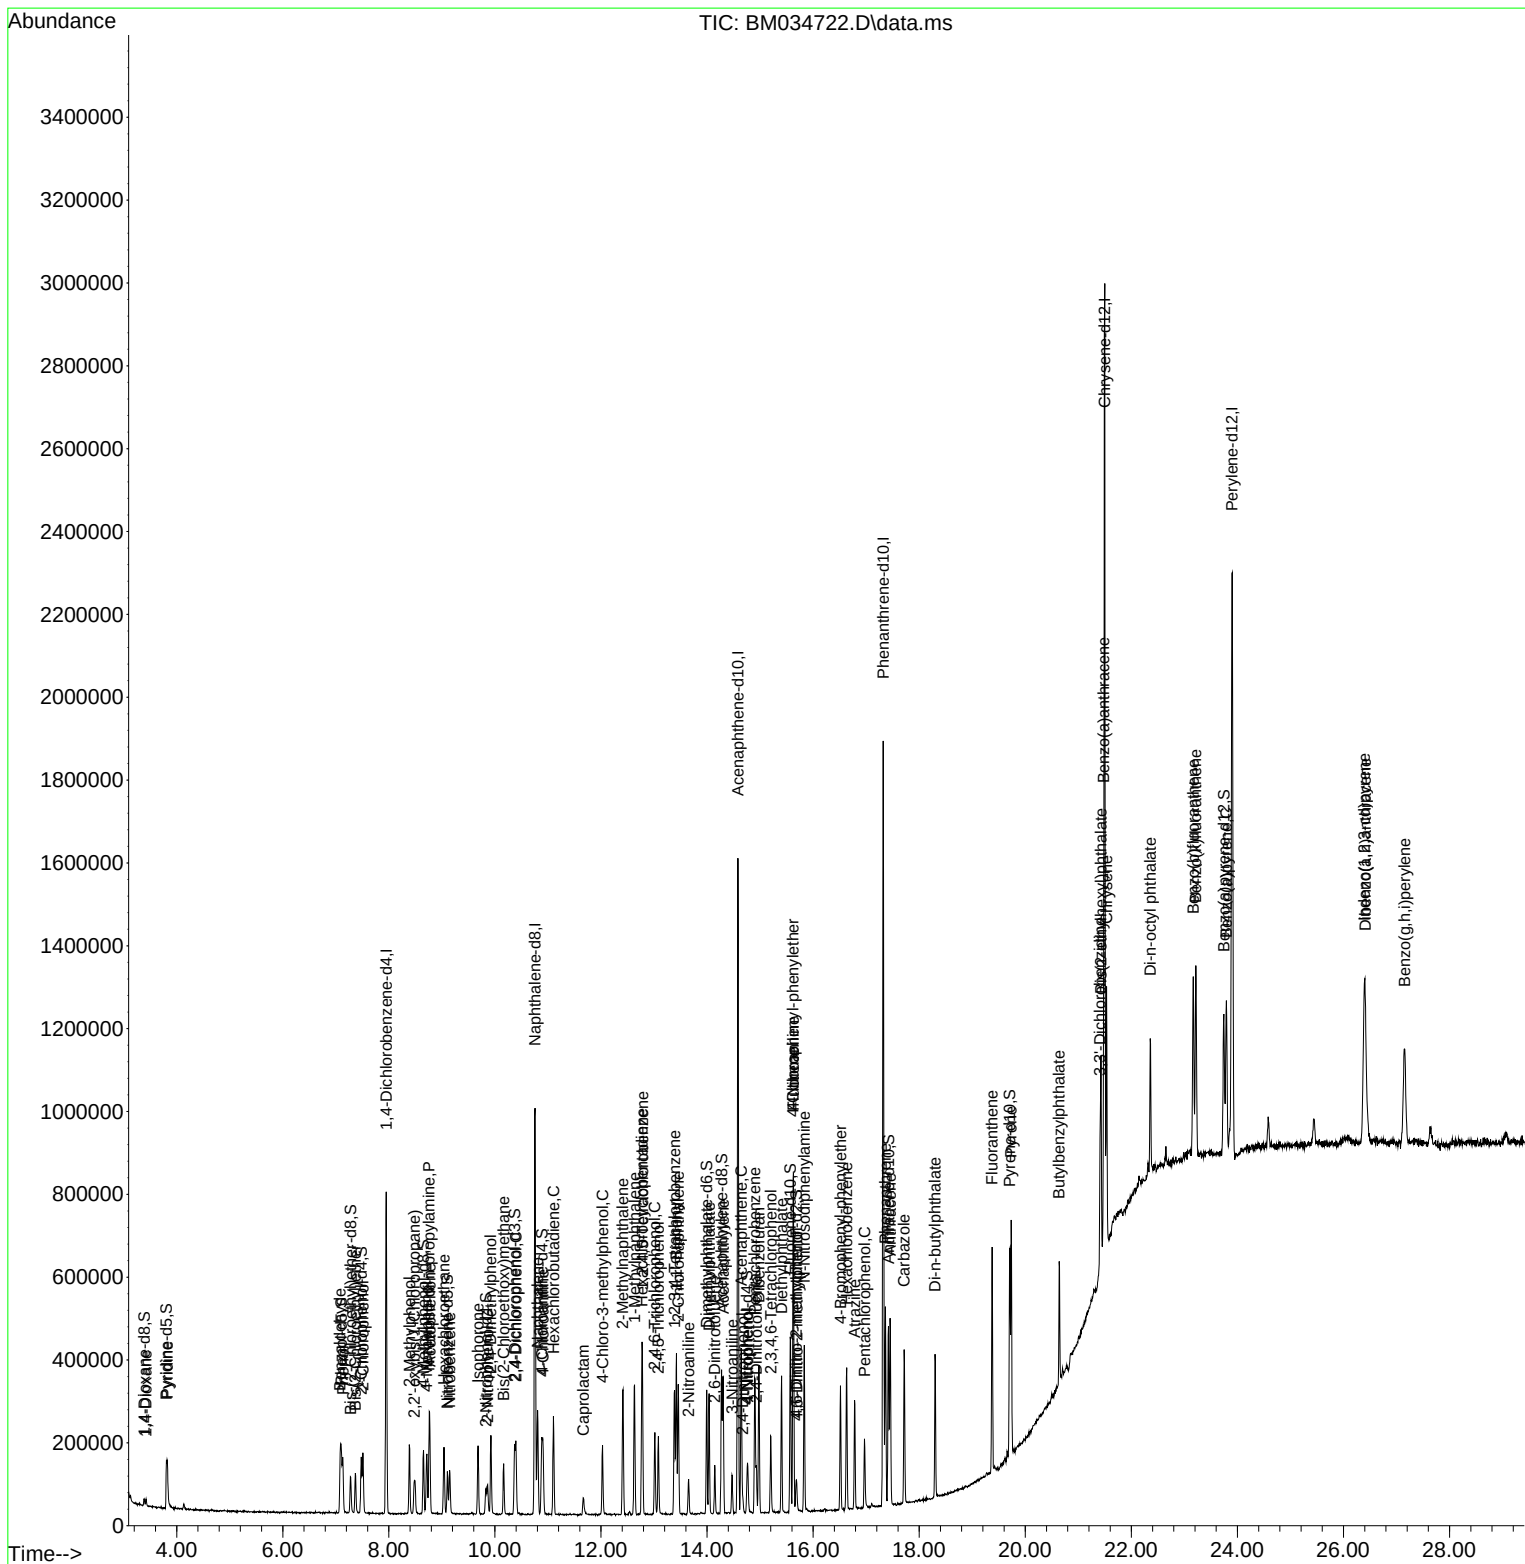




#2
1,4-Dioxane
Concen: 1.390 ng/uL
RT: 3.422 min Scan# 51
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion: 88 Resp: 9082
Ion Ratio Lower Upper
88 100
43 28.0 21.0 31.6
58 57.5 47.8 71.8

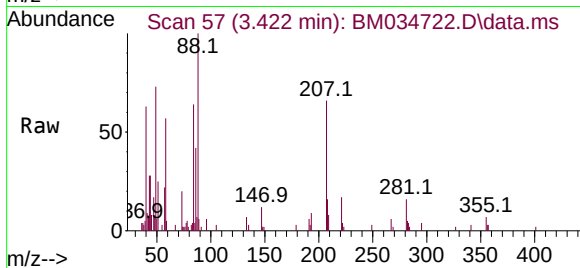

#5
Pyridine
Concen: 3.373 ng/uL
RT: 3.822 min Scan# 125
Delta R.T. 0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion: 79 Resp: 53115
Ion Ratio Lower Upper
79 100
52 71.4 47.7 71.5
51 40.4 25.6 38.4




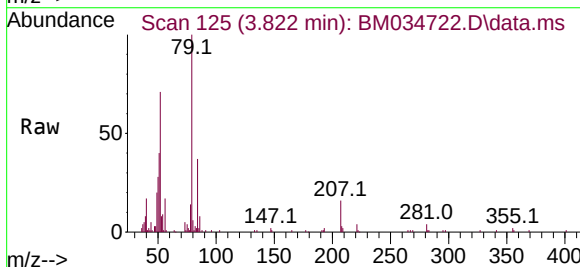




#6
Benzaldehyde
Concen: 4.466 ng/ul
RT: 7.081 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion: 77 Resp: 46843
Ion Ratio Lower Upper
77 100
105 96.4 80.8 121.2
106 91.3 76.6 115.0

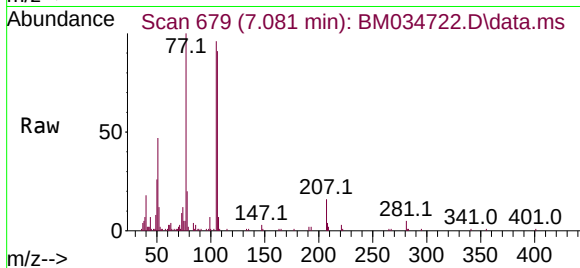

#8
Phenol
Concen: 3.559 ng/ul
RT: 7.134 min Scan# 688
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion: 94 Resp: 70047
Ion Ratio Lower Upper
94 100
65 27.5 22.9 34.3
66 38.8 33.7 50.5




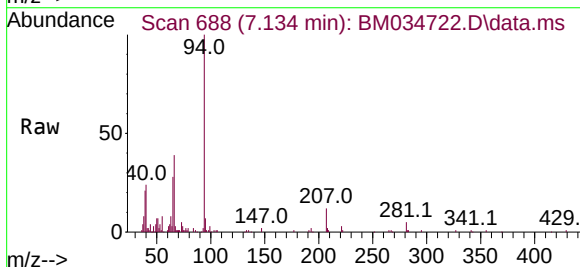




#10
 Bis(2-Chloroethyl)ether
 Concen: 3.368 ng/ul
 RT: 7.369 min Scan# 728
 Delta R.T. -0.000 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37




Instrument :
 BNA_M
 ClientSampleId :
 SSTD005018


Tgt Ion: 93	Resp:	54003
Ion	Ratio	Lower Upper
93	100	
63	69.5	54.7 82.1
95	33.8	26.6 39.8

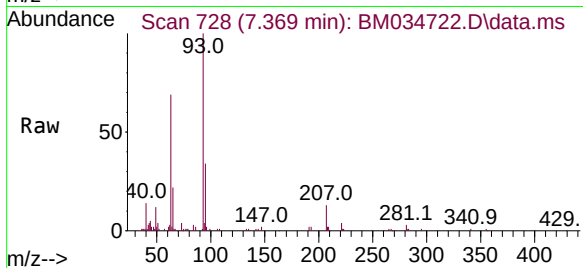

#12
 2-Chlorophenol
 Concen: 4.208 ng/ul
 RT: 7.510 min Scan# 752
 Delta R.T. -0.000 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37

Tgt Ion: 128	Resp:	64814
Ion	Ratio	Lower Upper
128	100	
64	37.7	30.6 46.0
130	31.2	25.8 38.6




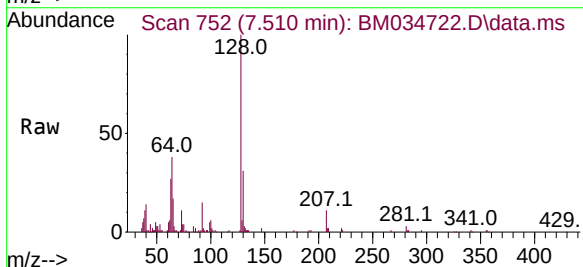




#13
2-Methylphenol
Concen: 3.654 ng/ul
RT: 8.392 min Scan# 902
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:108 Resp: 54140
Ion Ratio Lower Upper
108 100
107 89.3 71.9 107.9

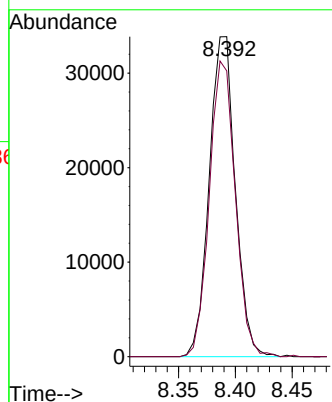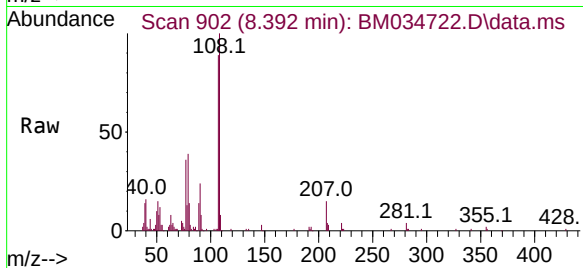

#14
2,2'-oxybis(1-Chloropropane)
Concen: 2.484 ng/ul
RT: 8.481 min Scan# 917
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion: 45 Resp: 63717
Ion Ratio Lower Upper
45 100
77 17.1 17.1 25.7#
79 11.5 12.8 19.2#



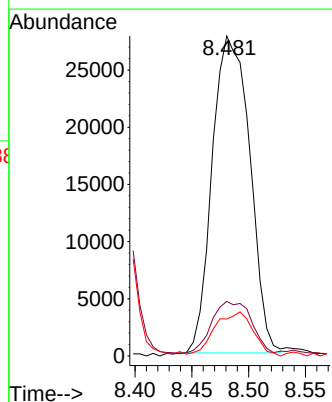
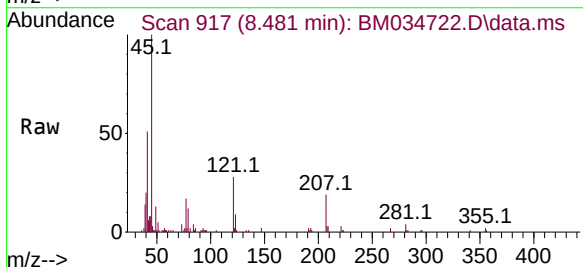




#16
Acetophenone
Concen: 3.879 ng/ul
RT: 8.775 min Scan# 967
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:105 Resp: 95108
Ion Ratio Lower Upper
105 100
77 70.6 59.4 89.2
51 24.5 19.3 28.9



#17
N-Nitroso-di-n-propylamine
Concen: 3.103 ng/ul
RT: 8.757 min Scan# 964
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion: 70 Resp: 40871
Ion Ratio Lower Upper
70 100
42 57.1 40.6 60.8
101 10.8 8.2 12.2
130 26.8 19.9 29.9



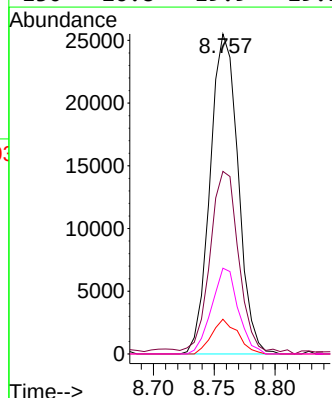





#18
4-Methylphenol
Concen: 3.669 ng/ul
RT: 8.716 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:108 Resp: 58386
Ion Ratio Lower Upper
108 100
107 112.2 89.0 133.4

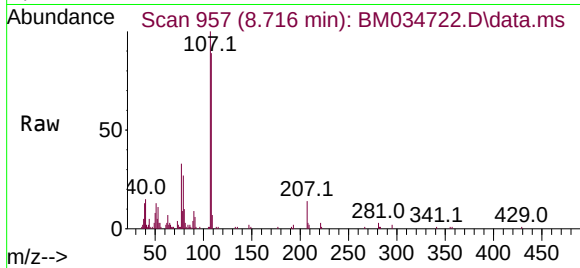

#19
Hexachloroethane
Concen: 3.914 ng/ul
RT: 9.039 min Scan# 1012
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:117 Resp: 26978
Ion Ratio Lower Upper
117 100
201 123.8 89.9 134.9
199 76.4 57.2 85.8




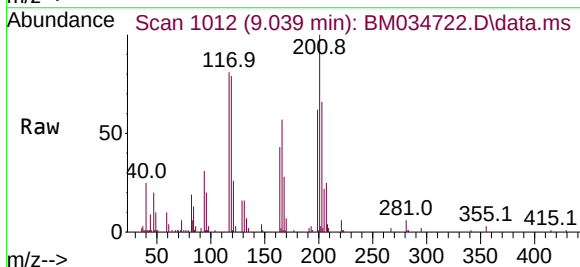




#22
Nitrobenzene
Concen: 3.146 ng/ul
RT: 9.145 min Scan# 1030
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion: 77 Resp: 53896
Ion Ratio Lower Upper
77 100
123 50.4 38.2 57.2
65 12.0 10.6 15.8



#23
Isophorone
Concen: 3.598 ng/ul
RT: 9.681 min Scan# 1121
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion: 82 Resp: 113074
Ion Ratio Lower Upper
82 100
95 7.3 6.8 10.2
138 20.6 16.5 24.7




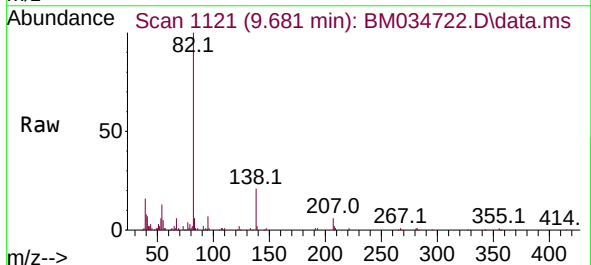




#25
2-Nitrophenol
Concen: 3.274 ng/ul
RT: 9.863 min Scan# 1152
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:139 Resp: 24315
Ion Ratio Lower Upper
139 100
65 42.5 37.8 56.6
109 30.8 26.5 39.7



#26
2,4-Dimethylphenol
Concen: 4.199 ng/ul
RT: 9.922 min Scan# 1162
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:107 Resp: 67840
Ion Ratio Lower Upper
107 100
121 49.9 40.8 61.2
122 85.2 69.0 103.6









#27
 Bis(2-Chloroethoxy)methane
 Concen: 3.842 ng/ul
 RT: 10.163 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37




Instrument :
 BNA_M
 ClientSampleId :
 SST005018


Tgt Ion:	93	Resp:	71192
Ion	Ratio	Lower	Upper
93	100		
95	32.7	25.4	38.2
123	11.5	9.5	14.3

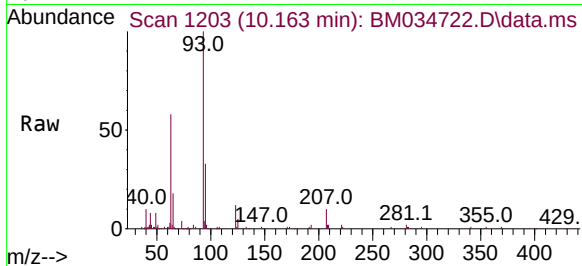

#29
 2,4-Dichlorophenol
 Concen: 5.157 ng/ul
 RT: 10.398 min Scan# 1243
 Delta R.T. -0.000 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37

Tgt Ion:	162	Resp:	63200
Ion	Ratio	Lower	Upper
162	100		
164	67.7	52.8	79.2
98	30.8	26.0	39.0




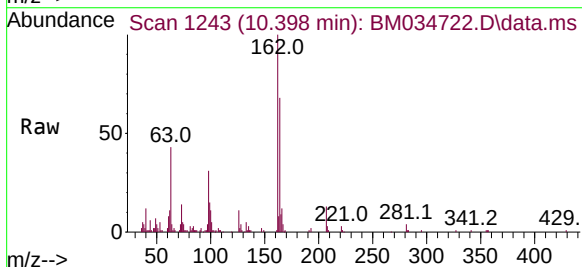




#30
Naphthalene
Concen: 4.625 ng/ul
RT: 10.804 min Scan# 11
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:128 Resp: 210704
Ion Ratio Lower Upper
128 100
129 11.1 8.7 13.1
127 13.1 9.9 14.9

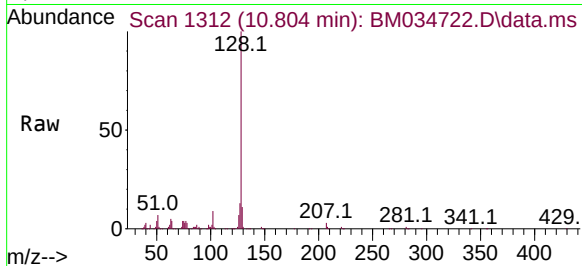

#32
4-Chloroaniline
Concen: 4.766 ng/ul
RT: 10.904 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:127 Resp: 82839
Ion Ratio Lower Upper
127 100
129 31.9 25.1 37.7

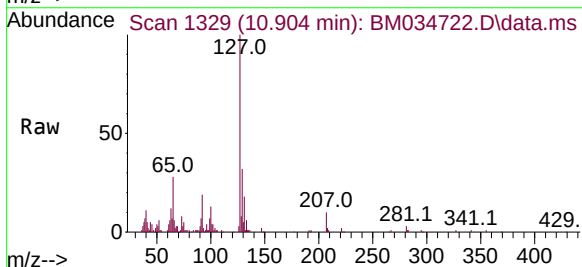



#33

Hexachlorobutadiene

Concen: 6.393 ng/ul

RT: 11.104 min Scan# 11

Delta R.T. -0.000 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37

Instrument :

BNA_M

ClientSampleId :

SSTD005018





Tgt Ion:225 Resp: 54205

Ion Ratio Lower Upper

225 100

223 60.3 50.6 75.8

227 64.1 50.3 75.5

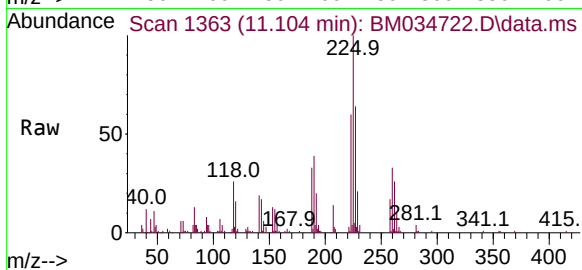

#34

Caprolactam

Concen: 4.496 ng/ul

RT: 11.669 min Scan# 1459

Delta R.T. -0.006 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37




Tgt Ion:113 Resp: 12297


Ion Ratio Lower Upper

113 100

55 126.4 100.9 151.3

56 99.7 81.0 121.4


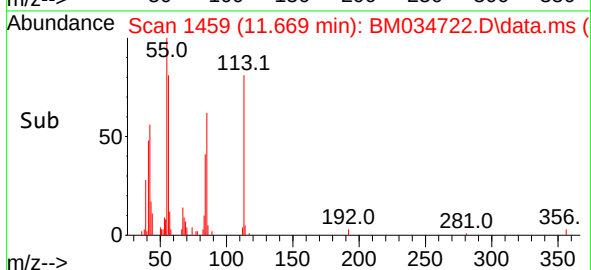

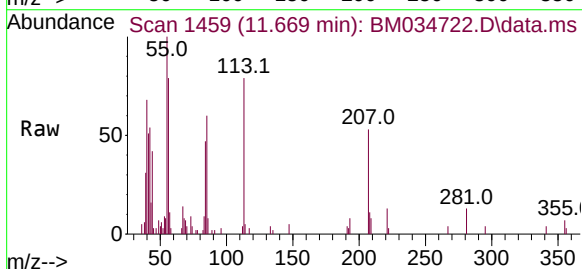




#35
 4-Chloro-3-methylphenol
 Concen: 4.326 ng/ul
 RT: 12.027 min Scan# 1520
 Delta R.T. -0.000 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37




Instrument :
 BNA_M
 ClientSampleId :
 SST005018


Tgt Ion:107 Resp: 58088
 Ion Ratio Lower Upper
 107 100
 144 27.6 23.0 34.4
 142 83.4 69.8 104.8

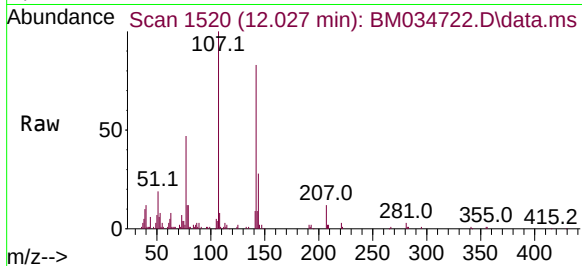

#36
 2-Methylnaphthalene
 Concen: 4.989 ng/ul
 RT: 12.410 min Scan# 1585
 Delta R.T. -0.006 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37

Tgt Ion:142 Resp: 147562
 Ion Ratio Lower Upper
 142 100
 141 88.9 71.4 107.0

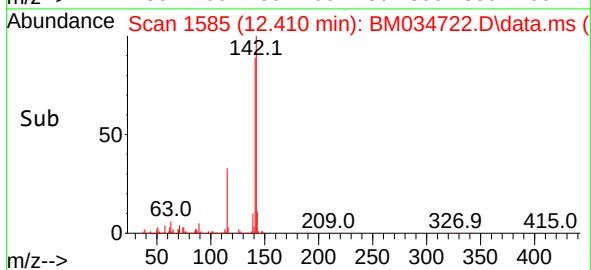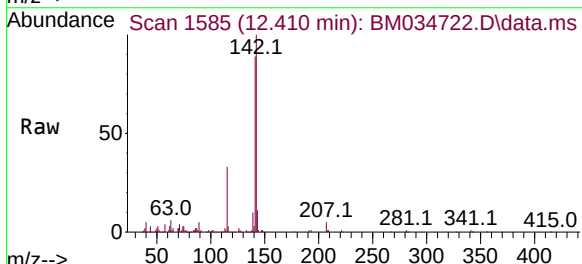



#37

1-Methylnaphthalene

Concen: 4.947 ng/ul

RT: 12.633 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37

Instrument :

BNA_M

ClientSampleId :

SSTD005018





Tgt Ion:142 Resp: 149623

Ion Ratio Lower Upper

142 100

141 93.5 74.5 111.7

116 3.6 3.0 4.6

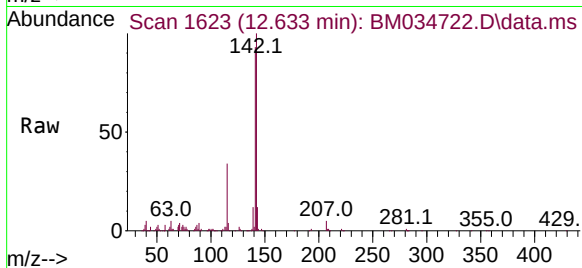

#39

1,2,4,5-Tetrachlorobenzene

Concen: 6.060 ng/ul

RT: 12.780 min Scan# 1648

Delta R.T. -0.000 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37

Tgt Ion:216 Resp: 99159




Ion Ratio Lower Upper


216 100

214 76.0 62.2 93.2

179 19.6 15.4 23.2

108 12.9 11.8 17.6


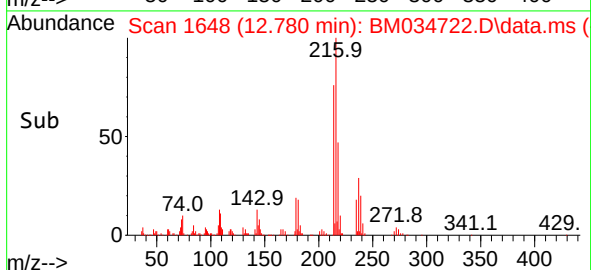

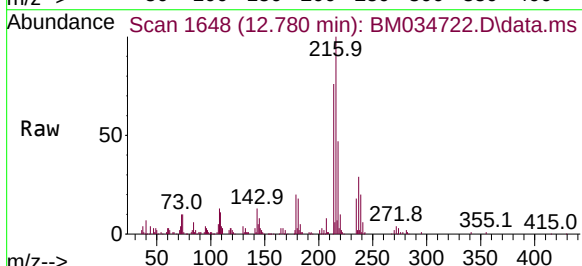




#40
Hexachlorocyclopentadiene
Concen: 5.234 ng/ul
RT: 12.769 min Scan# 1646
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:237 Resp: 53954
Ion Ratio Lower Upper
237 100
235 61.3 52.9 79.3
272 15.1 11.8 17.8

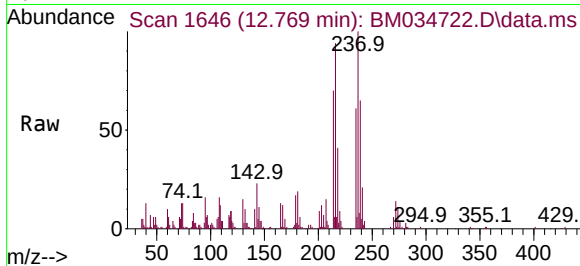

#41
2,4,6-Trichlorophenol
Concen: 4.936 ng/ul
RT: 13.016 min Scan# 1688
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:196 Resp: 50013
Ion Ratio Lower Upper
196 100
198 97.7 80.8 121.2
200 31.4 26.5 39.7


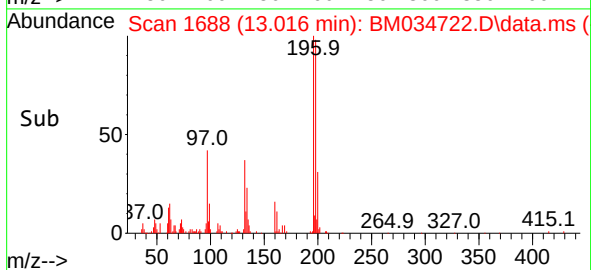

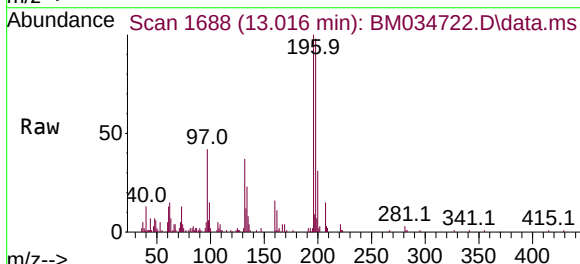




#42
2,4,5-Trichlorophenol
Concen: 5.251 ng/ul
RT: 13.080 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:196 Resp: 53281
Ion Ratio Lower Upper
196 100
198 100.0 78.0 117.0
200 30.8 24.5 36.7



#43
1,1'-Biphenyl
Concen: 4.794 ng/ul
RT: 13.421 min Scan# 1757
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:154 Resp: 206025
Ion Ratio Lower Upper
154 100
153 41.1 32.6 49.0
76 8.8 7.7 11.5




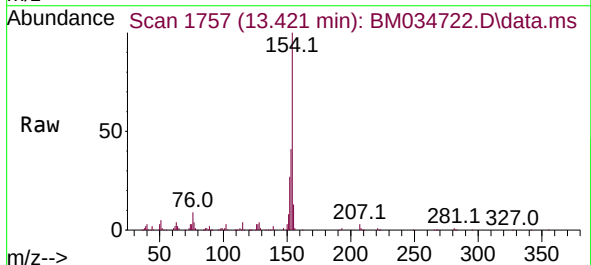




#44
2-Chloronaphthalene
Concen: 4.899 ng/ul
RT: 13.457 min Scan# 1763
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:162 Resp: 160760
Ion Ratio Lower Upper
162 100
164 32.7 26.6 40.0
127 37.9 29.6 44.4

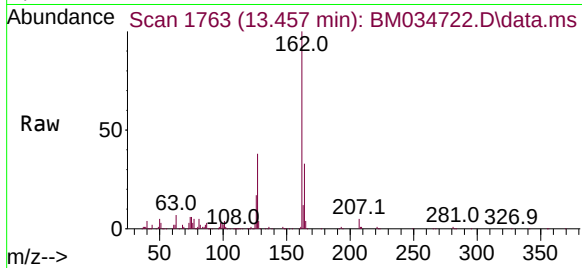

#45
2-Nitroaniline
Concen: 2.109 ng/ul
RT: 13.651 min Scan# 1796
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion: 65 Resp: 20317
Ion Ratio Lower Upper
65 100
92 75.6 57.4 86.2
138 125.7 94.8 142.2




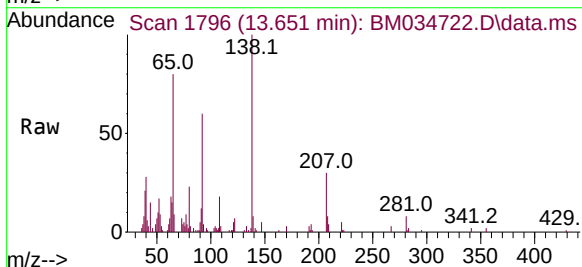




#47
Dimethylphthalate
Concen: 4.793 ng/ul
RT: 14.039 min Scan# 1862
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:163 Resp: 192397
Ion Ratio Lower Upper
163 100
194 4.9 3.4 5.2
164 10.2 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 3.023 ng/ul
RT: 14.145 min Scan# 1880
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:165 Resp: 23712
Ion Ratio Lower Upper
165 100
89 53.2 44.2 66.4
121 21.5 16.7 25.1


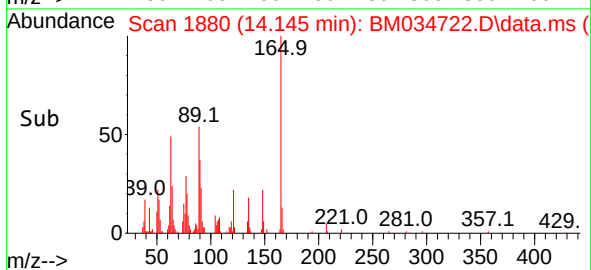






#50
Acenaphthylene
Concen: 4.629 ng/ul
RT: 14.304 min Scan# 1907
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:152 Resp: 247484
Ion Ratio Lower Upper
152 100
151 19.9 15.8 23.8
153 12.9 10.2 15.2



#51
3-Nitroaniline
Concen: 3.738 ng/ul
RT: 14.474 min Scan# 1936
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:138 Resp: 22148
Ion Ratio Lower Upper
138 100
108 23.7 8.3 12.5#
92 101.5 87.0 130.4




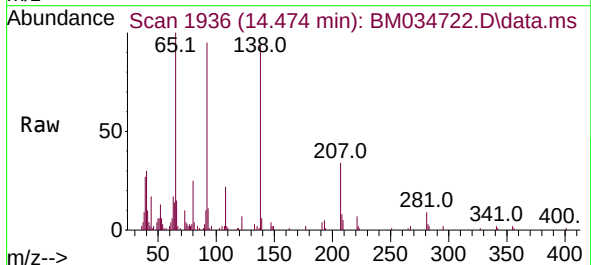




#52
Acenaphthene
Concen: 4.592 ng/ul
RT: 14.645 min Scan# 1965
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:153 Resp: 163675
Ion Ratio Lower Upper
153 100
152 47.1 37.4 56.0
154 90.8 71.0 106.4

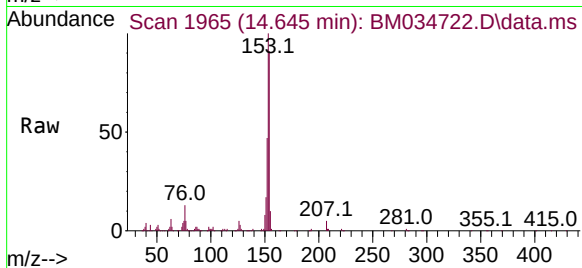

#53
2,4-Dinitrophenol
Concen: 2.736 ng/ul
RT: 14.674 min Scan# 1970
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:184 Resp: 9139
Ion Ratio Lower Upper
184 100
63 36.4 43.8 65.6#
154 55.8 49.9 74.9


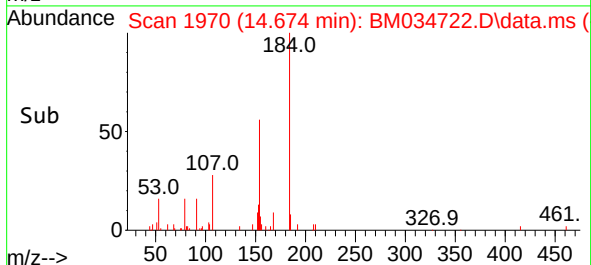
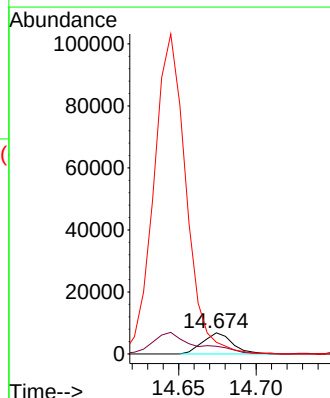
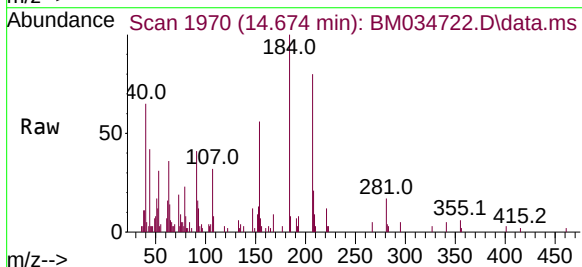




#55
4-Nitrophenol
Concen: 2.869 ng/ul
RT: 14.768 min Scan# 1986
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:109 Resp: 14746
Ion Ratio Lower Upper
109 100
139 152.7 94.6 142.0#
65 132.7 83.5 125.3#

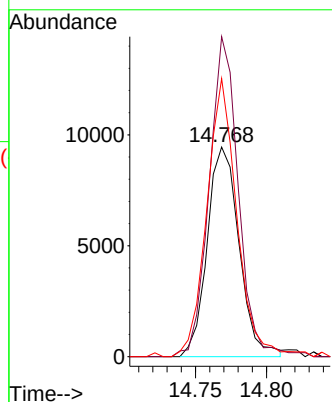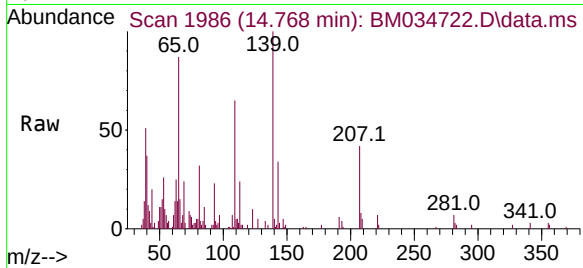

#56
Dibenzofuran
Concen: 4.986 ng/ul
RT: 14.980 min Scan# 2022
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:168 Resp: 242421
Ion Ratio Lower Upper
168 100
139 33.7 29.8 44.6




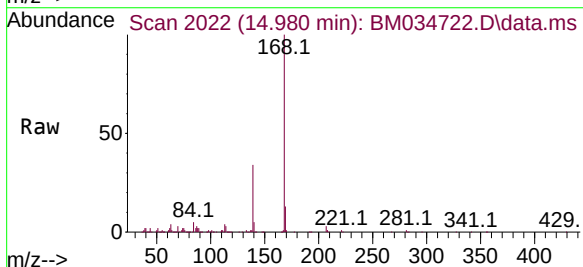




#57
2,4-Dinitrotoluene
Concen: 2.949 ng/ul
RT: 14.927 min Scan# 2013
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:165 Resp: 31655
Ion Ratio Lower Upper
165 100
63 36.8 30.2 45.4
182 4.5 2.2 3.2#

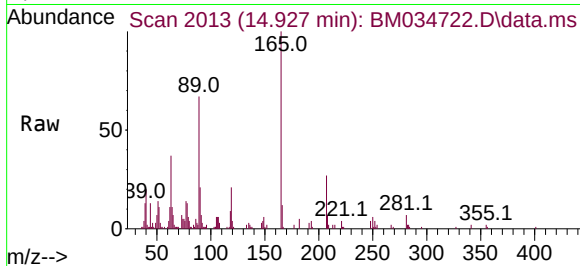

#58
2,3,4,6-Tetrachlorophenol
Concen: 4.977 ng/ul
RT: 15.204 min Scan# 2060
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:232 Resp: 43027
Ion Ratio Lower Upper
232 100
131 35.0 32.2 48.4
130 2.2 1.9 2.9
166 24.8 23.0 34.4




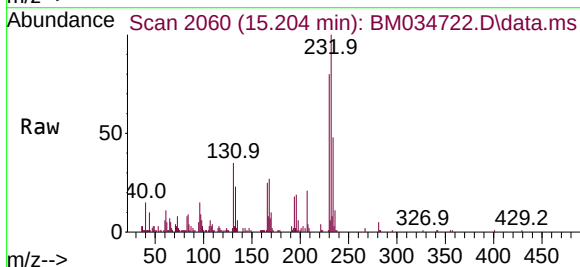




#59
Diethylphthalate
Concen: 4.330 ng/ul
RT: 15.404 min Scan# 2094
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:149 Resp: 178413
Ion Ratio Lower Upper
149 100
177 24.8 17.9 26.9
150 12.0 10.2 15.2

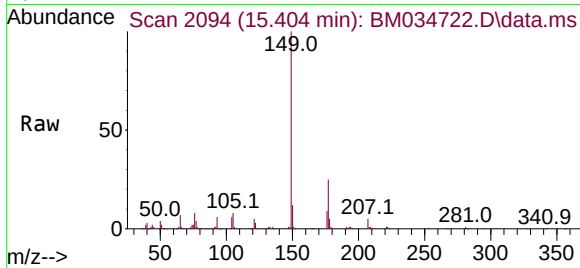

#61
Fluorene
Concen: 4.721 ng/ul
RT: 15.627 min Scan# 2132
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:166 Resp: 192483
Ion Ratio Lower Upper
166 100
165 99.1 76.9 115.3
167 13.5 10.8 16.2




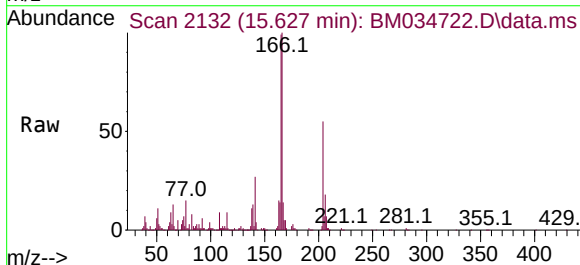




#62
4-Chlorophenyl-phenylether
Concen: 5.547 ng/ul
RT: 15.621 min Scan# 2131
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:204 Resp: 107540
Ion Ratio Lower Upper
204 100
206 33.0 25.5 38.3
141 54.1 44.2 66.2

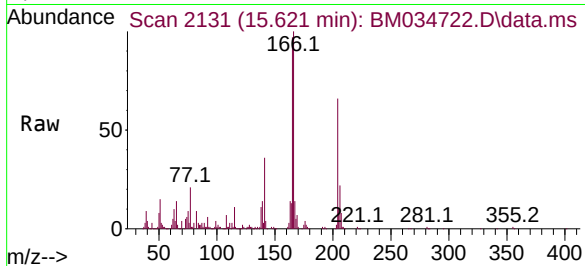

#63
4-Nitroaniline
Concen: 4.632 ng/ul
RT: 15.627 min Scan# 2132
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:138 Resp: 22975
Ion Ratio Lower Upper
138 100
92 50.8 36.3 54.5
108 76.2 68.9 103.3




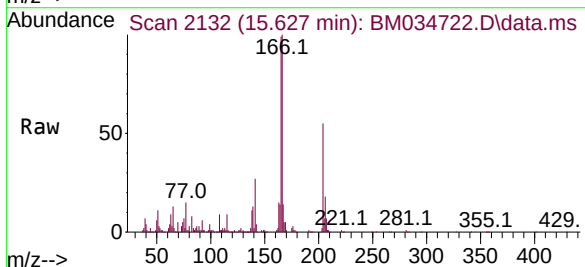




#66
 4,6-Dinitro-2-methylphenol
 Concen: 2.189 ng/ul
 RT: 15.692 min Scan# 2143
 Delta R.T. -0.000 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37




Instrument :
 BNA_M
 ClientSampleId :
 SSTD005018


Tgt Ion:198 Resp: 13889
 Ion Ratio Lower Upper
 198 100
 182 5.7 3.8 5.6#
 77 22.4 18.5 27.7

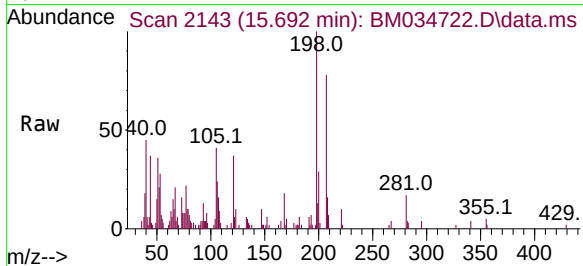

#67
 N-Nitrosodiphenylamine
 Concen: 4.567 ng/ul
 RT: 15.833 min Scan# 2167
 Delta R.T. -0.000 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37

Tgt Ion:169 Resp: 159256
 Ion Ratio Lower Upper
 169 100
 168 65.2 52.8 79.2
 167 36.6 28.1 42.1



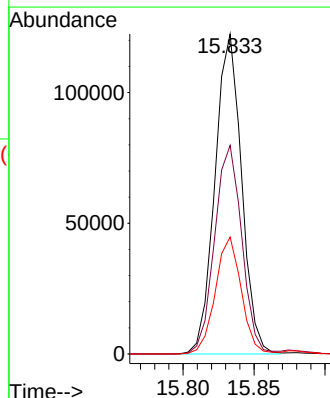
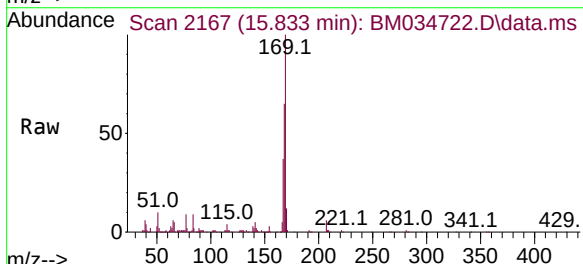




#68
4-Bromophenyl-phenylether
Concen: 5.540 ng/ul
RT: 16.515 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:248 Resp: 65348
Ion Ratio Lower Upper
248 100
250 99.3 78.4 117.6
141 61.6 51.4 77.2

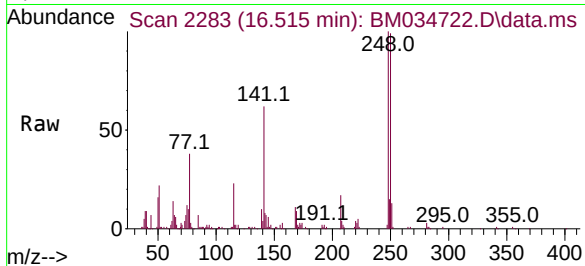

#69
Hexachlorobenzene
Concen: 5.651 ng/ul
RT: 16.633 min Scan# 2303
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:284 Resp: 79208
Ion Ratio Lower Upper
284 100
142 24.5 24.6 36.8#
249 30.4 24.1 36.1




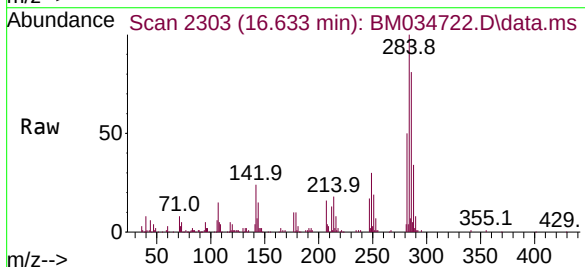




#70
 Atrazine
 Concen: 4.258 ng/ul
 RT: 16.780 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37




Instrument :
 BNA_M
 ClientSampleId :
 SSTD005018


Tgt Ion:200 Resp: 54808
 Ion Ratio Lower Upper
 200 100
 173 25.3 20.2 30.4
 215 49.4 38.4 57.6

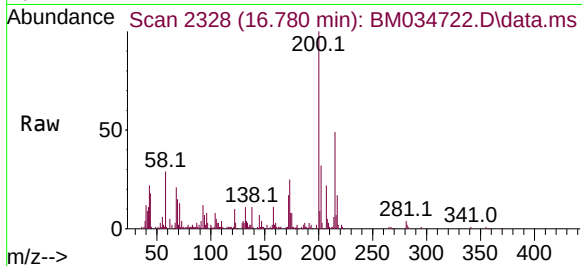

#71
 Pentachlorophenol
 Concen: 4.982 ng/ul
 RT: 16.968 min Scan# 2360
 Delta R.T. -0.000 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37

Tgt Ion:266 Resp: 33206
 Ion Ratio Lower Upper
 266 100
 264 66.2 49.3 73.9
 268 63.5 50.3 75.5

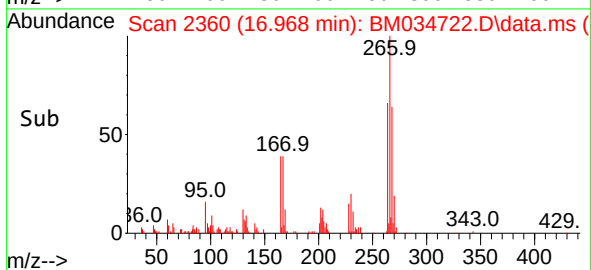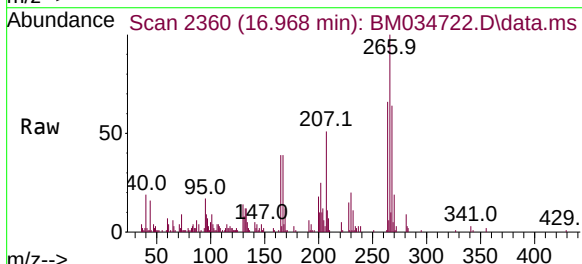



#72

Phenanthrene

Concen: 4.569 ng/ul

RT: 17.362 min Scan# 2427

Delta R.T. -0.000 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37

Instrument :

BNA_M

ClientSampleId :

SSTD005018





Tgt Ion:178 Resp: 294285

Ion Ratio Lower Upper

178 100

179 15.0 11.7 17.5

176 18.8 15.0 22.4

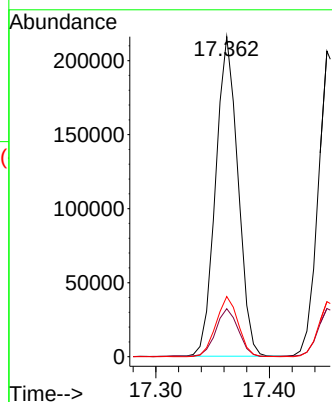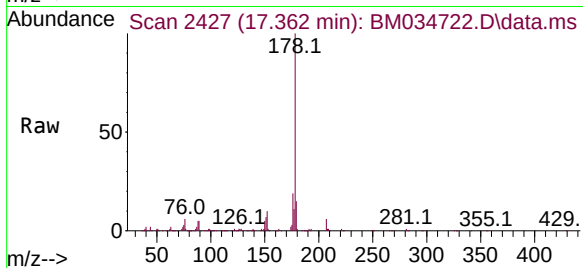

#74

Anthracene

Concen: 4.680 ng/ul

RT: 17.451 min Scan# 2442

Delta R.T. -0.006 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37




Tgt Ion:178 Resp: 293607


Ion Ratio Lower Upper

178 100

179 15.8 11.9 17.9

176 18.0 14.4 21.6




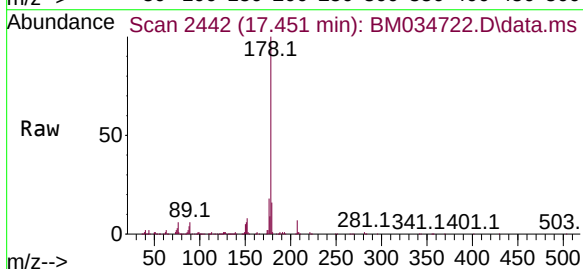




#75
1,2,3,4-Tetrachlorobenzene
Concen: 5.661 ng/uL
RT: 13.386 min Scan# 1
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:216 Resp: 101478
Ion Ratio Lower Upper
216 100
214 76.7 62.0 93.0
218 46.8 37.8 56.8

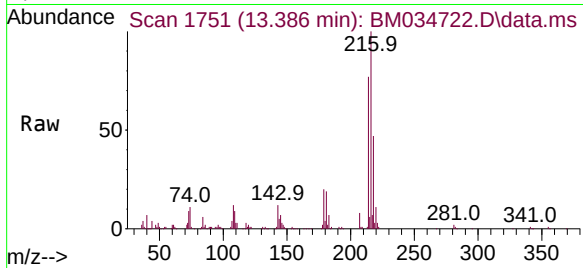

#76
Pentachlorobenzene
Concen: 5.767 ng/uL
RT: 14.898 min Scan# 2008
Delta R.T. -0.006 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:250 Resp: 97208
Ion Ratio Lower Upper
250 100
248 63.7 50.6 75.8
252 63.1 50.2 75.4


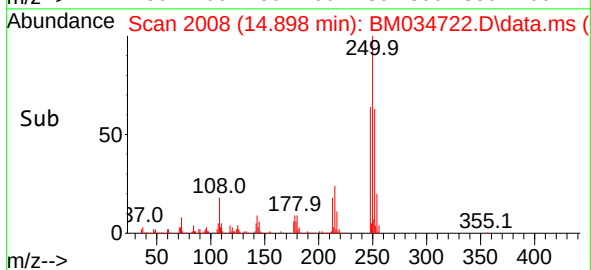

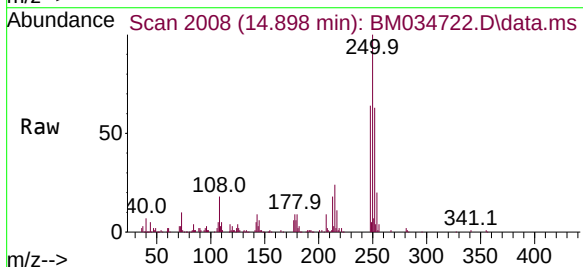




#77
 Carbazole
 Concen: 4.571 ng/ul
 RT: 17.715 min Scan# 2487
 Delta R.T. -0.006 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37




Instrument :
 BNA_M
 ClientSampleId :
 SSTD005018


Tgt Ion:167 Resp: 241782
 Ion Ratio Lower Upper
 167 100
 166 21.3 16.6 25.0
 139 11.7 9.9 14.9

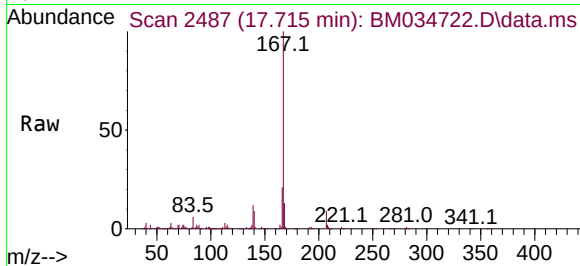

#78
 Di-n-butylphthalate
 Concen: 3.626 ng/ul
 RT: 18.298 min Scan# 2586
 Delta R.T. -0.006 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37

Tgt Ion:149 Resp: 249119
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.0
 104 5.2 4.2 6.2

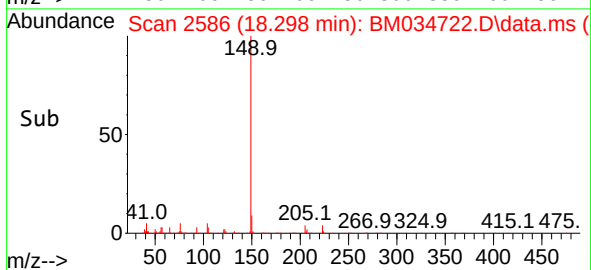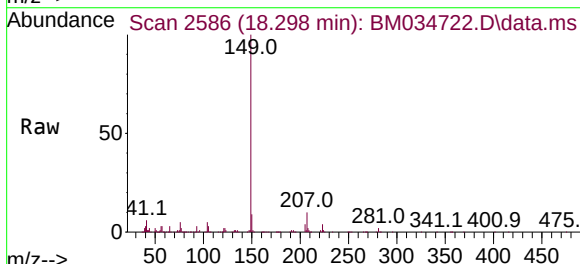



#80

Fluoranthene

Concen: 4.547 ng/ul

RT: 19.374 min Scan# 21

Delta R.T. -0.000 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37

Instrument :

BNA_M

ClientSampleId :

SSTD005018





Tgt Ion:202 Resp: 332262

Ion Ratio Lower Upper

202 100

101 7.7 6.2 9.2

100 5.6 4.7 7.1

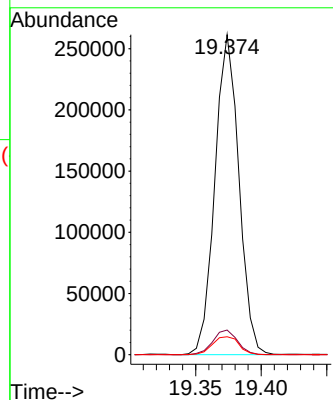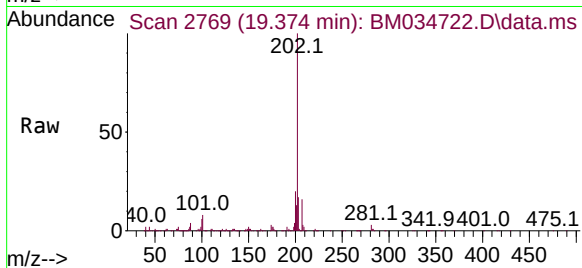

#82

Pyrene

Concen: 4.505 ng/ul

RT: 19.733 min Scan# 2830

Delta R.T. -0.006 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37




Tgt Ion:202 Resp: 346249


Ion Ratio Lower Upper

202 100

101 9.7 7.0 10.4

100 7.7 5.8 8.6


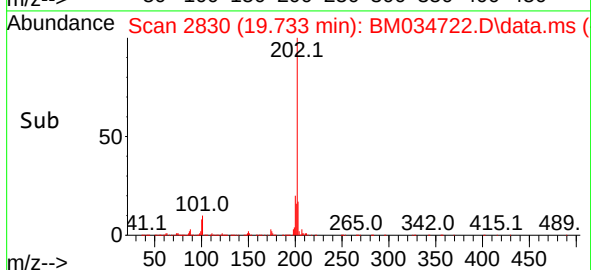
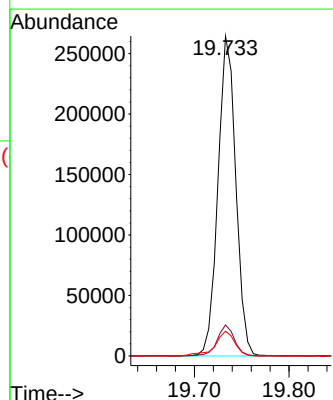
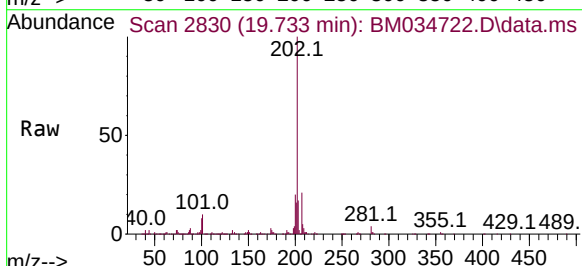




#83
 Butylbenzylphthalate
 Concen: 2.935 ng/ul
 RT: 20.639 min Scan# 2985
 Delta R.T. -0.006 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37




Instrument :
 BNA_M
 ClientSampleId :
 SSTD005018


Tgt Ion:149	Resp:	90607
Ion Ratio	Lower	Upper
149	100	
91	63.2	50.9 76.3
206	23.9	19.3 28.9

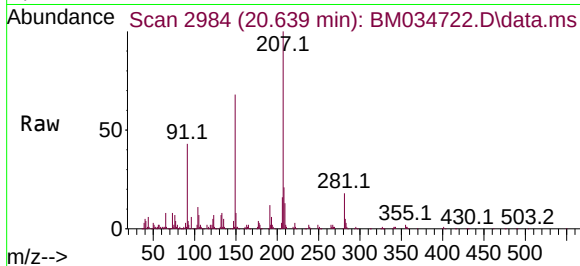

#84
 3,3'-Dichlorobenzidine
 Concen: 4.781 ng/ul
 RT: 21.409 min Scan# 3115
 Delta R.T. -0.000 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37

Tgt Ion:252	Resp:	96233
Ion Ratio	Lower	Upper
252	100	
254	64.3	50.7 76.1
126	9.3	6.6 9.8



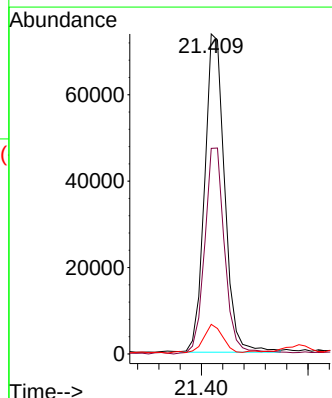
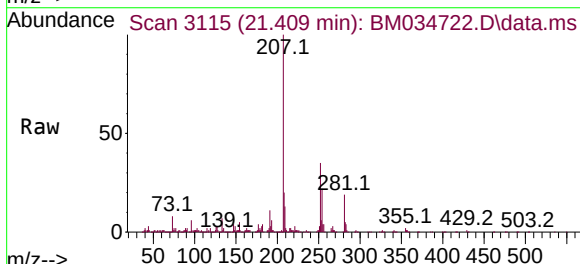




#85
Benzo(a)anthracene
Concen: 4.953 ng/ul
RT: 21.480 min Scan# 3127
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:228 Resp: 330419
Ion Ratio Lower Upper
228 100
229 20.1 15.4 23.2
226 25.4 21.0 31.4

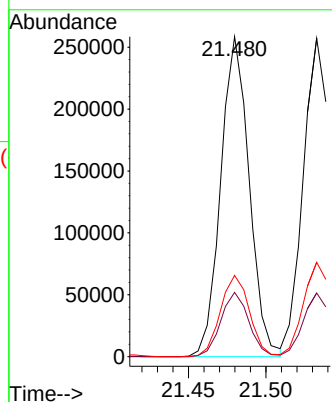

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.225 ng/ul
RT: 21.427 min Scan# 3118
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:149 Resp: 148037
Ion Ratio Lower Upper
149 100
167 29.0 22.1 33.1
279 5.7 4.2 6.2

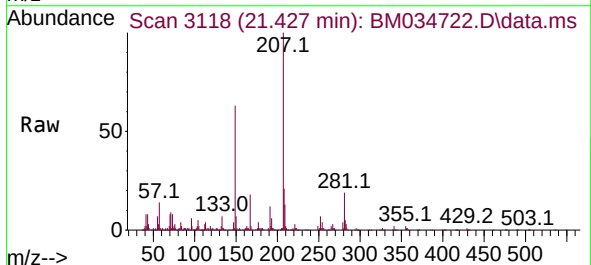



#87

Chrysene

Concen: 4.539 ng/ul

RT: 21.533 min Scan# 3136

Delta R.T. -0.000 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37

Instrument :

BNA_M

ClientSampleId :

SSTD005018





Tgt Ion:228 Resp: 322196

Ion Ratio Lower Upper

228 100

226 29.6 23.4 35.2

229 20.0 15.4 23.0



#89

Di-n-octyl phthalate

Concen: 2.902 ng/ul




RT: 22.356 min Scan# 3276


Delta R.T. -0.000 min

Lab File: BM034722.D

Acq: 20 Apr 2022 09:37

Tgt Ion:149 Resp: 235212









#90
Benzo(b)fluoranthene
Concen: 4.762 ng/ul
RT: 23.168 min Scan# 3414
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:252 Resp: 330212
Ion Ratio Lower Upper
252 100
253 22.0 17.4 26.0
125 7.9 5.8 8.6



#91
Benzo(k)fluoranthene
Concen: 4.444 ng/ul
RT: 23.215 min Scan# 3422
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:252 Resp: 311704
Ion Ratio Lower Upper
252 100
253 22.5 17.5 26.3
125 8.0 5.1 7.7#




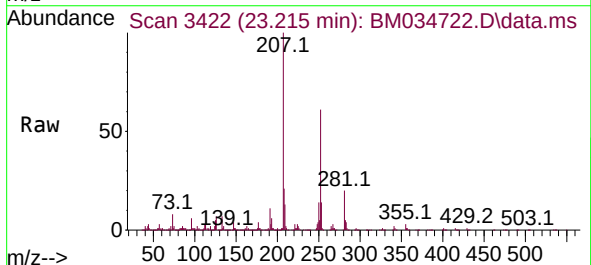




#93
Benzo(a)pyrene
Concen: 4.499 ng/ul
RT: 23.791 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37




Instrument :
BNA_M
ClientSampleId :
SSTD005018


Tgt Ion:252 Resp: 310819
Ion Ratio Lower Upper
252 100
253 22.5 17.5 26.3
125 8.7 6.2 9.4



#94
Indeno(1,2,3-cd)pyrene
Concen: 4.860 ng/ul
RT: 26.391 min Scan# 3962
Delta R.T. -0.000 min
Lab File: BM034722.D
Acq: 20 Apr 2022 09:37

Tgt Ion:276 Resp: 367344
Ion Ratio Lower Upper
276 100
138 17.5 13.6 20.4
277 23.9 19.9 29.9




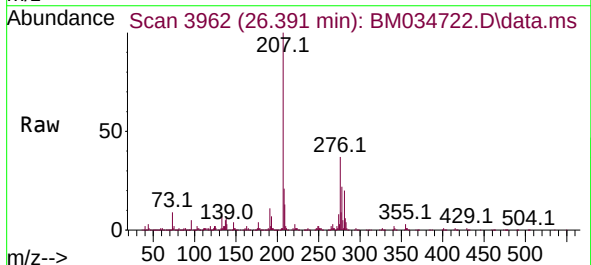




#95
 Dibenzo(a,h)anthracene
 Concen: 5.288 ng/ul
 RT: 26.409 min Scan# 3966
 Delta R.T. -0.006 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37

Instrument :
 BNA_M
 ClientSampleId :
 SSTD005018

Tgt Ion:278 Resp: 313637
 Ion Ratio Lower Upper
 278 100
 139 12.5 9.6 14.4
 279 23.6 19.3 28.9



#96
 Benzo(g,h,i)perylene
 Concen: 4.665 ng/ul
 RT: 27.150 min Scan# 4091
 Delta R.T. -0.006 min
 Lab File: BM034722.D
 Acq: 20 Apr 2022 09:37

Tgt Ion:276 Resp: 319048
 Ion Ratio Lower Upper
 276 100
 138 16.6 11.8 17.6
 277 23.5 18.8 28.2

