




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
Data File : BM039522.D  
Acq On : 20 Apr 2023 12:11  
Operator : CG/JU  
Sample : 02296-14DL3 60X  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:36:53 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Apr 19 08:18:41 2023  
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
Supervised By :Jagrut Upadhyay 04/21/2023

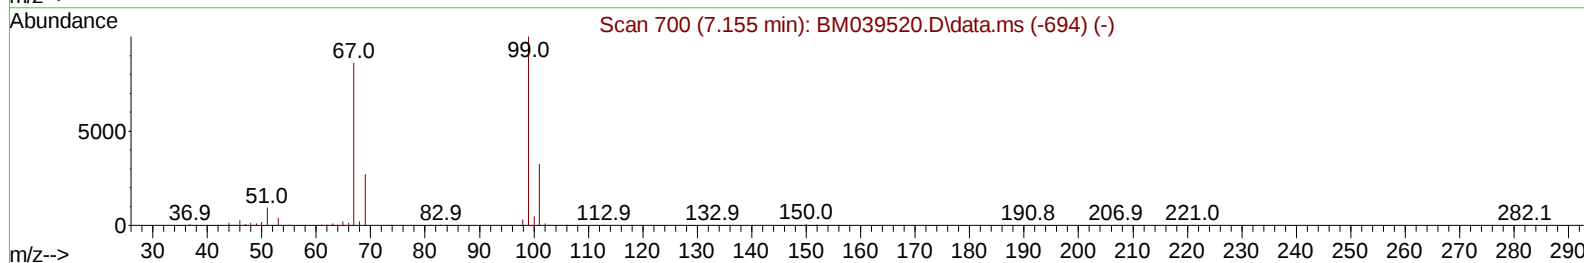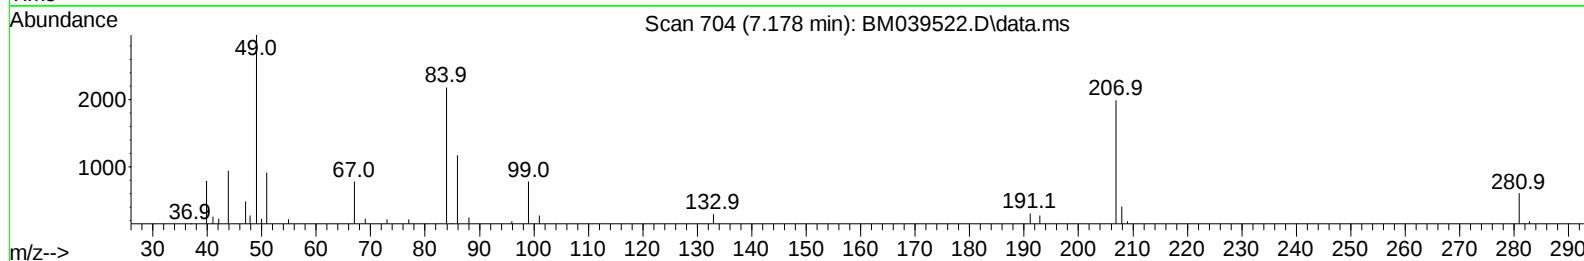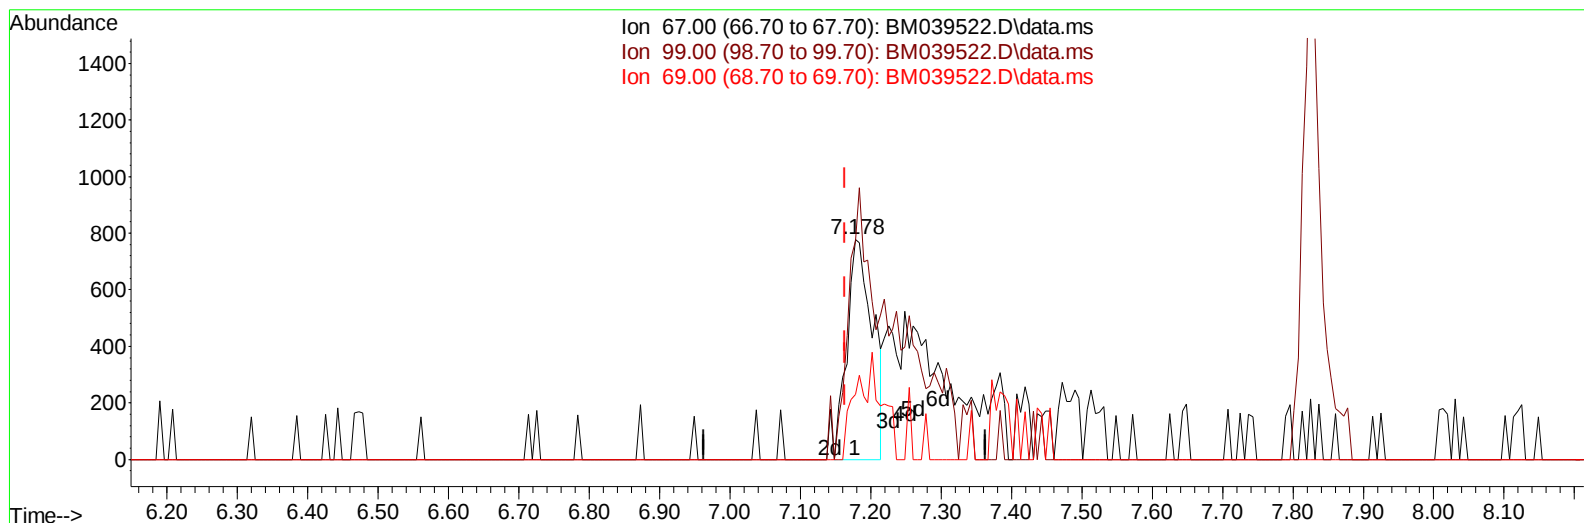

TIC: BM039522.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.178min (+ 0.015) 0.16 ng/u1

response 1941

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 67.00 | 100.00 | 100.00 |
| 99.00 | 117.70 | 99.49  |
| 69.00 | 30.90  | 29.43  |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
 Data File : BM039522.D  
 Acq On : 20 Apr 2023 12:11  
 Operator : CG/JU  
 Sample : 02296-14DL3 60X  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:36:53 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Apr 19 08:18:41 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
 Supervised By :Jagrut Upadhyay 04/21/2023

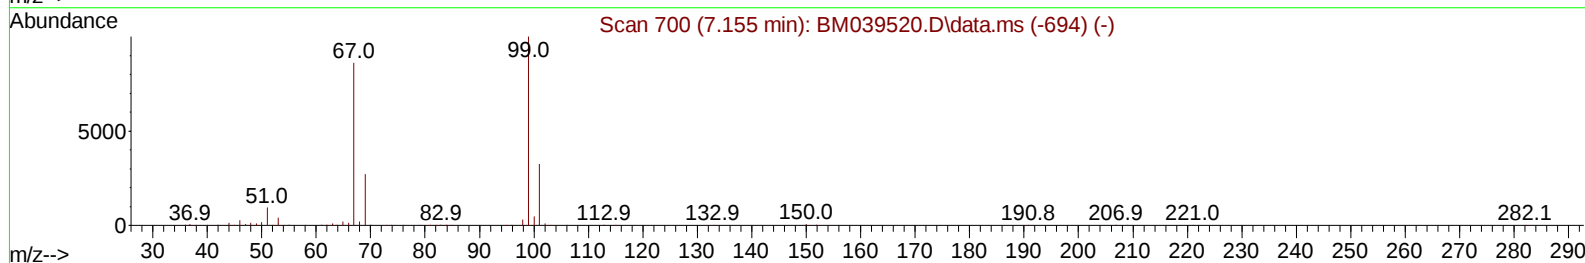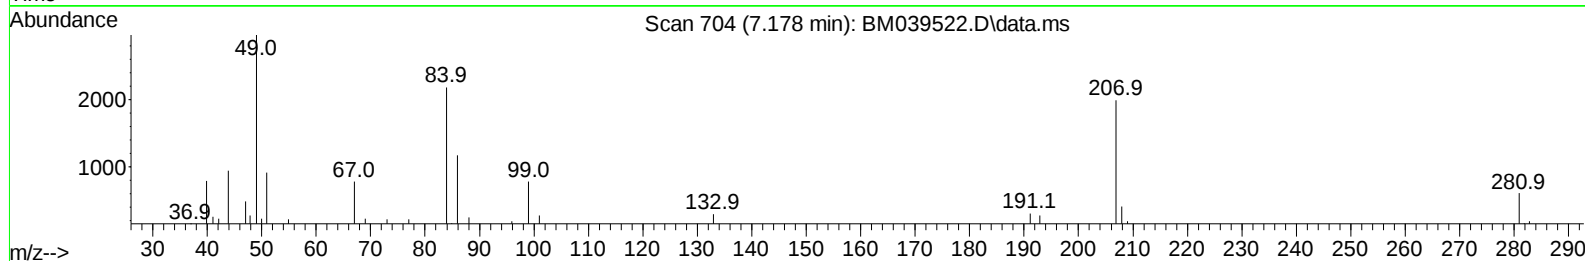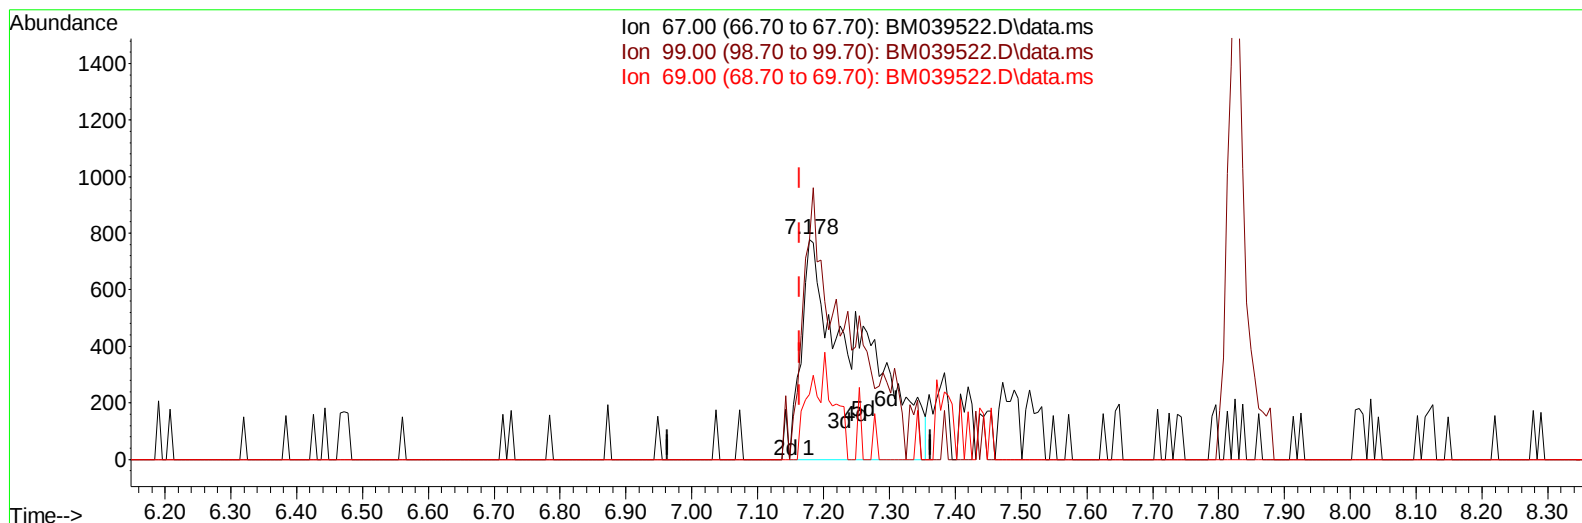

TIC: BM039522.D\data.ms

**(9) Bis-(2-Chloroethyl)ether-d8 (S)**

7.178min (+ 0.015) 0.38 ng/ul m

response 4691

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 67.00 | 100.00 | 100.00 |
| 99.00 | 117.70 | 99.49  |
| 69.00 | 30.90  | 29.43  |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
Data File : BM039522.D  
Acq On : 20 Apr 2023 12:11  
Operator : CG/JU  
Sample : 02296-14DL3 60X  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DCBL8DL3

## Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/21/2023  
Supervised By :Jagrut Upadhyay 04/21/2023

Quant Time: Apr 21 00:45:03 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Apr 19 08:18:41 2023  
Response via : Initial Calibration

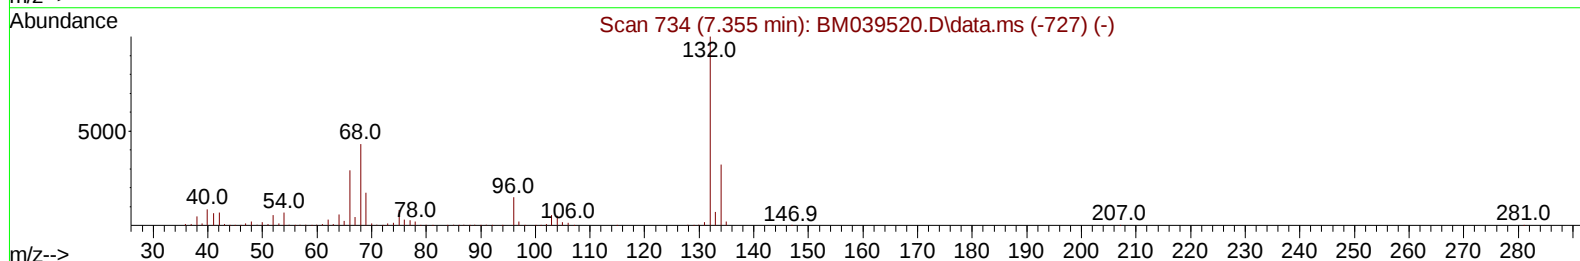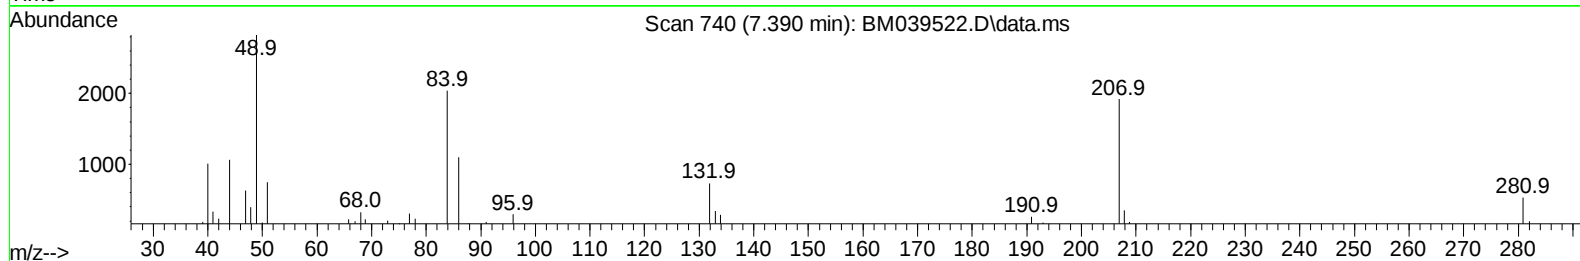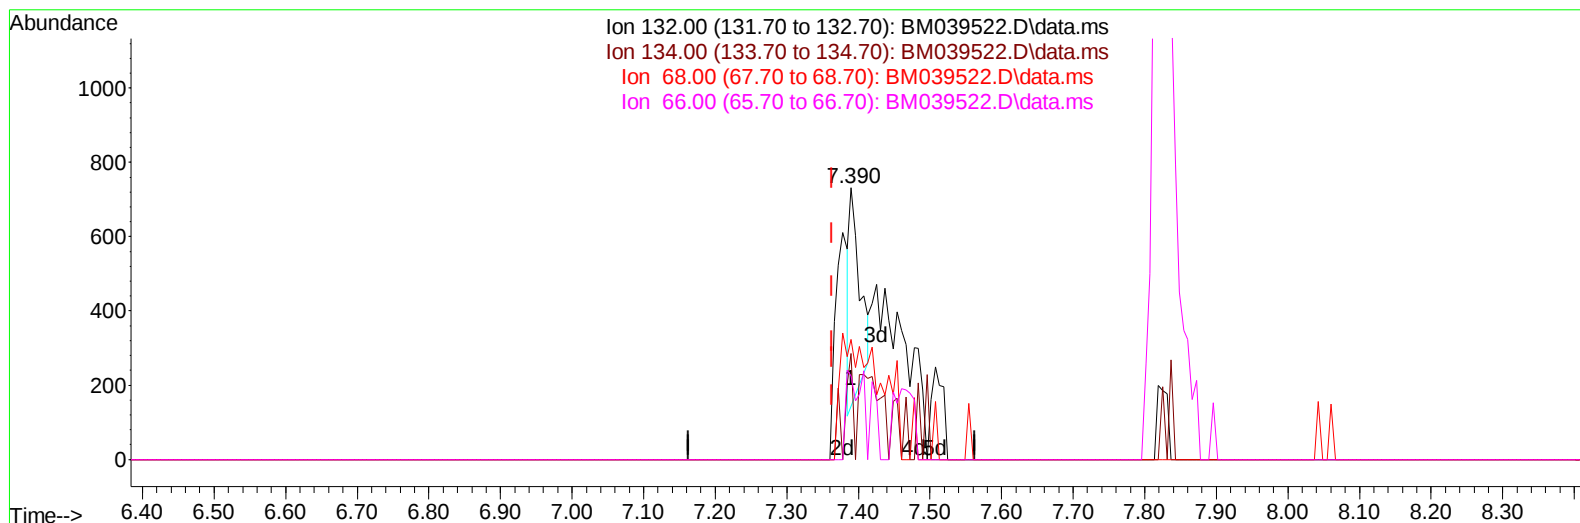

TIC: BM039522.D\data.ms

## (11) 2-Chloropheno1-d4 (S)

7.390min (+ 0.027) 0.04 ng/u1

response 582

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 132.00 | 100.00 | 100.00 |
| 134.00 | 33.00  | 39.12  |
| 68.00  | 42.40  | 44.19  |
| 66.00  | 29.00  | 30.78  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
Data File : BM039522.D  
Acq On : 20 Apr 2023 12:11  
Operator : CG/JU  
Sample : 02296-14DL3 60X  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DCBL8DL3

## Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/21/2023  
Supervised By :Jagrut Upadhyay 04/21/2023

Quant Time: Apr 21 00:45:03 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Apr 19 08:18:41 2023  
Response via : Initial Calibration

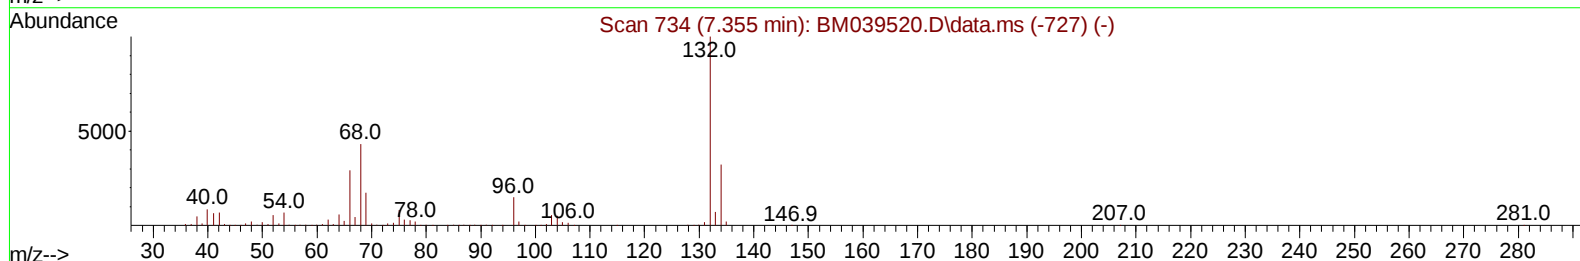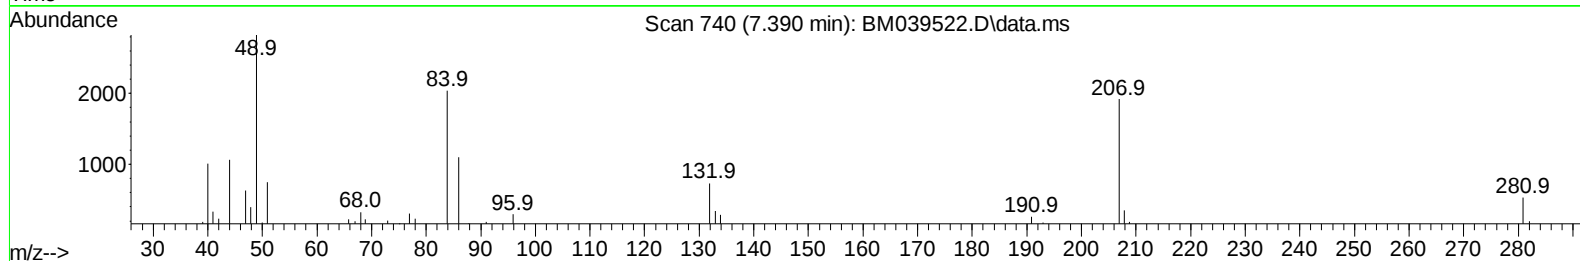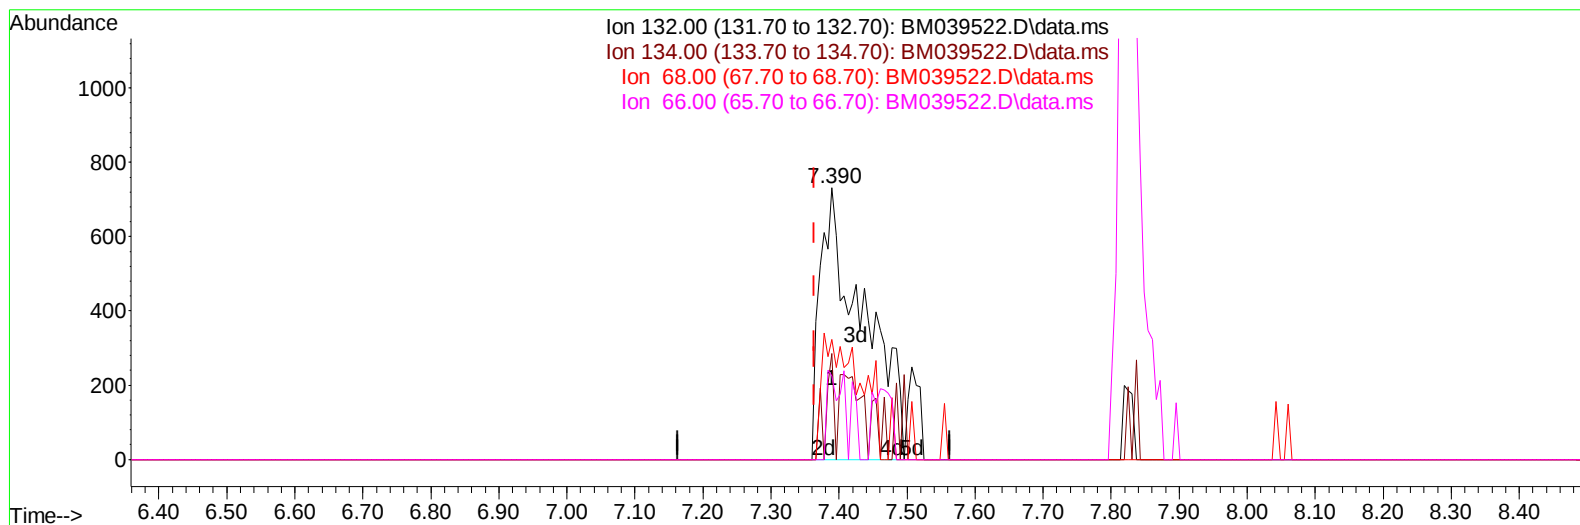

TIC: BM039522.D\data.ms

## (11) 2-Chlorophenol-d4 (S)

7.390min (+ 0.027) 0.22 ng/ul m

response 3201

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 132.00 | 100.00 | 100.00 |
| 134.00 | 33.00  | 39.12  |
| 68.00  | 42.40  | 44.19  |
| 66.00  | 29.00  | 30.78  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
 Data File : BM039522.D  
 Acq On : 20 Apr 2023 12:11  
 Operator : CG/JU  
 Sample : 02296-14DL3 60X  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:45:23 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Apr 19 08:18:41 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
 Supervised By :Jagrut Upadhyay 04/21/2023

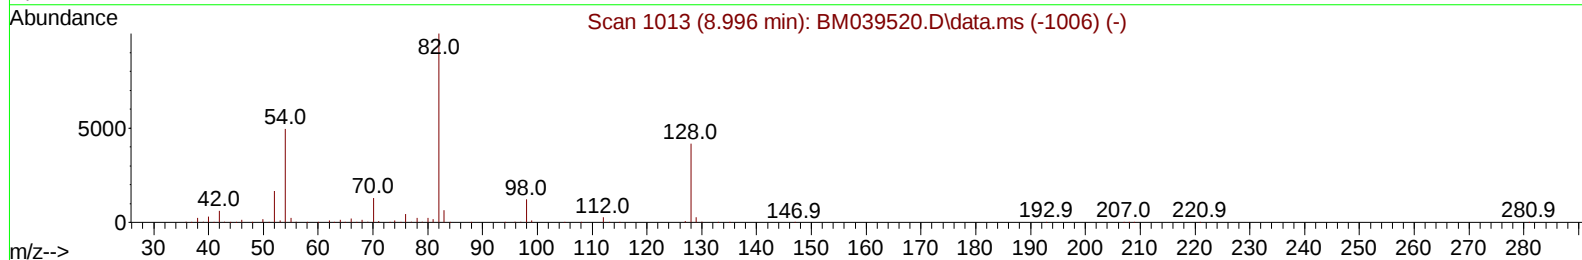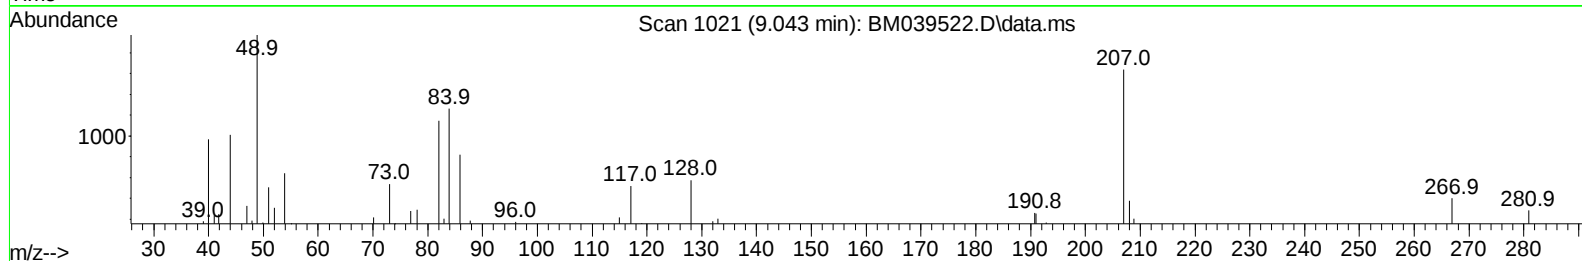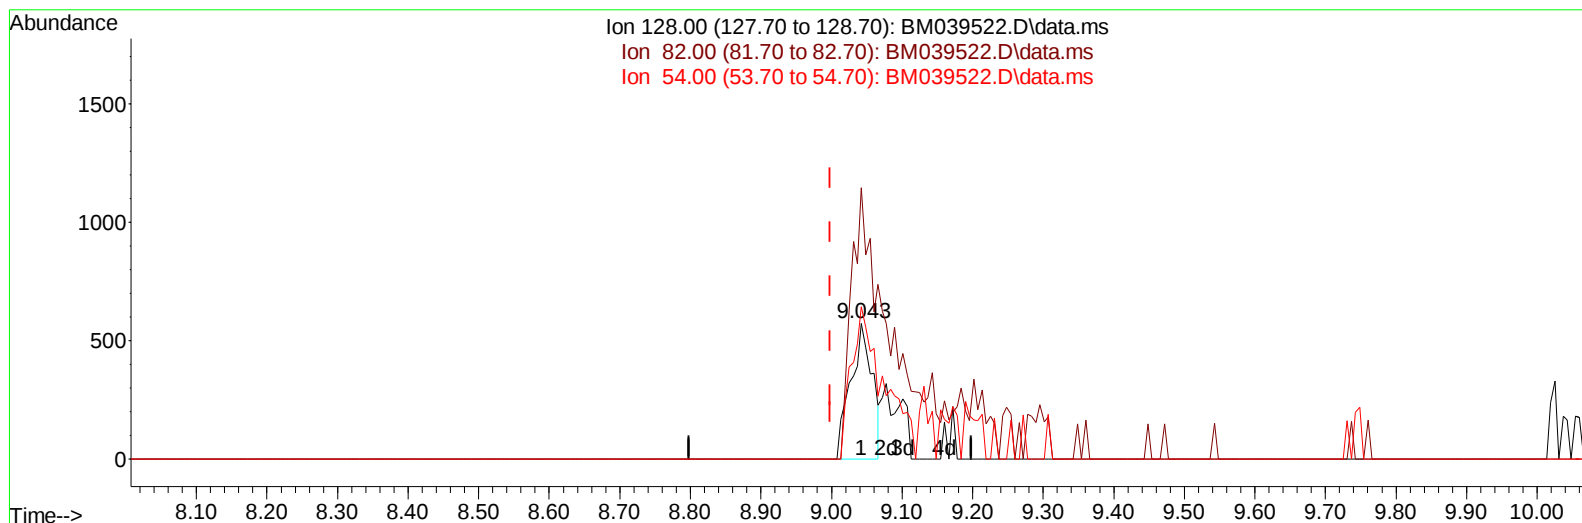

TIC: BM039522.D\data.ms

(21) Nitrobenzene-d5 (S)

9.043min (+ 0.044) 0.16 ng/u1

response 1229

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 128.00 | 100.00 | 100.00 |
| 82.00  | 243.80 | 199.65 |
| 54.00  | 122.00 | 112.20 |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
 Data File : BM039522.D  
 Acq On : 20 Apr 2023 12:11  
 Operator : CG/JU  
 Sample : 02296-14DL3 60X  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:45:23 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Apr 19 08:18:41 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
 Supervised By :Jagrut Upadhyay 04/21/2023

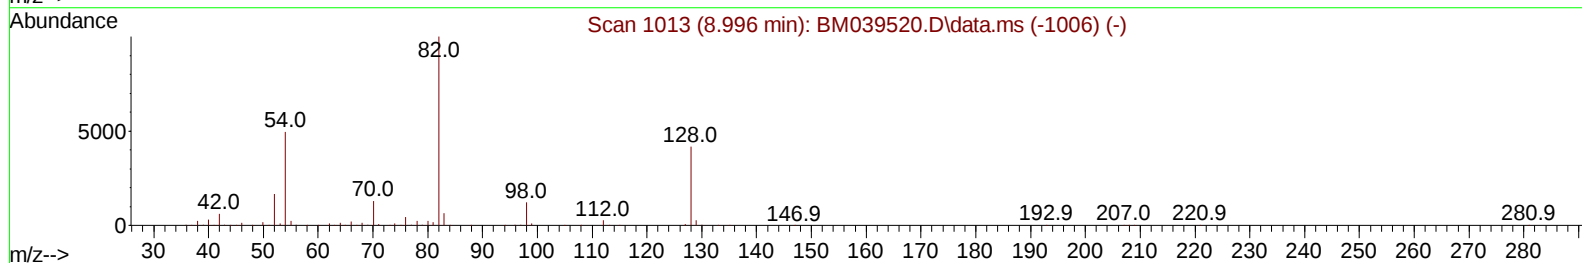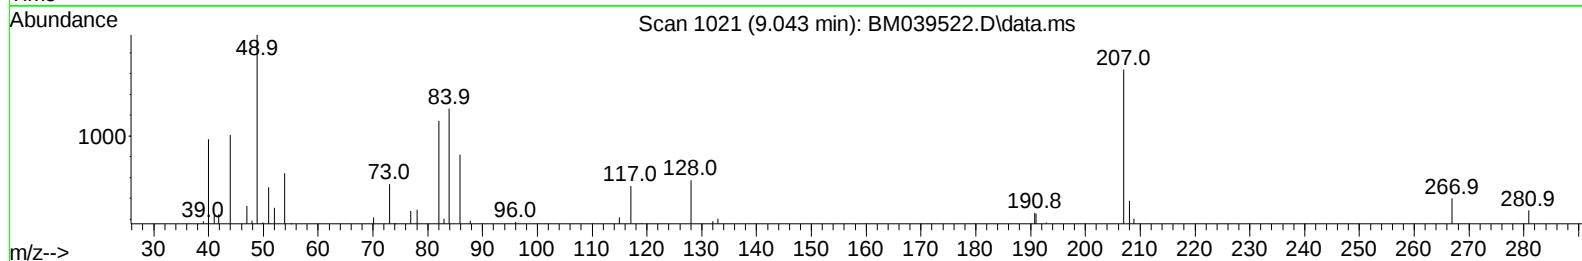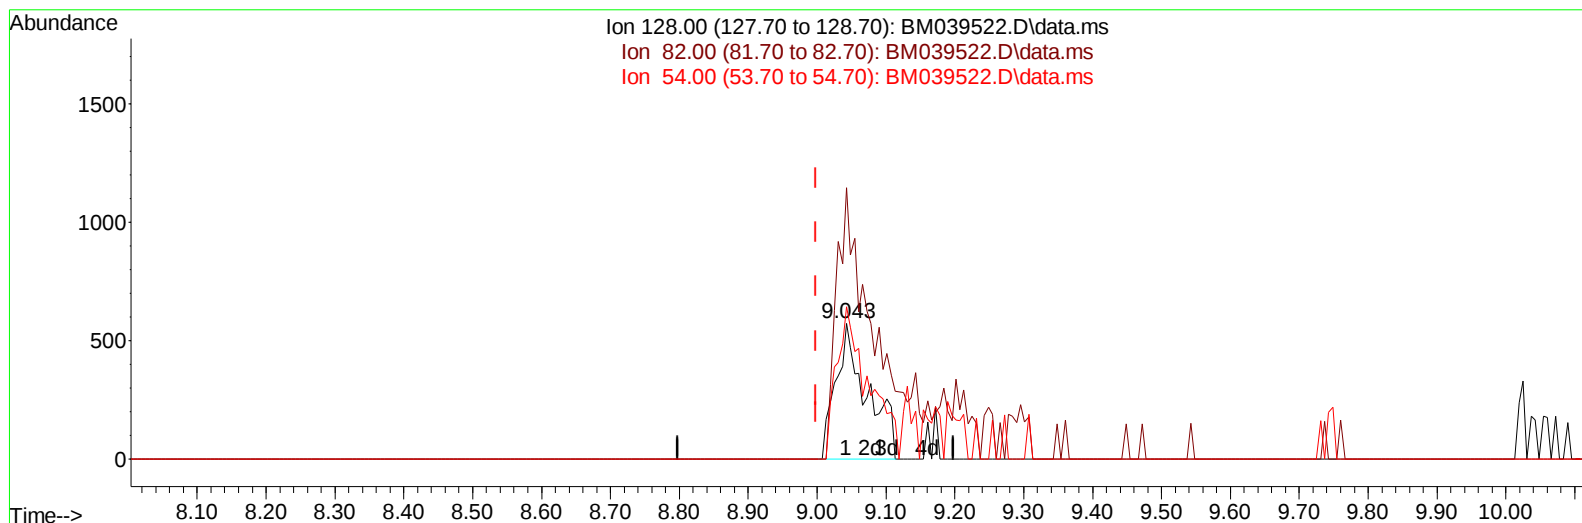

TIC: BM039522.D\data.ms

(21) Nitrobenzene-d5 (S)

9.043min (+ 0.044) 0.24 ng/ul m

response 1814

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 128.00 | 100.00 | 100.00 |
| 82.00  | 243.80 | 199.65 |
| 54.00  | 122.00 | 112.20 |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
Data File : BM039522.D  
Acq On : 20 Apr 2023 12:11  
Operator : CG/JU  
Sample : 02296-14DL3 60X  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:45:46 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Apr 19 08:18:41 2023  
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
Supervised By :Jagrut Upadhyay 04/21/2023

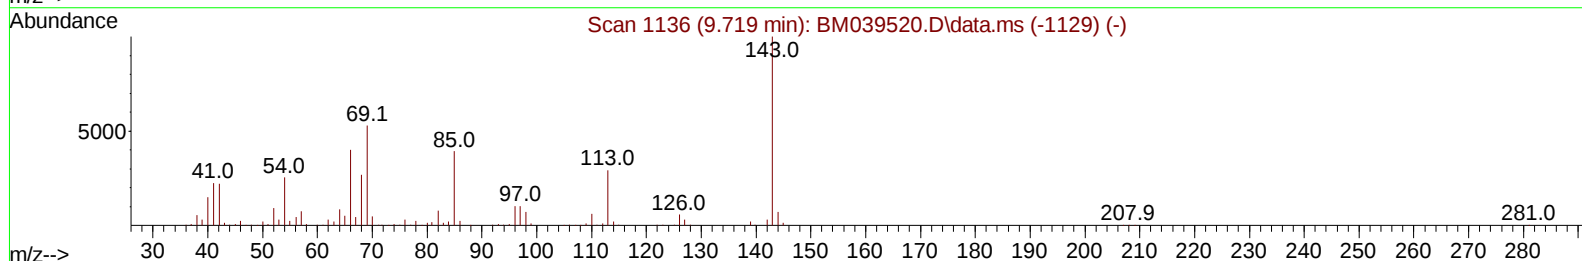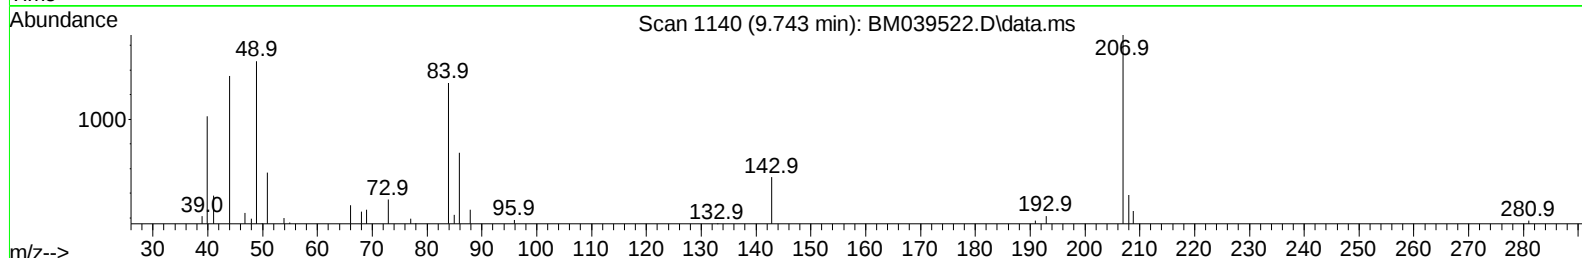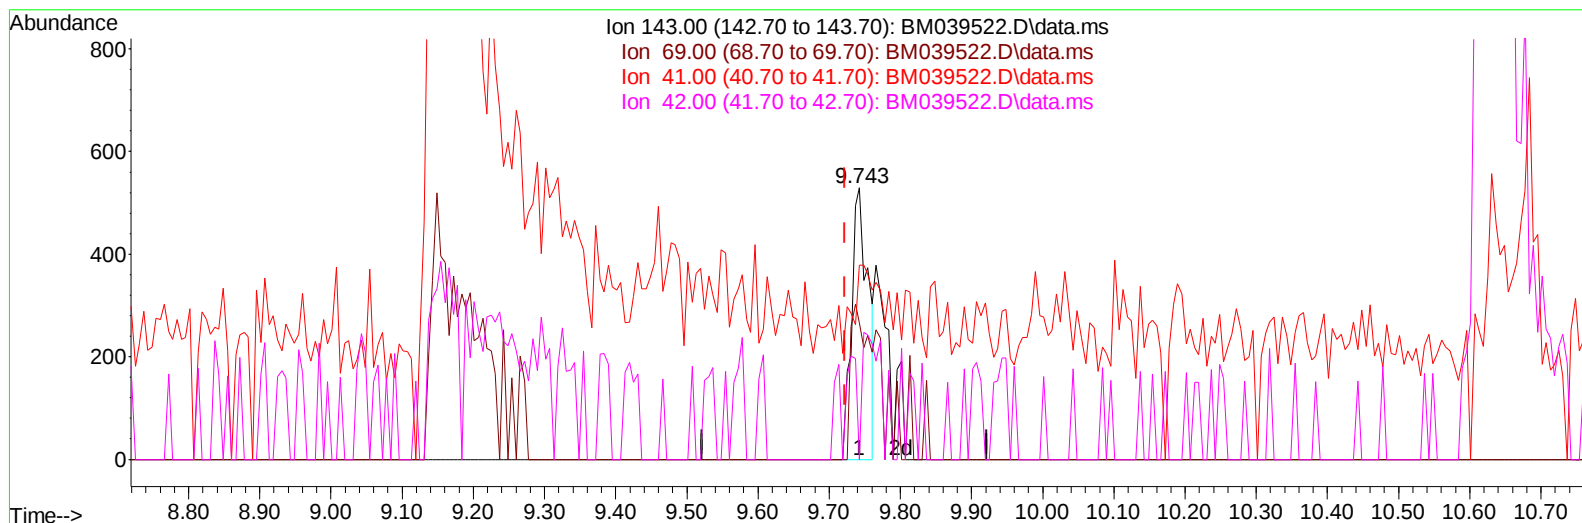

TIC: BM039522.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.743min (+ 0.021) 0.10 ng/u1

response 855

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 143.00 | 100.00 | 100.00 |
| 69.00  | 53.40  | 50.28  |
| 41.00  | 23.00  | 71.46# |
| 42.00  | 24.80  | 0.00#  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
 Data File : BM039522.D  
 Acq On : 20 Apr 2023 12:11  
 Operator : CG/JU  
 Sample : 02296-14DL3 60X  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:45:46 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Apr 19 08:18:41 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
 Supervised By :Jagrut Upadhyay 04/21/2023

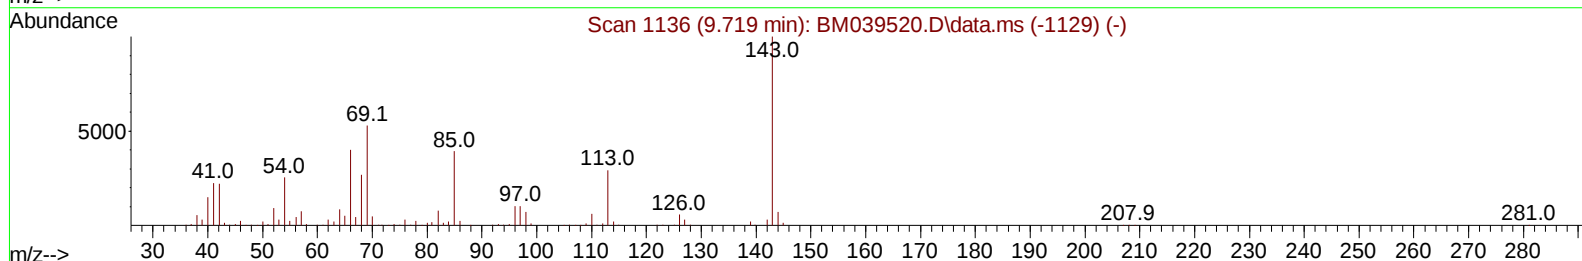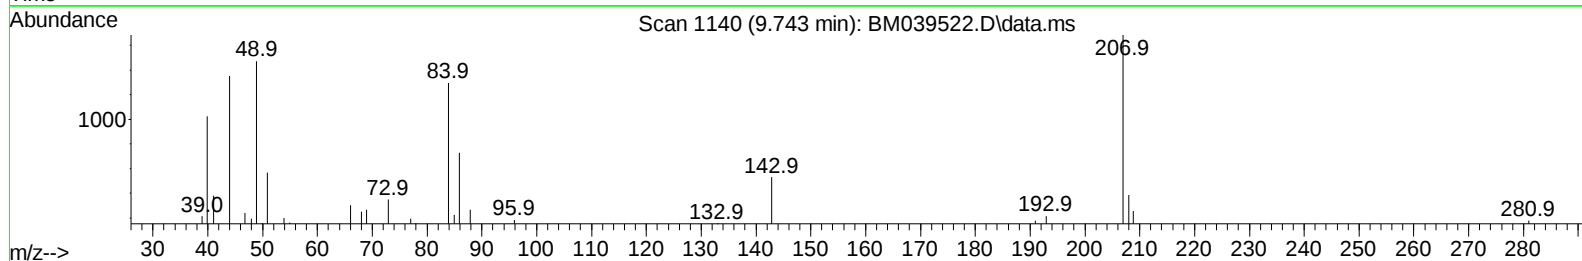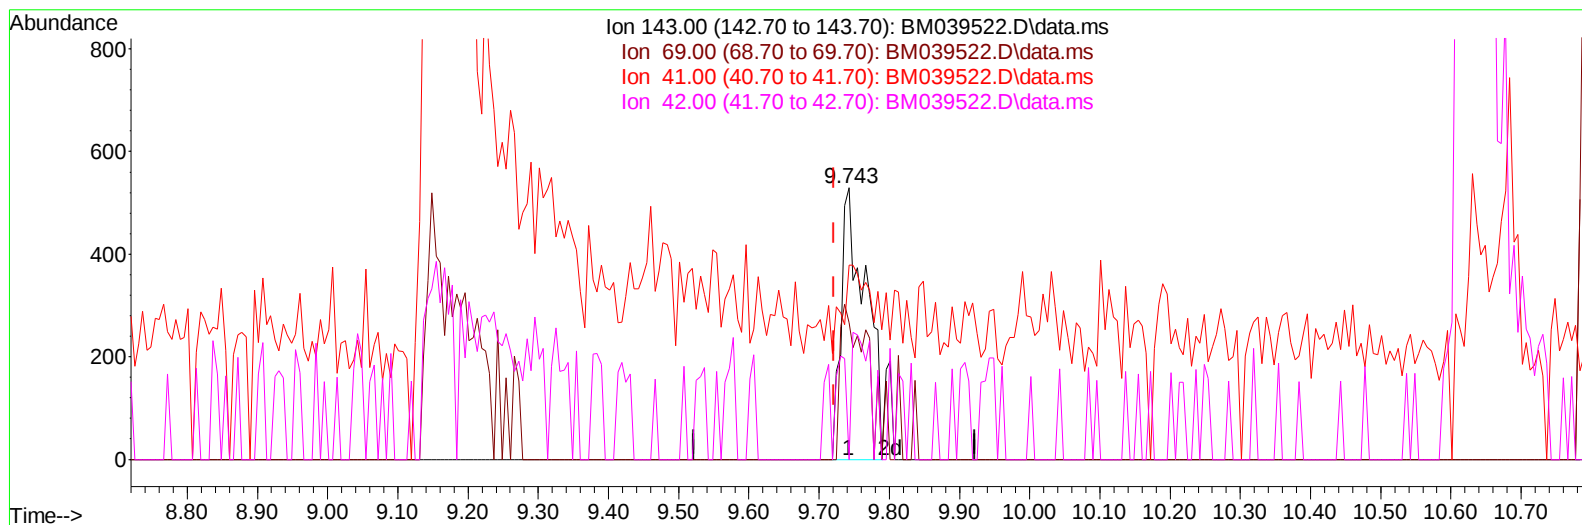

TIC: BM039522.D\data.ms

**(24) 2-Nitrophenol-d4 (S)**

9.743min (+ 0.021) 0.15 ng/ul m

response 1282

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 143.00 | 100.00 | 100.00 |
| 69.00  | 53.40  | 50.28  |
| 41.00  | 23.00  | 71.46# |
| 42.00  | 24.80  | 0.00#  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
 Data File : BM039522.D  
 Acq On : 20 Apr 2023 12:11  
 Operator : CG/JU  
 Sample : 02296-14DL3 60X  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:47:20 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Apr 19 08:18:41 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
 Supervised By :Jagrut Upadhyay 04/21/2023

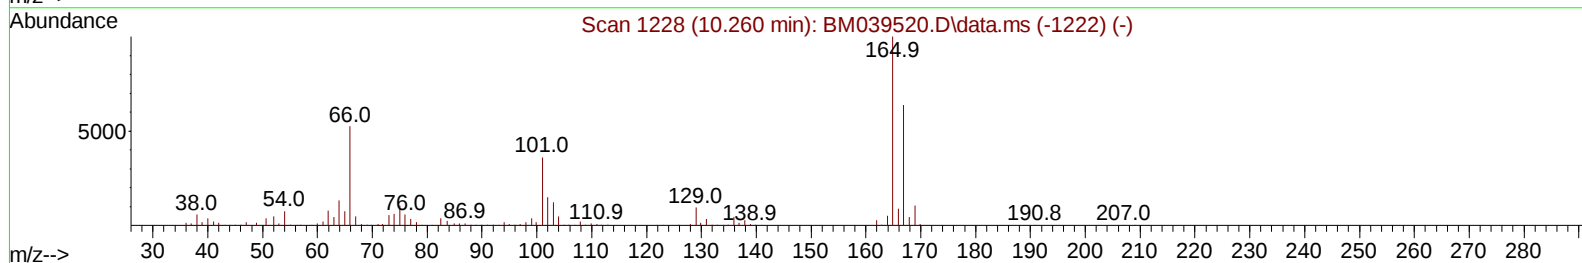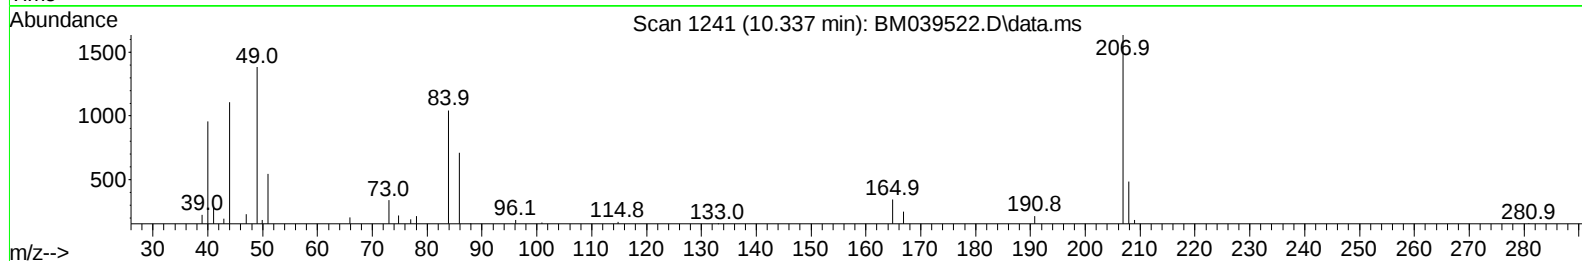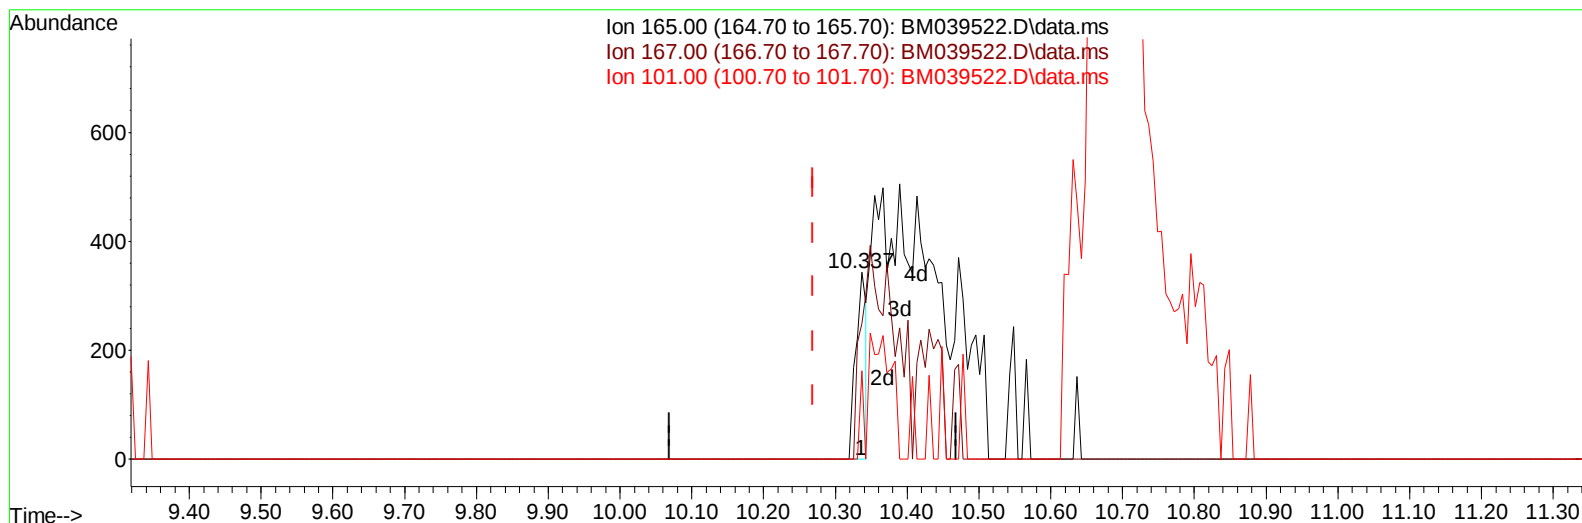

TIC: BM039522.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.337min (+ 0.068) 0.02 ng/u1

response 360

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 165.00 | 100.00 | 100.00 |
| 167.00 | 63.90  | 72.89  |
| 101.00 | 35.30  | 47.23# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
Data File : BM039522.D  
Acq On : 20 Apr 2023 12:11  
Operator : CG/JU  
Sample : 02296-14DL3 60X  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:47:20 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Apr 19 08:18:41 2023  
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
Supervised By :Jagrut Upadhyay 04/21/2023

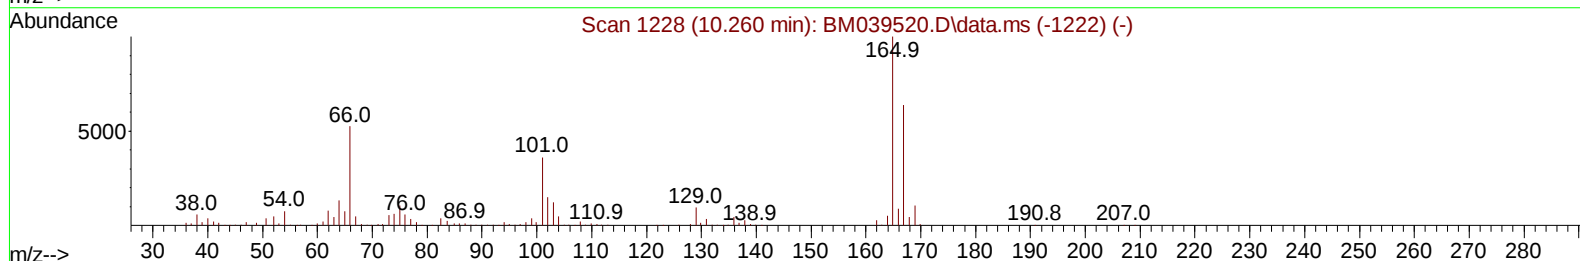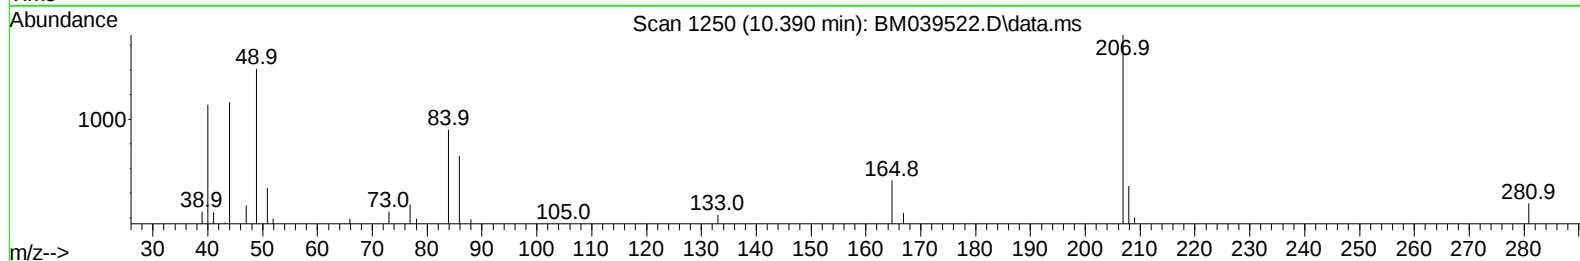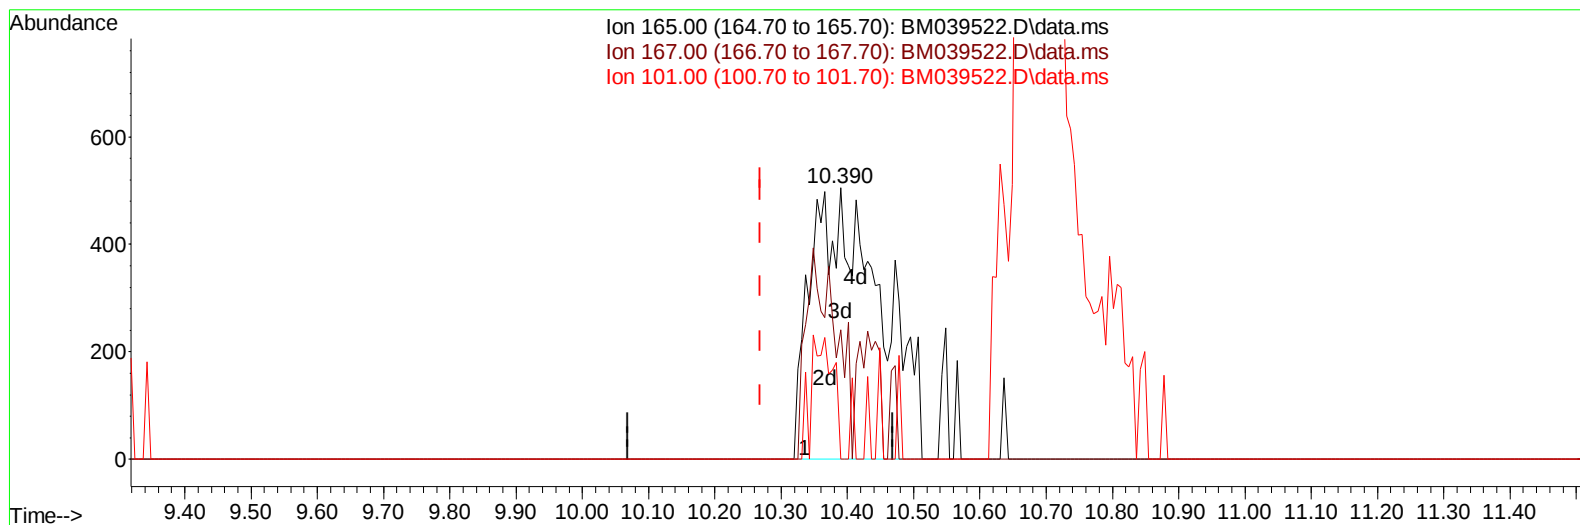

TIC: BM039522.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.390min (+ 0.121) 0.25 ng/ul m

response 3660

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 165.00 | 100.00 | 100.00 |
| 167.00 | 63.90  | 47.72# |
| 101.00 | 35.30  | 0.00#  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
Data File : BM039522.D  
Acq On : 20 Apr 2023 12:11  
Operator : CG/JU  
Sample : 02296-14DL3 60X  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:46:08 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Apr 19 08:18:41 2023  
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
Supervised By :Jagrut Upadhyay 04/21/2023

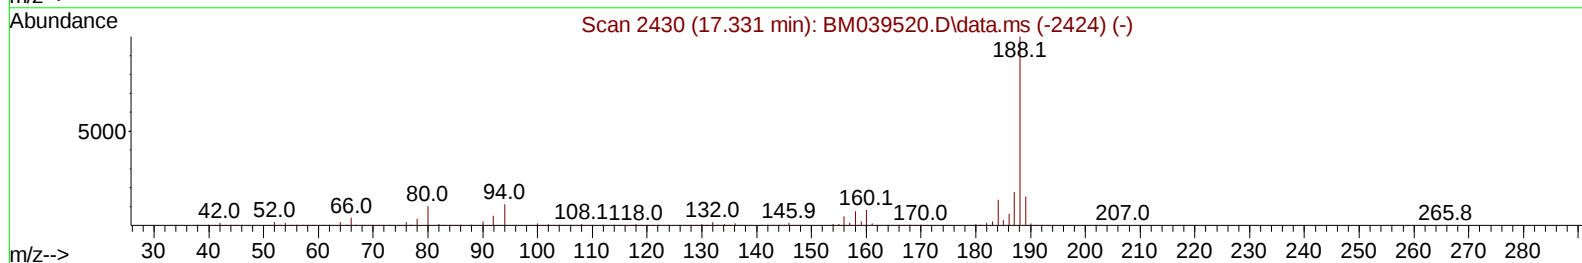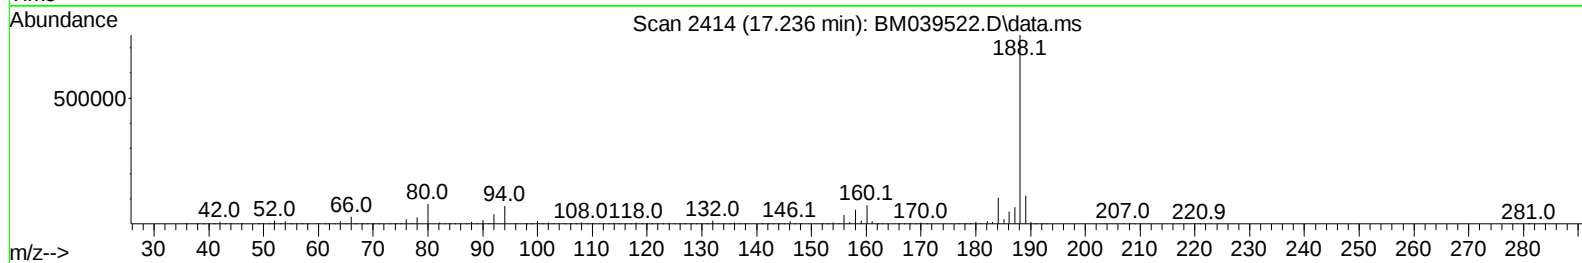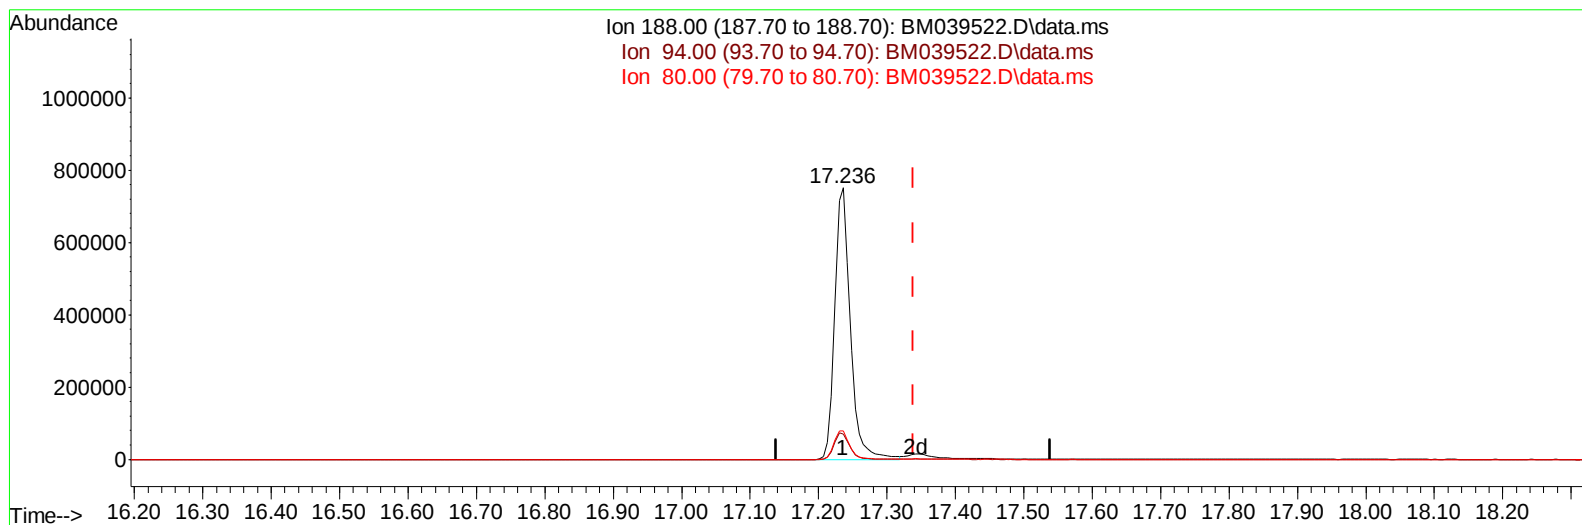

TIC: BM039522.D\data.ms

(73) Anthracene-d10 (S)

17.236min (-0.103) 20.79 ng/u1

response 1185498

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 11.60  | 9.40   |
| 80.00  | 10.20  | 10.42  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
 Data File : BM039522.D  
 Acq On : 20 Apr 2023 12:11  
 Operator : CG/JU  
 Sample : 02296-14DL3 60X  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:46:08 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Apr 19 08:18:41 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
 Supervised By :Jagrut Upadhyay 04/21/2023

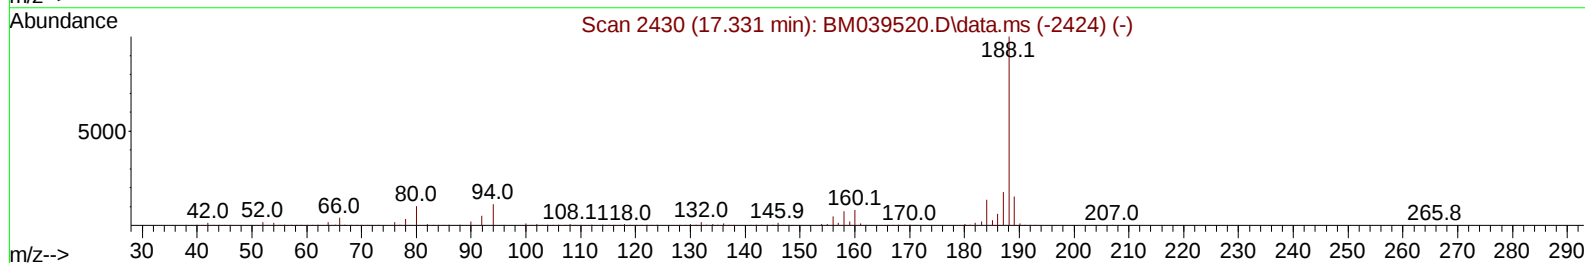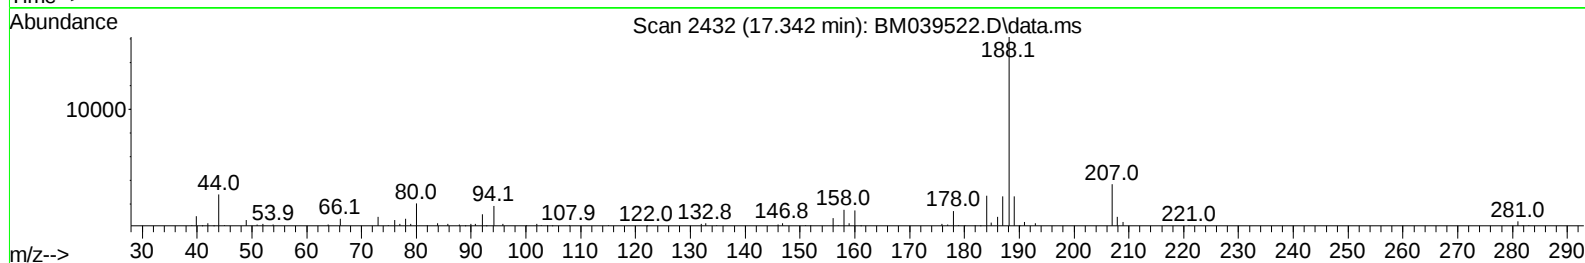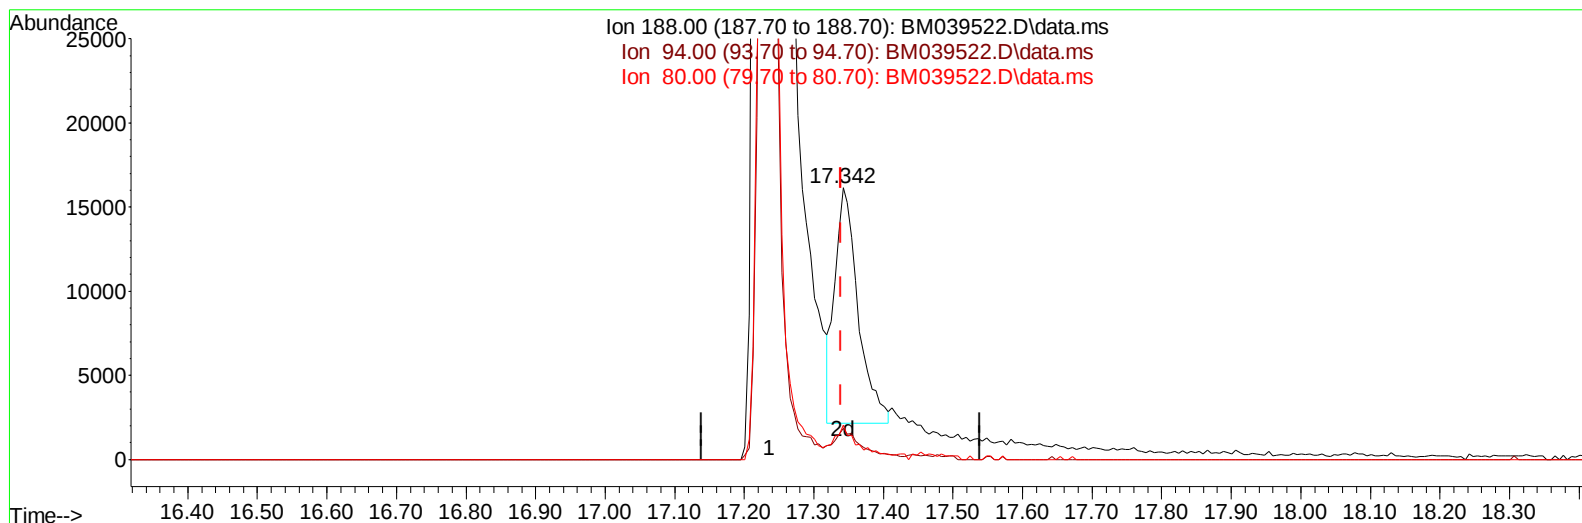

TIC: BM039522.D\data.ms

**(73) Anthracene-d10 (S)**

17.342min (+ 0.003) 0.57 ng/ul m

response 32464

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 11.60  | 11.51  |
| 80.00  | 10.20  | 12.66# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
 Data File : BM039522.D  
 Acq On : 20 Apr 2023 12:11  
 Operator : CG/JU  
 Sample : 02296-14DL3 60X  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:47:20 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Apr 19 08:18:41 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
 Supervised By :Jagrut Upadhyay 04/21/2023

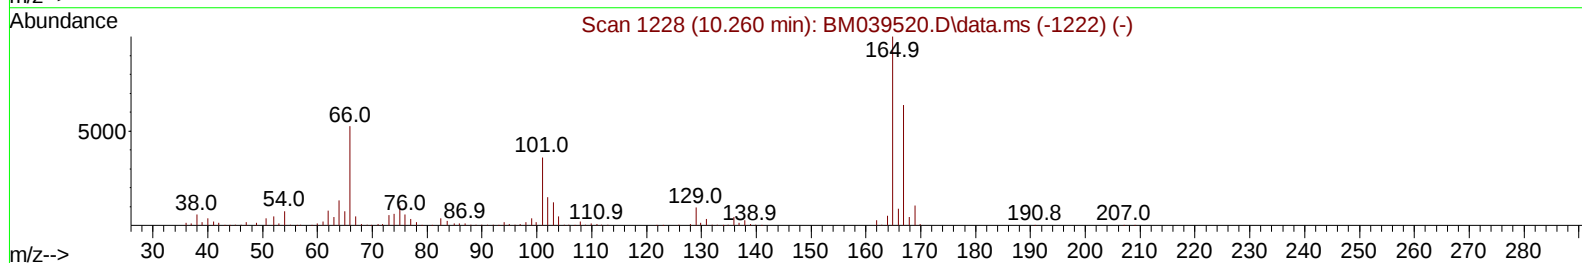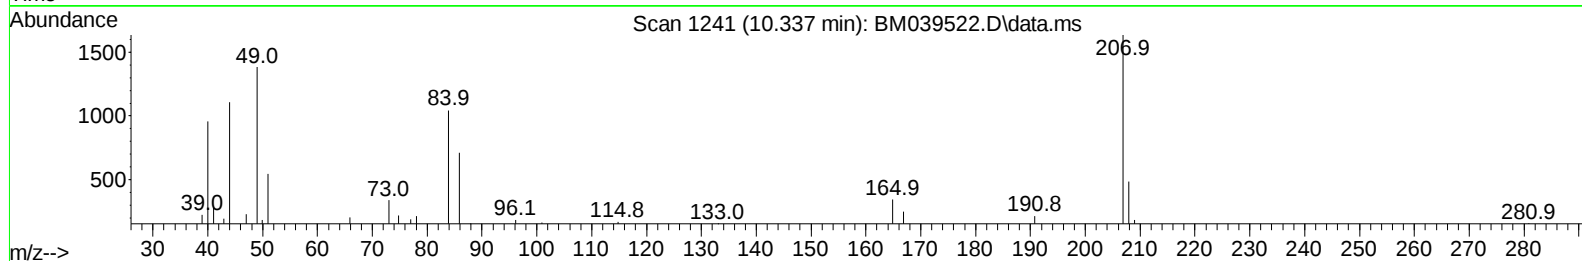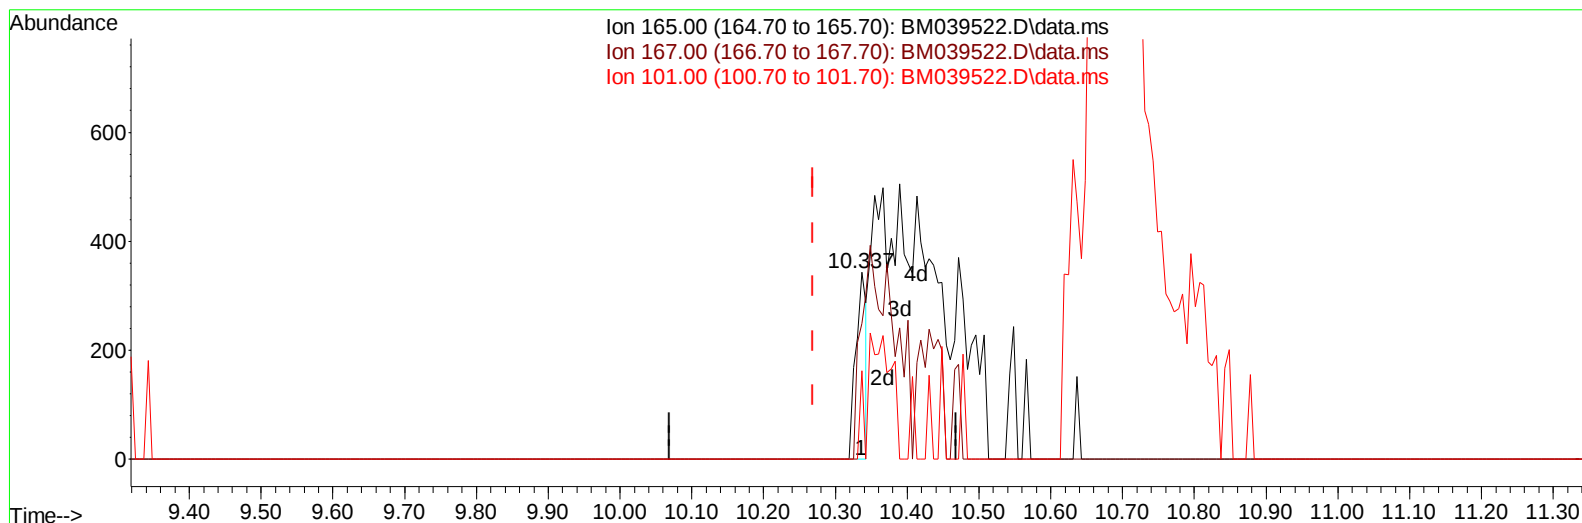

TIC: BM039522.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.337min (+ 0.068) 0.02 ng/u1

response 360

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 165.00 | 100.00 | 100.00 |
| 167.00 | 63.90  | 72.89  |
| 101.00 | 35.30  | 47.23# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
Data File : BM039522.D  
Acq On : 20 Apr 2023 12:11  
Operator : CG/JU  
Sample : 02296-14DL3 60X  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:47:20 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Apr 19 08:18:41 2023  
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
Supervised By :Jagrut Upadhyay 04/21/2023

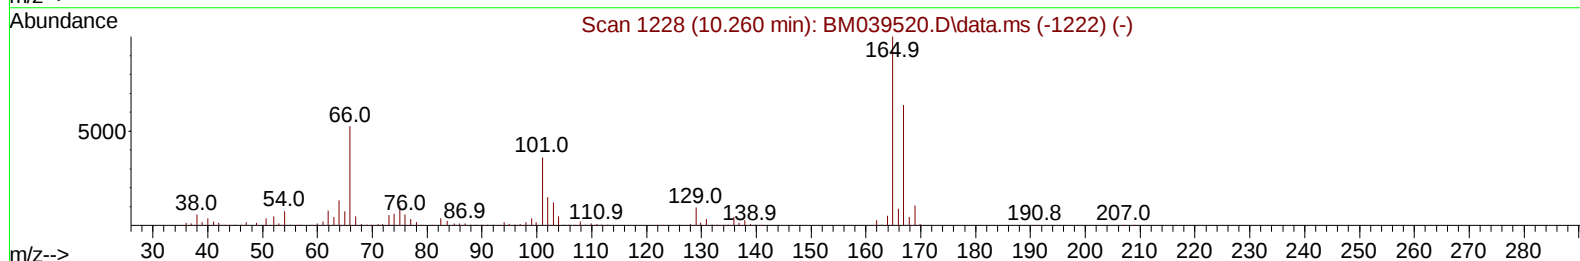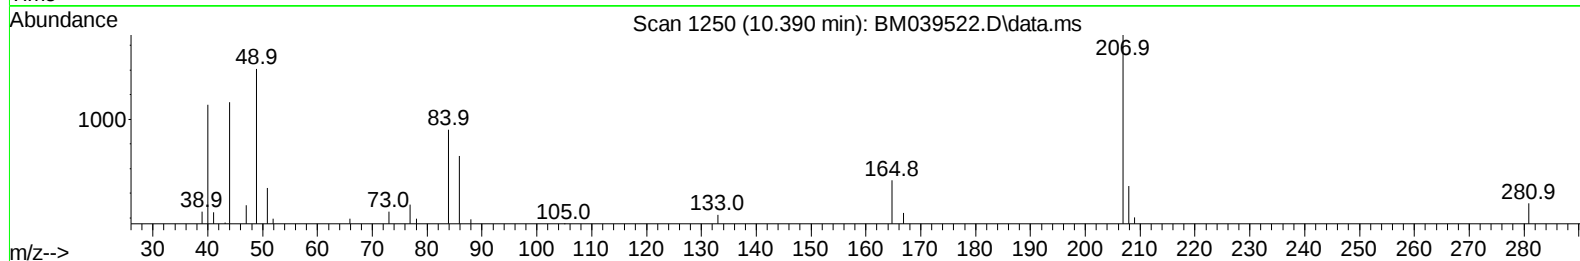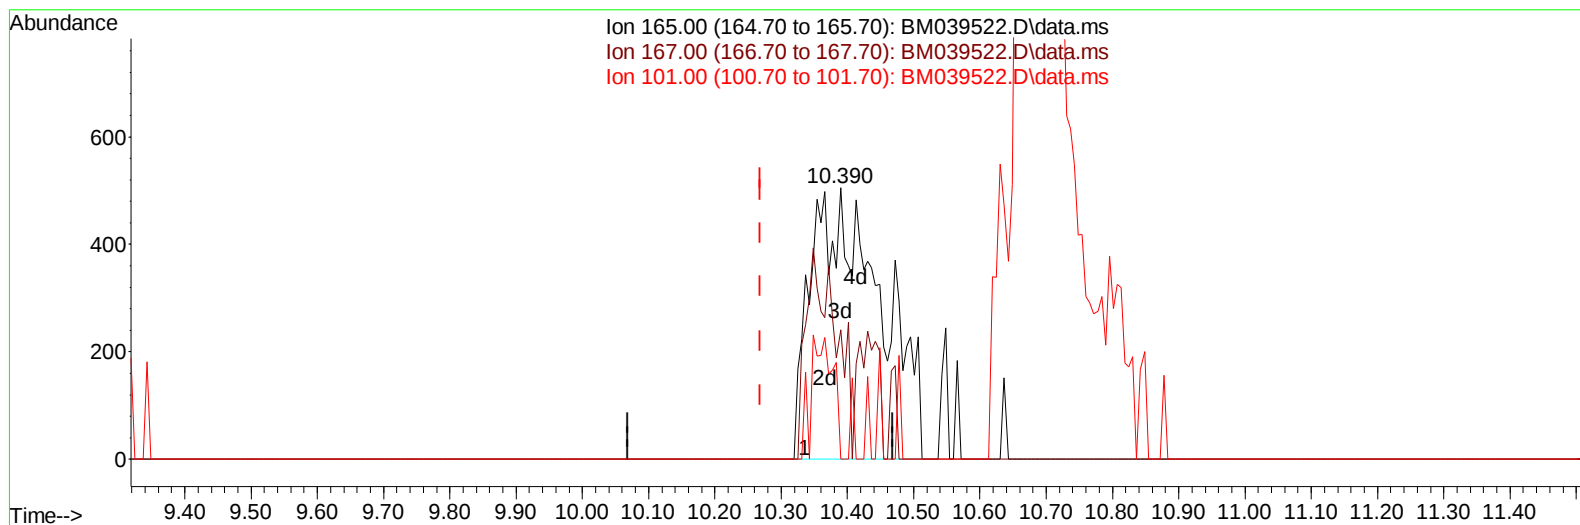

TIC: BM039522.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.390min (+ 0.121) 0.25 ng/ul m

response 3660

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 165.00 | 100.00 | 100.00 |
| 167.00 | 63.90  | 47.72# |
| 101.00 | 35.30  | 0.00#  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
 Data File : BM039522.D  
 Acq On : 20 Apr 2023 12:11  
 Operator : CG/JU  
 Sample : 02296-14DL3 60X  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DCBL8DL3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 03:19:48 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Apr 19 08:18:41 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
 Supervised By :Jagrut Upadhyay 04/21/2023

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.825  | 152  | 203670   | 20.000 | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 10.631 | 136  | 933727   | 20.000 | ng/ul  | 0.00     |
| 38) Acenaphthene-d10          | 14.483 | 164  | 603379   | 20.000 | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.236 | 188  | 1185498  | 20.000 | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 21.430 | 240  | 865997   | 20.000 | ng/ul  | 0.00     |
| 88) Perylene-d12              | 23.795 | 264  | 935843   | 20.000 | ng/ul  | 0.00     |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 0.000  | 96   | 0d       | 0.000  | ng/uL  |          |
| 4) Pyridine-d5                | 0.000  | 84   | 0d       | 0.000  | ng/ul  |          |
| 7) Phenol-d5                  | 0.000  | 99   | 0d       | 0.000  | ng/ul  |          |
| 9) Bis-(2-Chloroethyl)eth...  | 7.178  | 67   | 4691m    | 0.381  | ng/ul  | 0.01     |
| 11) 2-Chlorophenol-d4         | 7.390  | 132  | 3201m    | 0.219  | ng/ul  | 0.03     |
| 15) 4-Methylphenol-d8         | 0.000  | 113  | 0d       | 0.000  | ng/ul  |          |
| 21) Nitrobenzene-d5           | 9.043  | 128  | 1814m    | 0.241  | ng/ul  | 0.04     |
| 24) 2-Nitrophenol-d4          | 9.743  | 143  | 1282m    | 0.152  | ng/ul  | 0.02     |
| 28) 2,4-Dichlorophenol-d3     | 10.390 | 165  | 3660m    | 0.252  | ng/ul  | 0.12     |
| 31) 4-Chloroaniline-d4        | 0.000  | 131  | 0d       | 0.000  | ng/ul  |          |
| 46) Dimethylphthalate-d6      | 13.907 | 166  | 21518    | 0.442  | ng/ul  | 0.00     |
| 49) Acenaphthylene-d8         | 14.178 | 160  | 21618    | 0.395  | ng/ul  | 0.00     |
| 54) 4-Nitrophenol-d4          | 0.000  | 143  | 0        | 0.000  | ng/ul  |          |
| 60) Fluorene-d10              | 15.489 | 176  | 18187    | 0.456  | ng/ul  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 0.000  | 200  | 0        | 0.000  | ng/ul  |          |
| 73) Anthracene-d10            | 17.342 | 188  | 32464m   | 0.569  | ng/ul  | 0.00     |
| 81) Pyrene-d10                | 19.636 | 212  | 26949    | 0.468  | ng/ul  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.648 | 264  | 22697    | 0.449  | ng/ul  | 0.00     |
| Target Compounds              |        |      |          |        |        |          |
|                               |        |      |          |        | Qvalue |          |
| 30) Naphthalene               | 10.684 | 128  | 2407944  | 46.609 | ng/ul  | 100      |
| 37) 1-Methylnaphthalene       | 12.519 | 142  | 177320   | 5.095  | ng/ul  | 100      |
| 43) 1,1'-Biphenyl             | 13.325 | 154  | 67330    | 1.444  | ng/ul  | 98       |
| 52) Acenaphthene              | 14.548 | 153  | 167371   | 4.157  | ng/ul  | 99       |
| 56) Dibenzofuran              | 14.889 | 168  | 195039   | 3.564  | ng/ul  | 98       |
| 72) Phenanthrene              | 17.277 | 178  | 91800    | 1.395  | ng/ul  | 98       |
| 77) Carbazole                 | 17.666 | 167  | 68339    | 1.165  | ng/ul  | 99       |
| -----                         |        |      |          |        |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM042023\  
Data File : BM039522.D  
Acq On : 20 Apr 2023 12:11  
Operator : CG/JU  
Sample : 02296-14DL3 60X  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DCBL8DL3

## Manual IntegrationsAPPROVED

Quant Time: Apr 21 03:19:48 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM041823.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Apr 19 08:18:41 2023  
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/21/2023  
Supervised By :Jagrut Upadhyay 04/21/2023

