




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039525.D
 Acq On : 20 Apr 2023 15:14
 Operator : CG/JU
 Sample : PB152232BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK230

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:37:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 19 08:18:41 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/02/2023
 Supervised By :Jagrut Upadhyay 05/02/2023

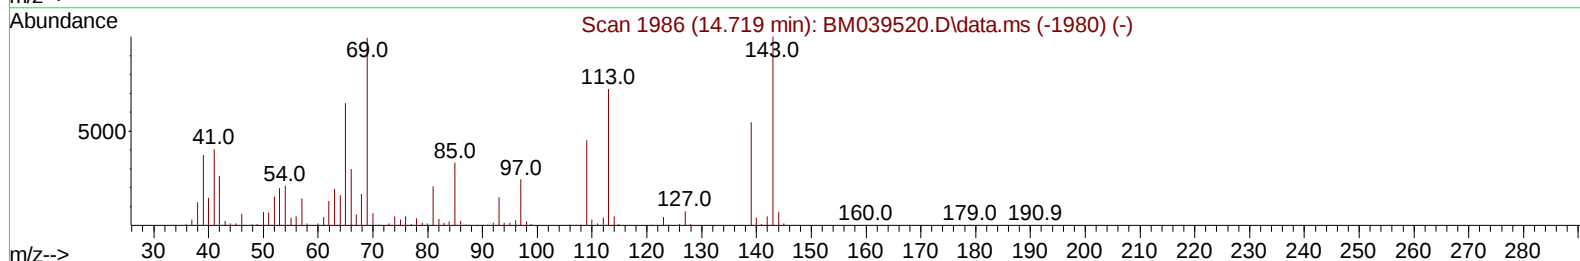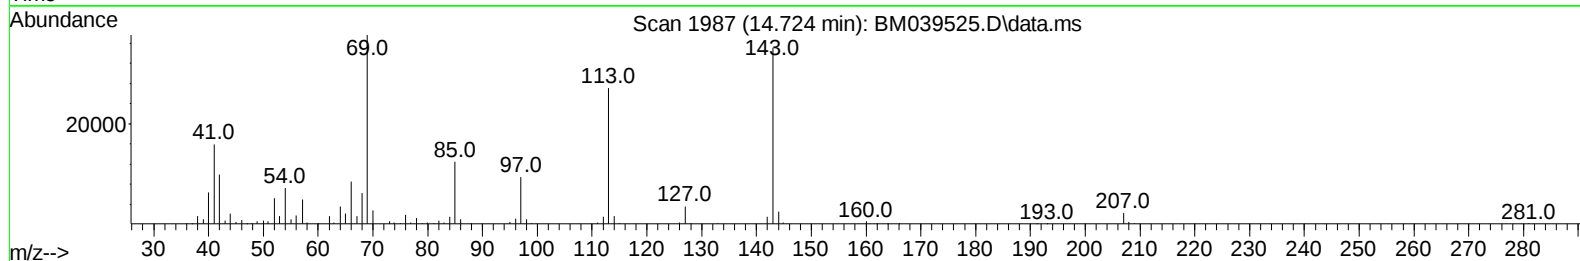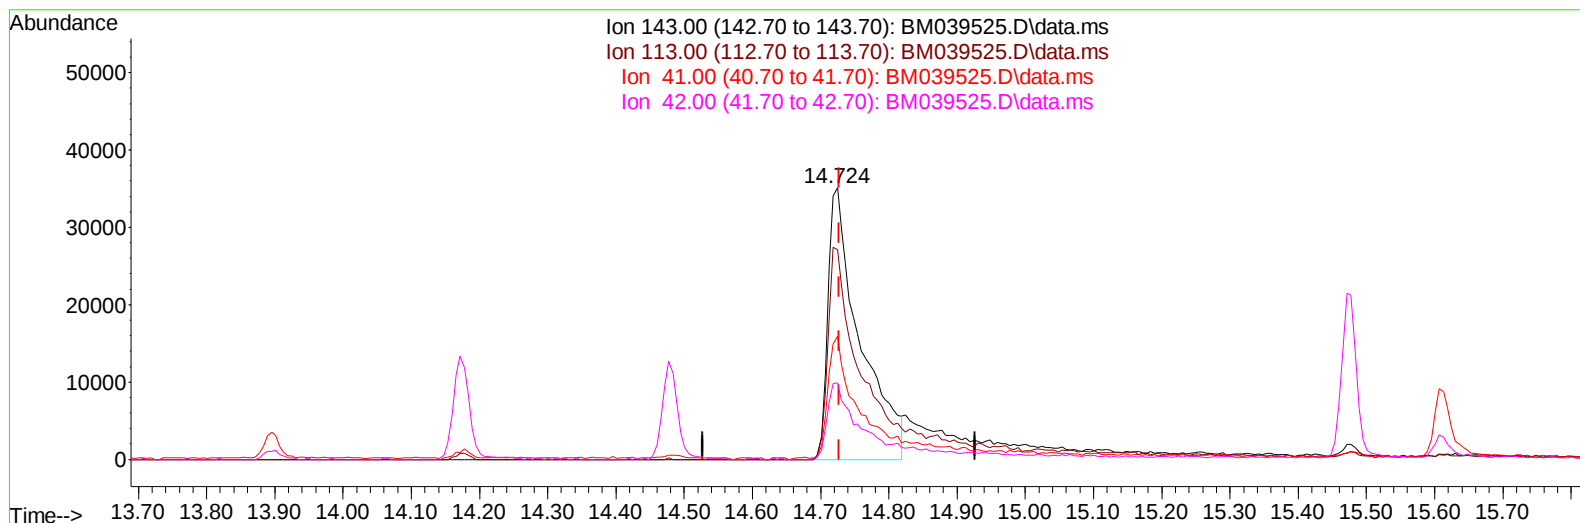

TIC: BM039525.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.724min (-0.003) 15.30 ng/u1

response 113474

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.20	77.18
41.00	39.90	45.36
42.00	26.60	28.23




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039525.D
Acq On : 20 Apr 2023 15:14
Operator : CG/JU
Sample : PB152232BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK230

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/02/2023
Supervised By :Jagrut Upadhyay 05/02/2023

Quant Time: Apr 21 00:37:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 08:18:41 2023
Response via : Initial Calibration

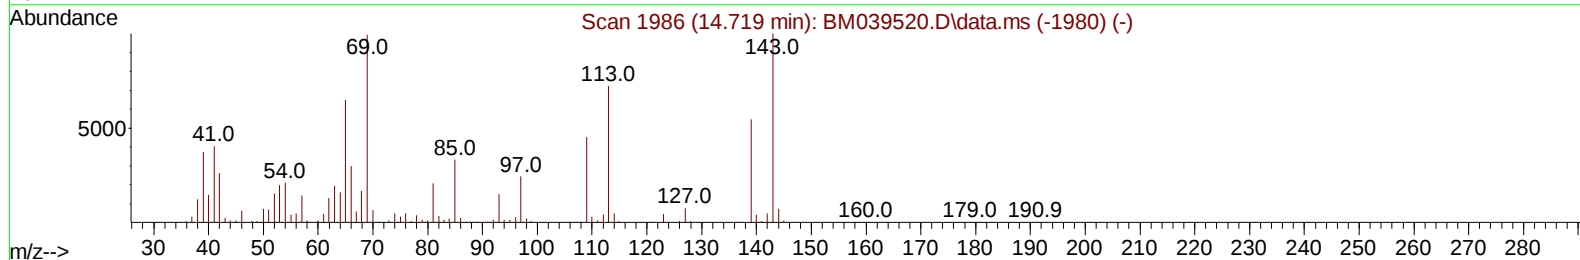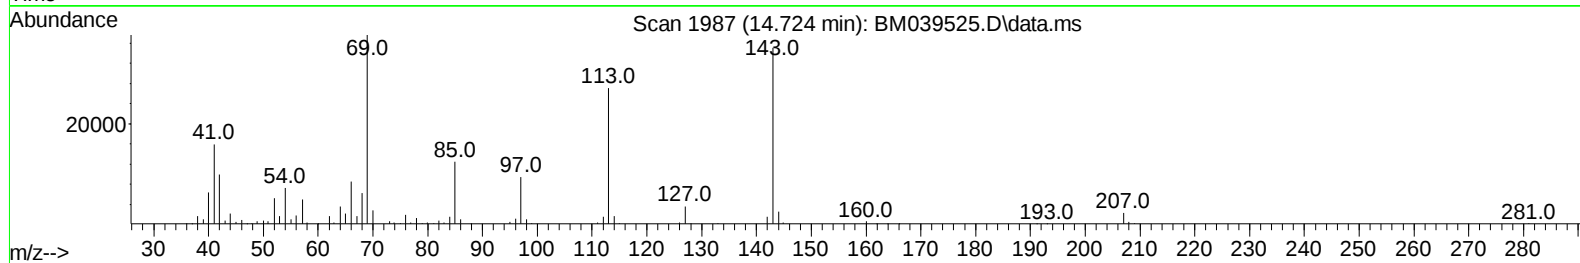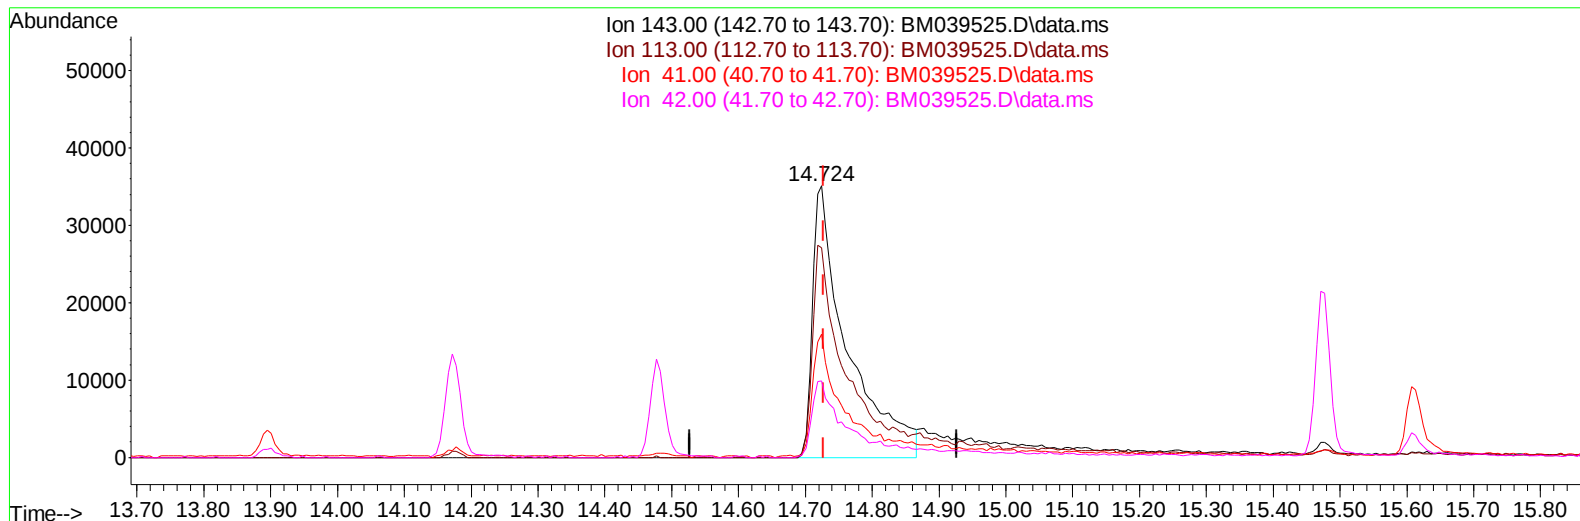

TIC: BM039525.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.724min (-0.003) 16.99 ng/ul m

response 125999

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.20	77.18
41.00	39.90	45.36
42.00	26.60	28.23

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039525.D
 Acq On : 20 Apr 2023 15:14
 Operator : CG/JU
 Sample : PB152232BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK230

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/02/2023
 Supervised By :Jagrut Upadhyay 05/02/2023

Quant Time: Apr 21 01:12:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 19 08:18:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	202610	20.000	ng/ul	0.00
20) Naphthalene-d8	10.631	136	931801	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.483	164	607623	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.230	188	1272922	20.000	ng/ul	0.00
79) Chrysene-d12	21.424	240	912798	20.000	ng/ul	0.00
88) Perylene-d12	23.789	264	892393	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	32837	6.221	ng/uL	0.00
4) Pyridine-d5	3.637	84	417708	28.164	ng/ul	0.00
7) Phenol-d5	7.007	99	529139	28.534	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.160	67	372456	30.388	ng/ul	0.00
11) 2-Chlorophenol-d4	7.354	132	451934	31.068	ng/ul	0.00
15) 4-Methylphenol-d8	8.554	113	430374	28.811	ng/ul	0.00
21) Nitrobenzene-d5	8.995	128	221331	29.524	ng/ul	0.00
24) 2-Nitrophenol-d4	9.719	143	248646	29.538	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.266	165	409332	28.261	ng/ul	0.00
31) 4-Chloroaniline-d4	10.784	131	588080	27.185	ng/ul	0.00
46) Dimethylphthalate-d6	13.895	166	1517283	30.962	ng/ul	0.00
49) Acenaphthylene-d8	14.172	160	1679297	30.504	ng/ul	0.00
54) 4-Nitrophenol-d4	14.724	143	125999m	16.989	ng/ul	0.00
60) Fluorene-d10	15.477	176	1280910	31.904	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.613	200	174538	20.633	ng/ul	0.00
73) Anthracene-d10	17.330	188	1943959	31.755	ng/ul	0.00
81) Pyrene-d10	19.630	212	2087734	34.420	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.636	264	1529482	31.746	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039525.D
Acq On : 20 Apr 2023 15:14
Operator : CG/JU
Sample : PB152232BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK230

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/02/2023
Supervised By :Jagrut Upadhyay 05/02/2023

Quant Time: Apr 21 01:12:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 19 08:18:41 2023
Response via : Initial Calibration

