

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039521.D
 Acq On : 20 Apr 2023 11:15
 Operator : CG/JU
 Sample : PB152232BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	26	30	39	rBV	70918	92916	2.27%	0.197%
2	3.637	99	102	128	rBV	681845	1059490	25.83%	2.244%
3	3.966	155	158	163	rVB2	14420	21348	0.52%	0.045%
4	7.007	668	675	694	rBV	664058	1298927	31.66%	2.751%
5	7.160	695	701	726	rVB	657541	1155768	28.17%	2.448%
6	7.354	728	734	751	rBV	824639	1432401	34.92%	3.034%
7	7.825	807	814	828	rBV	634212	1123164	27.38%	2.379%
8	8.554	931	938	961	rBV	827296	1677741	40.90%	3.553%
9	8.748	968	971	979	rVB8	5801	12545	0.31%	0.027%
10	8.995	1005	1013	1037	rBV	725553	1370138	33.40%	2.902%
11	9.719	1129	1136	1155	rBV	592270	1132691	27.61%	2.399%
12	10.266	1222	1229	1265	rBV	758248	1683451	41.04%	3.565%
13	10.630	1284	1291	1310	rBV	964689	1672337	40.77%	3.542%
14	10.783	1310	1317	1338	rBV	689420	1591930	38.81%	3.372%
15	11.089	1368	1369	1377	rVB7	3019	4144	0.10%	0.009%
16	12.272	1562	1570	1574	rBV6	6116	14376	0.35%	0.030%
17	13.383	1753	1759	1762	rBV4	4870	6921	0.17%	0.015%
18	13.895	1840	1846	1866	rBV	1802786	2681000	65.35%	5.678%
19	14.171	1886	1893	1916	rBV	2068791	3214847	78.37%	6.809%
20	14.477	1939	1945	1961	rBV	1429894	2248802	54.82%	4.763%
21	14.730	1982	1988	2014	rBV	120329	561691	13.69%	1.190%
22	15.477	2108	2115	2132	rBV	2487508	3803809	92.73%	8.056%
23	15.612	2132	2138	2152	rVV	489438	887705	21.64%	1.880%
24	15.718	2153	2156	2164	rVB6	17257	33367	0.81%	0.071%
25	16.595	2303	2305	2310	rVB5	3029	4980	0.12%	0.011%
26	16.824	2340	2344	2346	rBV4	2647	4171	0.10%	0.009%
27	17.024	2373	2378	2381	rBV5	3566	6978	0.17%	0.015%
28	17.230	2407	2413	2424	rBV	1638717	2390773	58.28%	5.063%
29	17.330	2424	2430	2451	rVB	2512649	3805536	92.77%	8.060%
30	19.195	2743	2747	2753	rBV4	27636	40165	0.98%	0.085%
31	19.271	2756	2760	2764	rBV	21253	32389	0.79%	0.069%
32	19.630	2815	2821	2839	rBV	2908972	4102228	100.00%	8.688%
33	21.424	3121	3126	3142	rBV	1318538	2201282	53.66%	4.662%
34	23.635	3495	3502	3514	rBV2	1776848	3629194	88.47%	7.686%
35	23.788	3522	3528	3548	rVB2	1013481	2216995	54.04%	4.695%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039521.D
Acq On : 20 Apr 2023 11:15
Operator : CG/JU
Sample : PB152232BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK232

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47216200

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039521.D
Acq On : 20 Apr 2023 11:15
Operator : CG/JU
Sample : PB152232BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK232

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

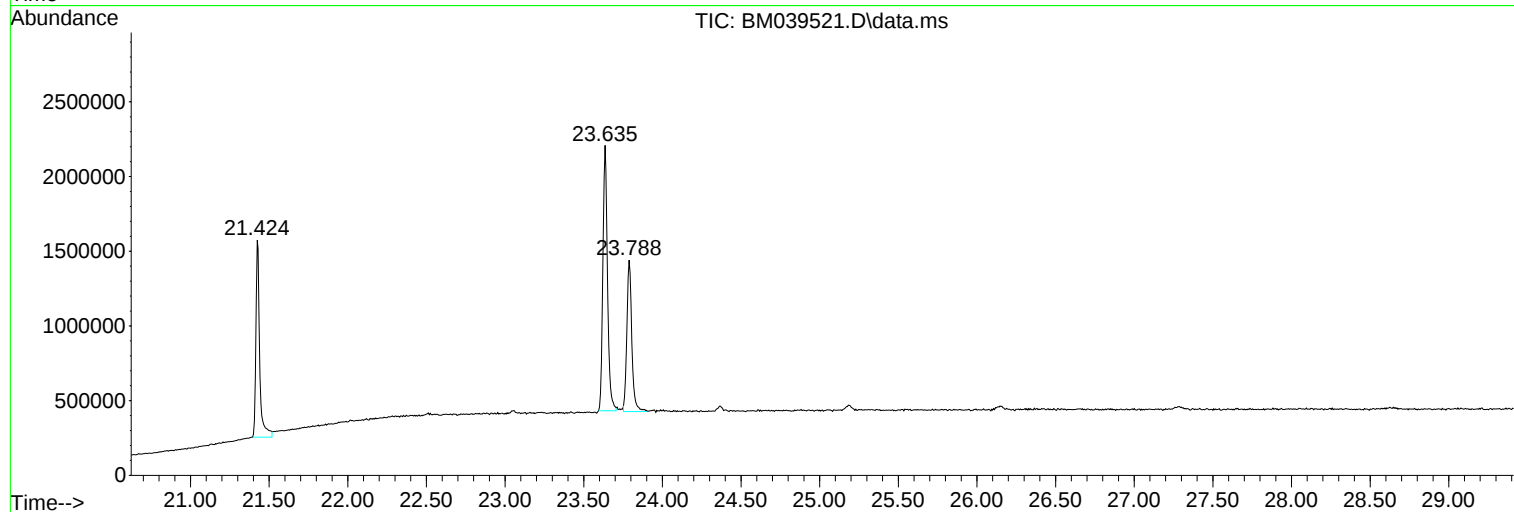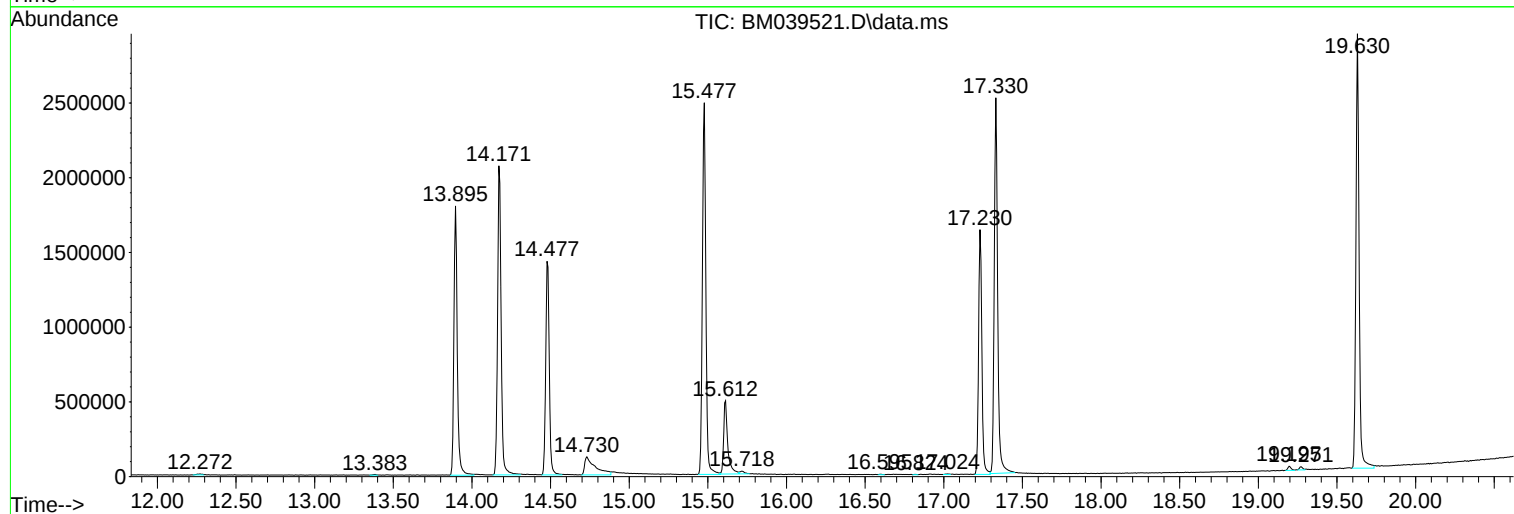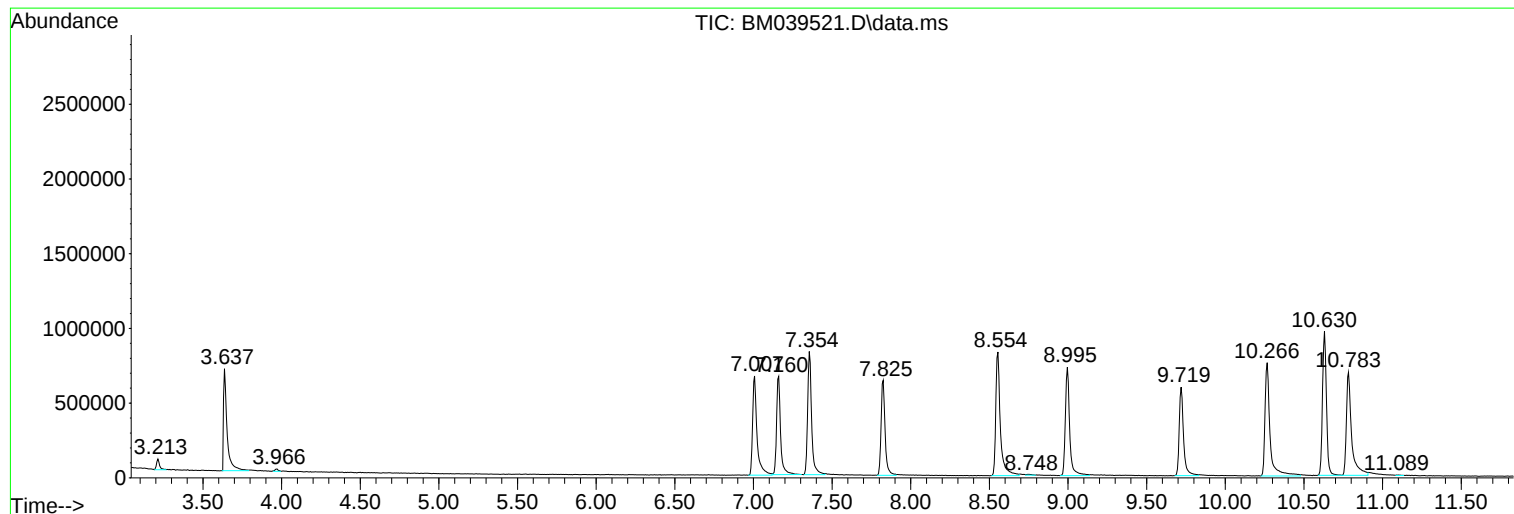

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039521.D
Acq On : 20 Apr 2023 11:15
Operator : CG/JU
Sample : PB152232BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK232

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039521.D
Acq On : 20 Apr 2023 11:15
Operator : CG/JU
Sample : PB152232BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK232

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------