

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039525.D
 Acq On : 20 Apr 2023 15:14
 Operator : CG/JU
 Sample : PB152230BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK230

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	26	30	37	rBV	67736	85535	1.56%	0.148%
2	3.637	99	102	125	rBV	722366	1164132	21.18%	2.013%
3	3.966	155	158	163	rVB	15095	20325	0.37%	0.035%
4	7.007	668	675	695	rBV	756402	1481756	26.96%	2.563%
5	7.160	695	701	720	rVB	758292	1298202	23.62%	2.245%
6	7.354	728	734	755	rBV	917737	1599283	29.10%	2.766%
7	7.825	807	814	833	rBV	711345	1256108	22.85%	2.172%
8	8.554	931	938	961	rBV	989249	1959582	35.65%	3.389%
9	8.995	1006	1013	1032	rBV	867442	1582376	28.79%	2.737%
10	9.719	1129	1136	1158	rBV	721112	1356896	24.69%	2.347%
11	10.266	1222	1229	1257	rBV	915360	1937282	35.25%	3.350%
12	10.631	1284	1291	1304	rBV	1109227	1909964	34.75%	3.303%
13	10.784	1310	1317	1347	rBV	863972	1973417	35.91%	3.413%
14	12.254	1563	1567	1570	rBV5	5976	11372	0.21%	0.020%
15	13.377	1753	1758	1764	rBV7	7663	12555	0.23%	0.022%
16	13.895	1839	1846	1862	rBV	2223860	3302608	60.09%	5.712%
17	14.172	1886	1893	1913	rBV	2442208	3911856	71.18%	6.765%
18	14.477	1938	1945	1963	rBV	1731931	2713641	49.37%	4.693%
19	14.724	1980	1987	2015	rBV	232662	882755	16.06%	1.527%
20	15.477	2108	2115	2132	rBV	3224793	4770606	86.80%	8.251%
21	15.613	2132	2138	2152	rBV	707954	1210381	22.02%	2.093%
22	17.024	2373	2378	2383	rBV4	4768	8100	0.15%	0.014%
23	17.230	2407	2413	2424	rBV	2152617	3134518	57.03%	5.421%
24	17.330	2424	2430	2455	rVB	3316232	5033884	91.59%	8.706%
25	19.195	2743	2747	2752	rBV2	34517	49590	0.90%	0.086%
26	19.271	2756	2760	2764	rBV	26656	38379	0.70%	0.066%
27	19.630	2815	2821	2839	rBV	4036629	5496055	100.00%	9.505%
28	21.424	3121	3126	3140	rBV	1772490	2674170	48.66%	4.625%
29	23.636	3495	3502	3520	rBV2	2069469	4482352	81.56%	7.752%
30	23.789	3522	3528	3545	rVB2	1108626	2464132	44.83%	4.262%




Sum of corrected areas: 57821812

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039525.D
Acq On : 20 Apr 2023 15:14
Operator : CG/JU
Sample : PB152230BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK230

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

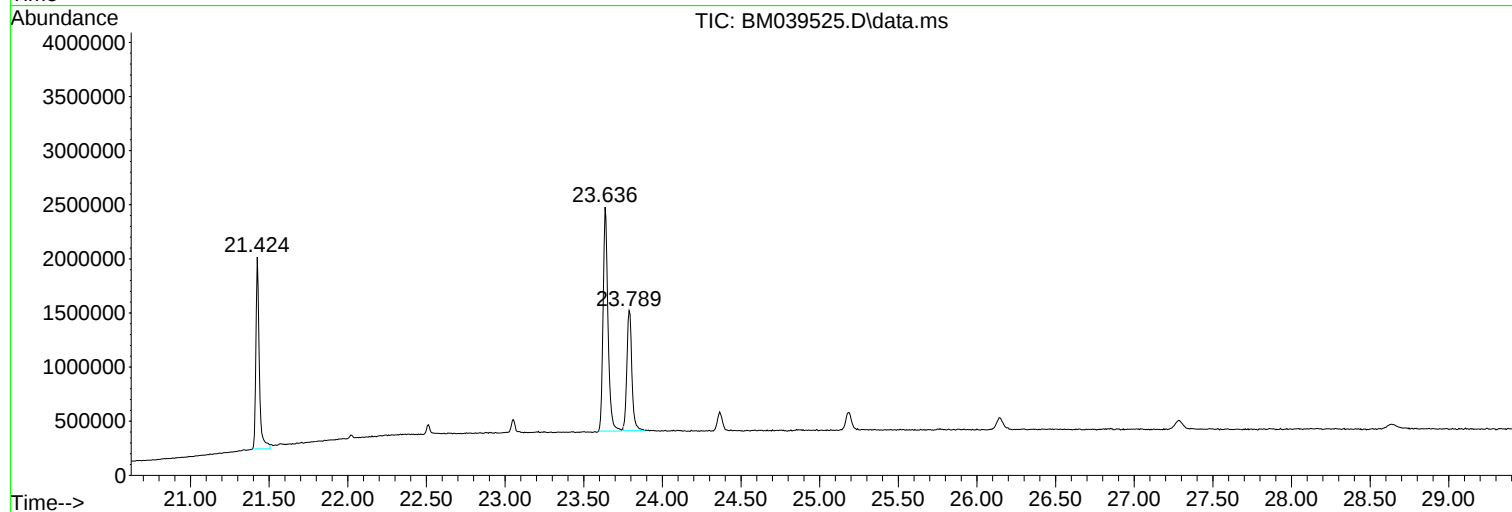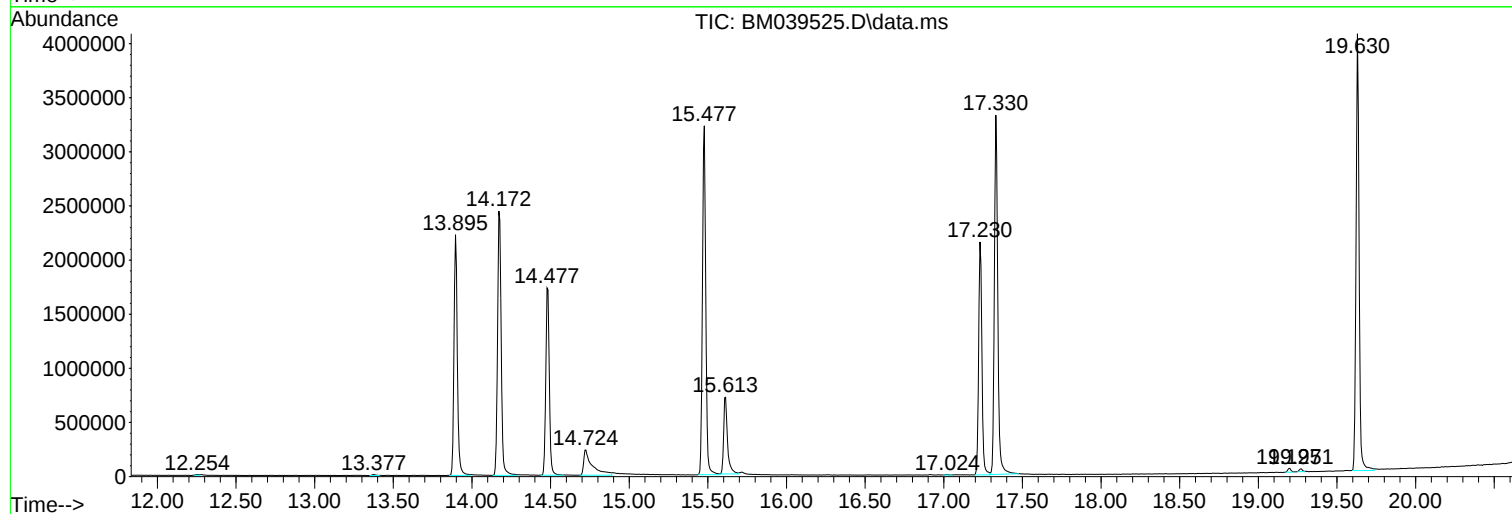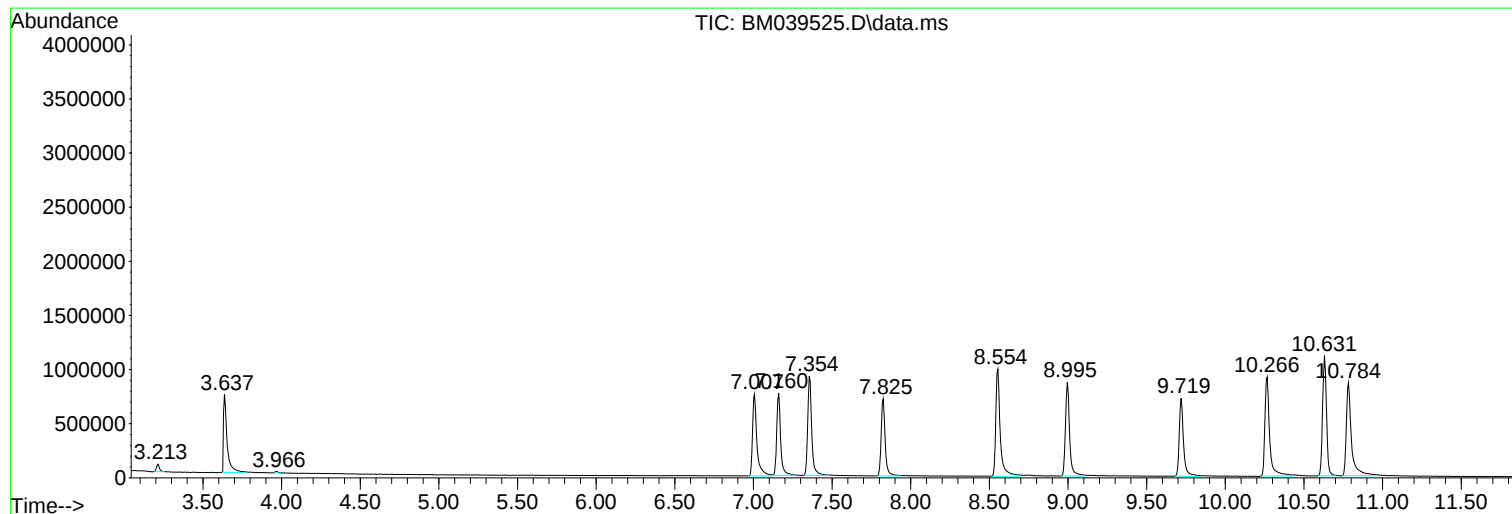

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039525.D
Acq On : 20 Apr 2023 15:14
Operator : CG/JU
Sample : PB152230BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK230

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039525.D
Acq On : 20 Apr 2023 15:14
Operator : CG/JU
Sample : PB152230BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK230

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc