

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039534.D
 Acq On : 20 Apr 2023 20:49
 Operator : CG/JU
 Sample : 02340-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.178	20	24	27	rBV	76419	100267	2.02%	0.211%
2	3.213	27	30	34	rVV	49798	68653	1.38%	0.144%
3	3.249	34	36	43	rVB	30740	36373	0.73%	0.076%
4	3.649	101	104	118	rBV	121692	221559	4.47%	0.465%
5	3.966	155	158	165	rVB	15227	21489	0.43%	0.045%
6	4.501	243	249	258	rVB	182821	279191	5.63%	0.586%
7	7.007	669	675	690	rBV	106501	270320	5.45%	0.568%
8	7.154	694	700	713	rBV	614027	1079925	21.78%	2.269%
9	7.354	728	734	754	rBV	569709	1026576	20.70%	2.156%
10	7.825	806	814	825	rBV	605119	1099518	22.17%	2.310%
11	8.554	932	938	963	rBV	383810	850255	17.15%	1.786%
12	8.995	1006	1013	1032	rBV	739237	1382683	27.88%	2.905%
13	9.719	1129	1136	1153	rBV	553898	1070030	21.58%	2.248%
14	10.266	1222	1229	1252	rBV	668631	1489323	30.03%	3.129%
15	10.630	1284	1291	1306	rBV	979979	1705048	34.38%	3.582%
16	10.783	1310	1317	1339	rBV	358986	892449	18.00%	1.875%
17	11.507	1434	1440	1443	rBV7	3448	6862	0.14%	0.014%
18	12.242	1558	1565	1574	rBV3	10558	26319	0.53%	0.055%
19	13.377	1750	1758	1763	rVV	31575	52728	1.06%	0.111%
20	13.454	1767	1771	1776	rVB8	3628	6388	0.13%	0.013%
21	13.895	1839	1846	1863	rBV	2137102	3042225	61.35%	6.391%
22	14.171	1886	1893	1911	rBV	2325214	3560169	71.79%	7.479%
23	14.477	1938	1945	1958	rBV	1618609	2484826	50.11%	5.220%
24	14.783	1988	1997	2001	rBV7	13385	43560	0.88%	0.092%
25	15.177	2059	2064	2068	rVB5	4191	7008	0.14%	0.015%
26	15.477	2106	2115	2131	rBV	2802346	4412553	88.98%	9.269%
27	15.613	2132	2138	2152	rVV	598855	1042622	21.02%	2.190%
28	15.712	2153	2155	2161	rVB4	16840	29157	0.59%	0.061%
29	15.848	2173	2178	2185	rBV	36938	55122	1.11%	0.116%
30	16.042	2209	2211	2218	rVB8	3495	5051	0.10%	0.011%
31	16.265	2243	2249	2252	rBV7	3864	6524	0.13%	0.014%
32	16.412	2270	2274	2279	rBV8	3274	5133	0.10%	0.011%
33	16.912	2357	2359	2362	rVB4	5190	4996	0.10%	0.010%
34	17.018	2374	2377	2384	rBV6	4409	8555	0.17%	0.018%
35	17.230	2407	2413	2424	rBV	1907344	2741628	55.29%	5.759%
36	17.330	2424	2430	2458	rVB2	3029486	4615322	93.07%	9.695%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039534.D
 Acq On : 20 Apr 2023 20:49
 Operator : CG/JU
 Sample : 02340-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	17.901	2523	2527	2532	rBV7	13986	22027	0.44%	0.046%
38	18.130	2562	2566	2571	rBV4	25866	45384	0.92%	0.095%
39	18.989	2708	2712	2715	rBV2	19550	26954	0.54%	0.057%
40	19.195	2743	2747	2752	rBV2	37286	50057	1.01%	0.105%
41	19.265	2755	2759	2765	rBV	33110	59733	1.20%	0.125%
42	19.418	2782	2785	2789	rBV6	11942	19392	0.39%	0.041%
43	19.553	2805	2808	2812	rBV4	16886	23643	0.48%	0.050%
44	19.630	2815	2821	2833	rBV	3550007	4959078	100.00%	10.417%
45	21.424	3121	3126	3140	rBV	1600782	2365889	47.71%	4.970%
46	23.636	3495	3502	3518	rBV2	1896987	4076487	82.20%	8.563%
47	23.788	3522	3528	3544	rVB2	1003299	2205132	44.47%	4.632%




Sum of corrected areas: 47604183

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039534.D
Acq On : 20 Apr 2023 20:49
Operator : CG/JU
Sample : 02340-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

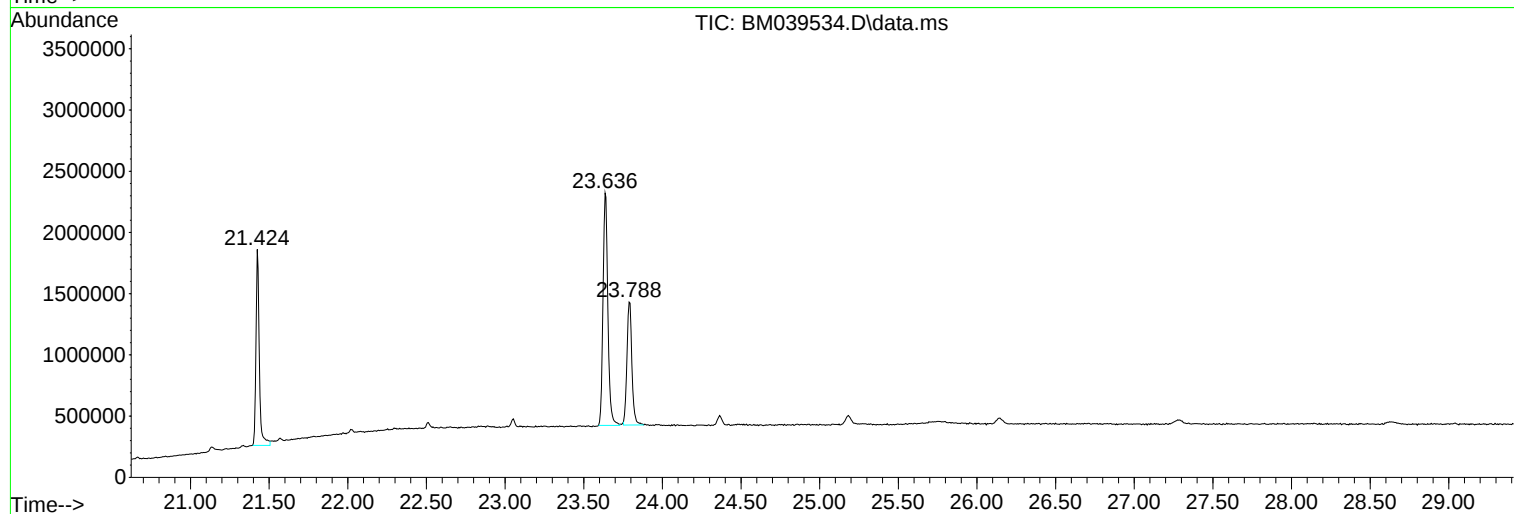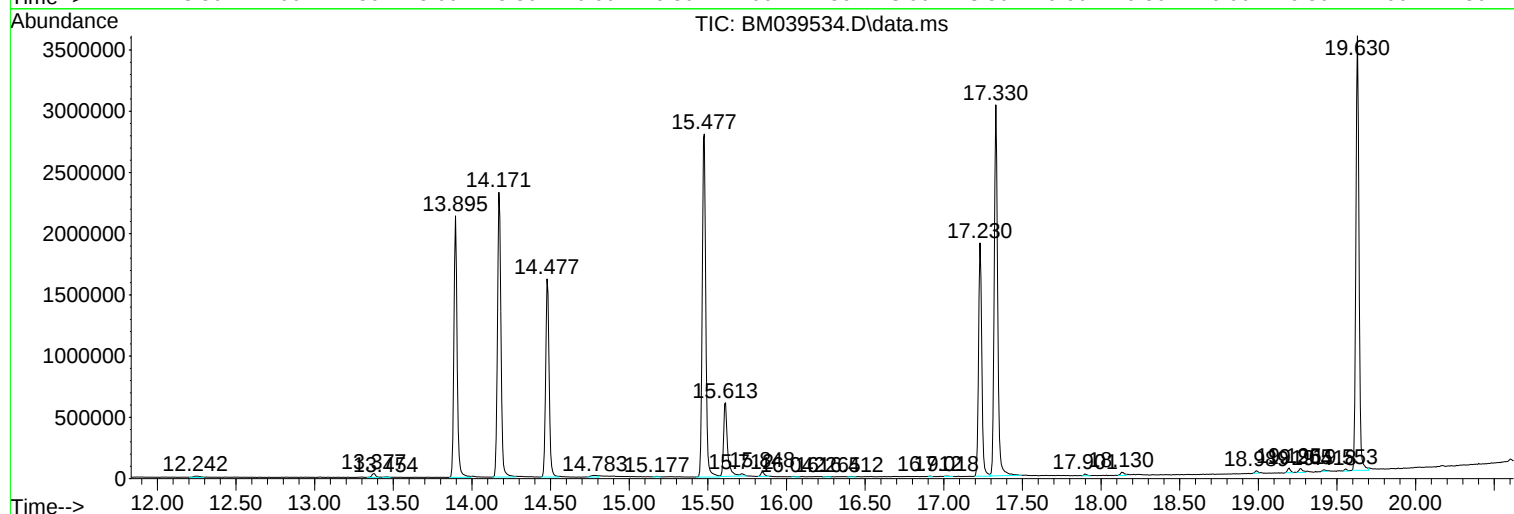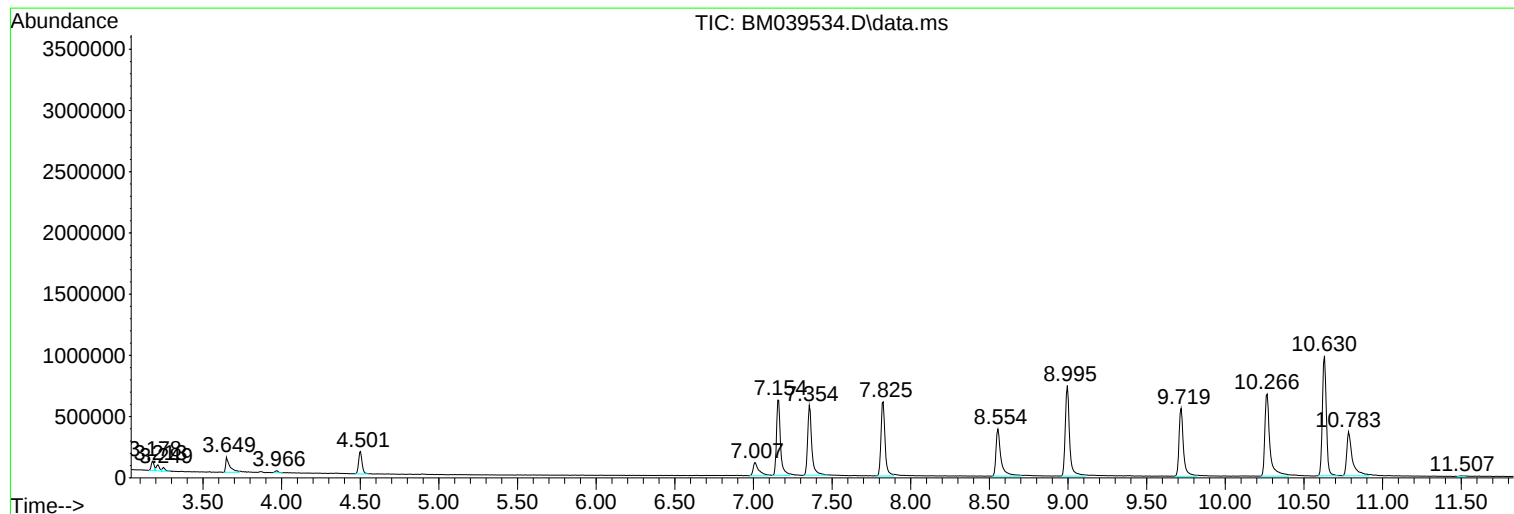

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039534.D
Acq On : 20 Apr 2023 20:49
Operator : CG/JU
Sample : 02340-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039534.D
Acq On : 20 Apr 2023 20:49
Operator : CG/JU
Sample : 02340-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc