

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039535.D
 Acq On : 20 Apr 2023 21:25
 Operator : CG/JU
 Sample : 02340-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039535.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.178	20	24	28	rBV	118664	170169	3.46%	0.357%
2	3.213	28	30	33	rVV	49679	56058	1.14%	0.118%
3	3.249	33	36	43	rVB	37915	51289	1.04%	0.108%
4	3.649	102	104	122	rBV	97724	197567	4.01%	0.415%
5	3.966	154	158	164	rVB2	17082	26381	0.54%	0.055%
6	4.501	243	249	260	rBV	517363	789517	16.03%	1.657%
7	7.007	670	675	693	rBV	96848	245992	5.00%	0.516%
8	7.154	694	700	722	rVV	575598	1037911	21.08%	2.178%
9	7.354	728	734	754	rBV	546697	997831	20.26%	2.094%
10	7.825	807	814	833	rBV	642652	1186323	24.09%	2.489%
11	8.554	932	938	956	rBV	365608	793831	16.12%	1.666%
12	8.995	1006	1013	1029	rBV	687600	1301476	26.43%	2.731%
13	9.383	1074	1079	1084	rVB5	6497	12611	0.26%	0.026%
14	9.719	1129	1136	1151	rBV	518283	1004533	20.40%	2.108%
15	10.266	1220	1229	1251	rBV	654781	1457140	29.59%	3.058%
16	10.630	1283	1291	1309	rBV	1052486	1851322	37.60%	3.885%
17	10.783	1309	1317	1335	rBV	288807	738079	14.99%	1.549%
18	12.248	1557	1566	1572	rBV7	7199	18868	0.38%	0.040%
19	13.377	1751	1758	1766	rVV2	18234	32983	0.67%	0.069%
20	13.454	1768	1771	1778	rVB7	3456	6426	0.13%	0.013%
21	13.895	1838	1846	1862	rBV	2112202	2987941	60.68%	6.270%
22	14.171	1885	1893	1917	rBV	2270274	3456797	70.20%	7.254%
23	14.377	1924	1928	1935	rVB9	4191	7544	0.15%	0.016%
24	14.477	1938	1945	1962	rBV	1714021	2621843	53.24%	5.502%
25	14.777	1990	1996	2002	rBV5	11161	35221	0.72%	0.074%
26	15.265	2073	2079	2084	rVB6	4505	6494	0.13%	0.014%
27	15.477	2108	2115	2132	rBV	2746677	4275963	86.83%	8.973%
28	15.612	2132	2138	2150	rVV	464051	821122	16.67%	1.723%
29	15.718	2153	2156	2162	rVB4	14786	26546	0.54%	0.056%
30	15.848	2172	2178	2189	rVB	74527	126172	2.56%	0.265%
31	16.042	2208	2211	2218	rBV7	3091	6621	0.13%	0.014%
32	16.912	2356	2359	2363	rBV6	4219	5643	0.11%	0.012%
33	17.018	2375	2377	2384	rVB5	4837	8734	0.18%	0.018%
34	17.230	2407	2413	2424	rBV	1957889	2895928	58.81%	6.077%
35	17.330	2424	2430	2449	rVB	2937658	4455599	90.48%	9.350%
36	18.142	2565	2568	2570	rBV4	6920	9412	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039535.D
 Acq On : 20 Apr 2023 21:25
 Operator : CG/JU
 Sample : 02340-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	18.553	2635	2638	2643	rVB5	11364	11600	0.24%	0.024%
38	18.989	2710	2712	2715	rBV4	6453	7451	0.15%	0.016%
39	19.195	2743	2747	2753	rBV	39555	57473	1.17%	0.121%
40	19.265	2755	2759	2765	rBV	29484	49394	1.00%	0.104%
41	19.553	2806	2808	2811	rVB4	12613	12235	0.25%	0.026%
42	19.630	2815	2821	2842	rVV	3556606	4924352	100.00%	10.334%
43	21.136	3073	3077	3086	rBV3	108606	255047	5.18%	0.535%
44	21.424	3121	3126	3137	rBV	1676910	2382814	48.39%	5.000%
45	23.635	3495	3502	3518	rBV2	1921862	3965036	80.52%	8.321%
46	23.788	3521	3528	3540	rVV2	1056073	2263996	45.98%	4.751%




Sum of corrected areas: 47653285

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039535.D
Acq On : 20 Apr 2023 21:25
Operator : CG/JU
Sample : 02340-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

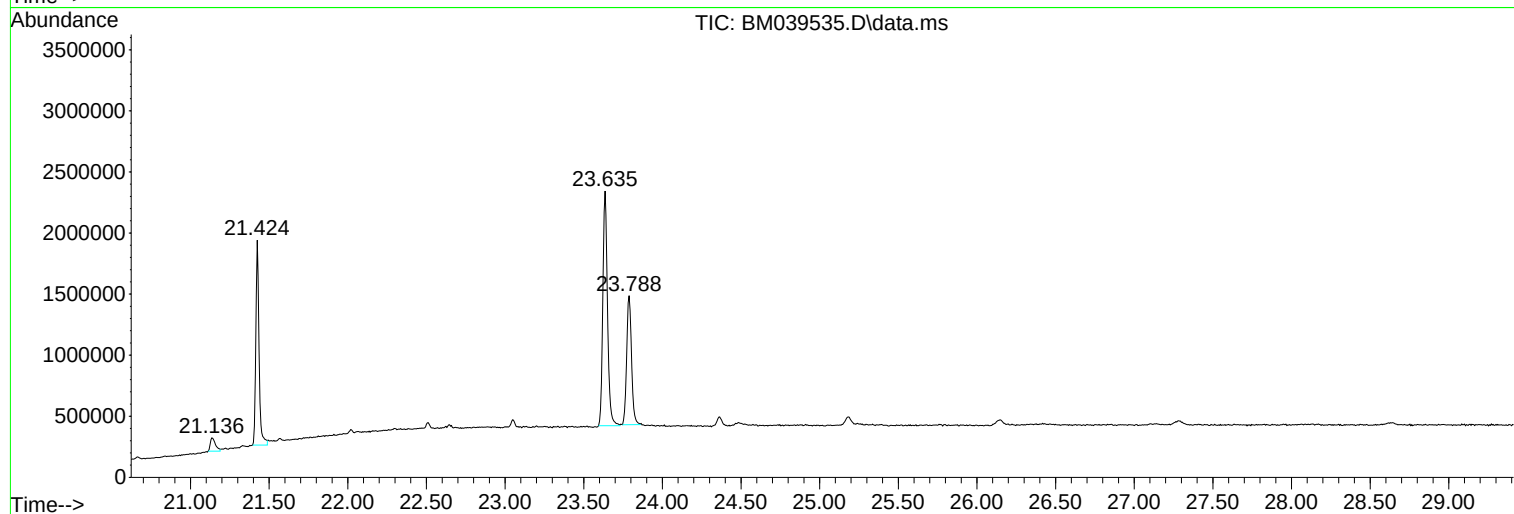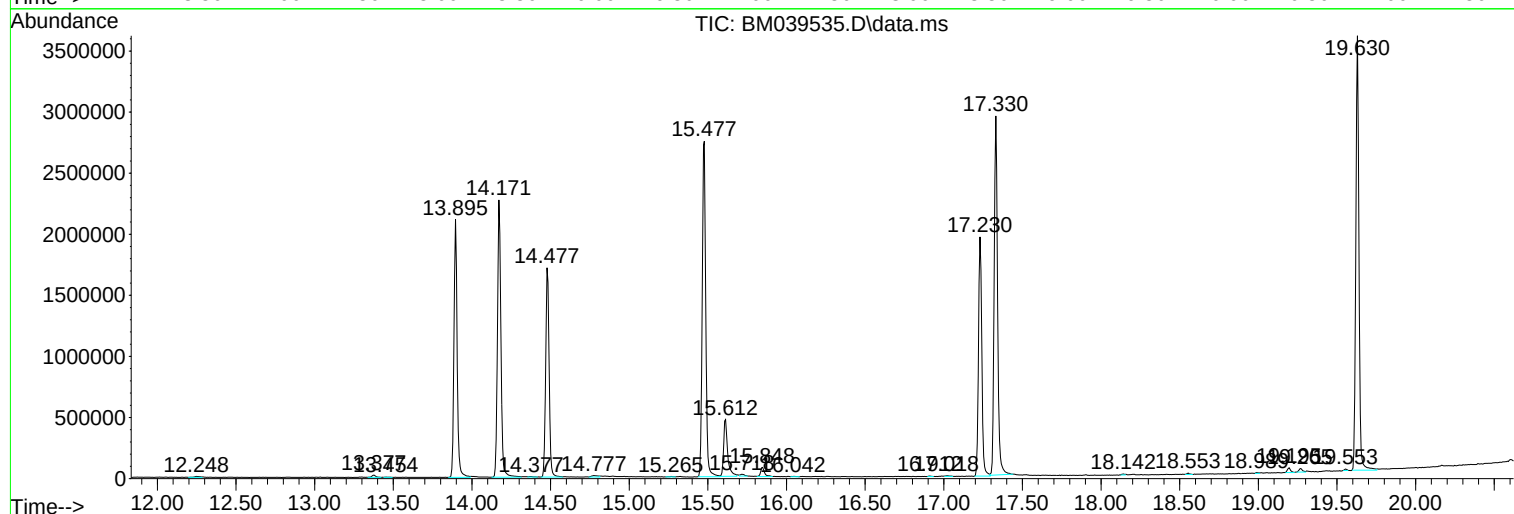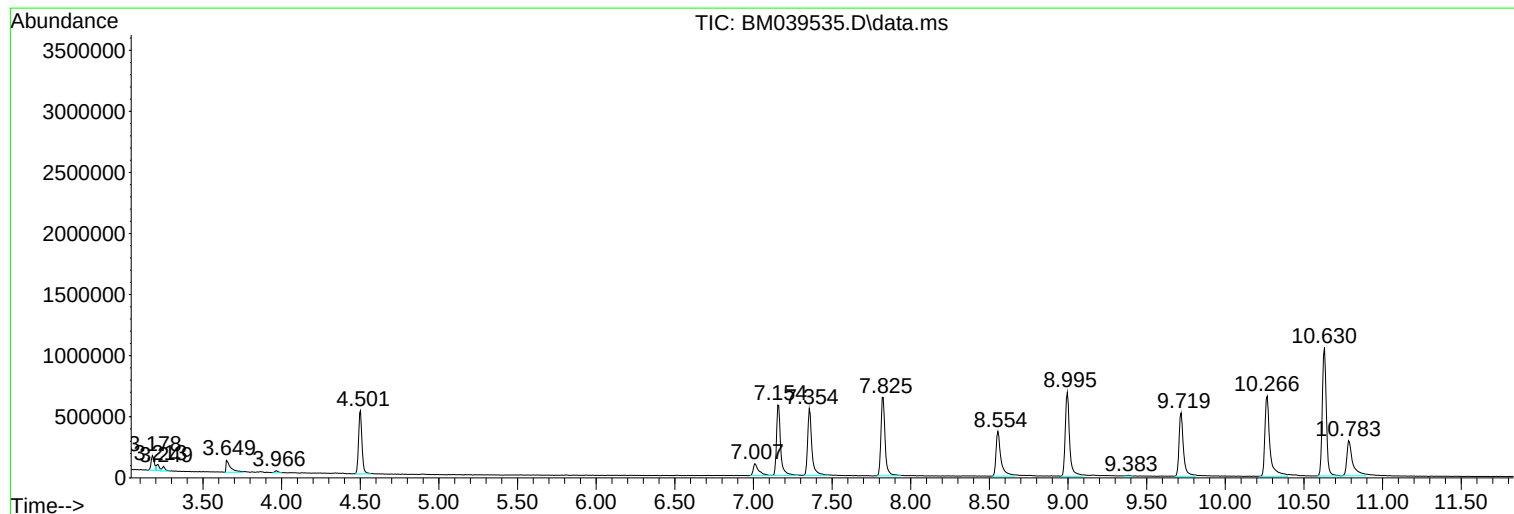

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039535.D
Acq On : 20 Apr 2023 21:25
Operator : CG/JU
Sample : 02340-13
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
BHE14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.136	2.14 ng/ul	255047	Chrysene-d12		21.424	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Nonadecene		266	C19H38	018435-45-5	96
2	Dichloroacetic acid, heptadecyl ...		366	C19H36Cl2O2	1000282-98-2	94
3	Heptadecyl heptafluorobutyrate		452	C21H35F7O2	959085-66-6	94
4	Heptafluorobutyric acid, pentade...		424	C19H31F7O2	959261-23-5	94
5	1-Tetracosene		336	C24H48	010192-32-2	94

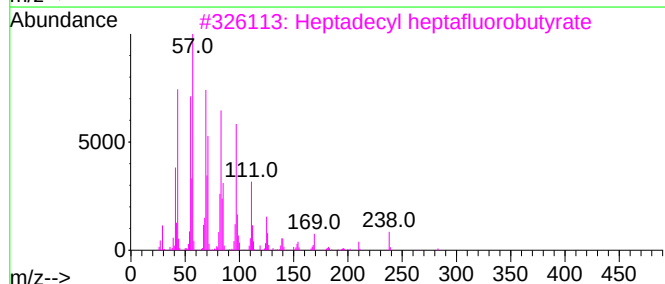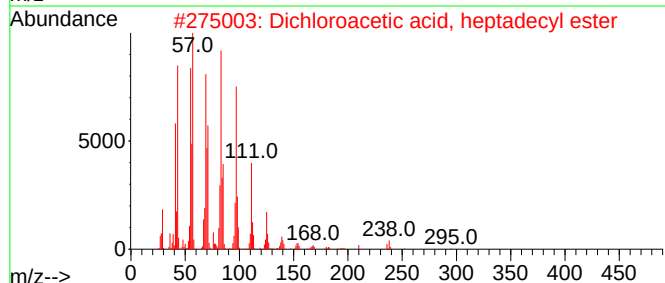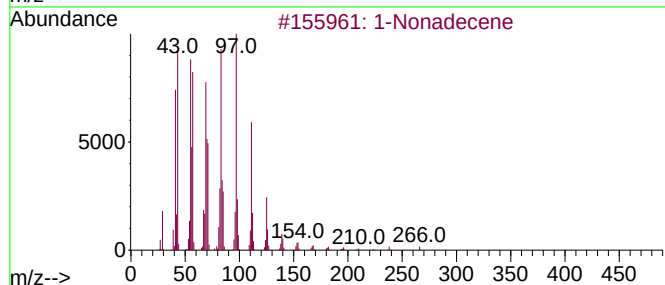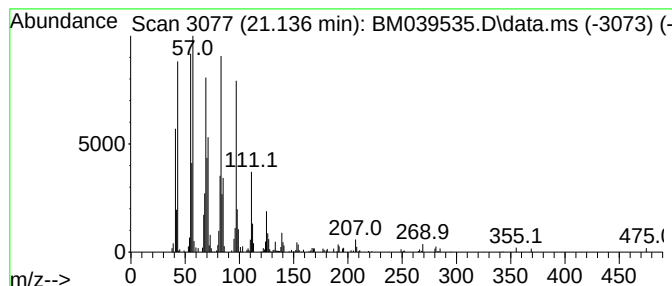

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039535.D
Acq On : 20 Apr 2023 21:25
Operator : CG/JU
Sample : 02340-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.136	2.1	ng/u1	255047	5	21.424	2382810	20.0