

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039536.D
 Acq On : 20 Apr 2023 22:01
 Operator : CG/JU
 Sample : 02340-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	27	30	39	rVB	46796	66033	1.17%	0.130%
2	3.660	104	106	125	rBV	43213	90670	1.60%	0.179%
3	3.966	155	158	166	rVB	14580	22271	0.39%	0.044%
4	4.501	245	249	254	rVB4	13796	22689	0.40%	0.045%
5	7.007	669	675	693	rBV	94289	240960	4.26%	0.476%
6	7.160	694	701	723	rVV	621717	1109788	19.62%	2.192%
7	7.354	728	734	757	rVV	577920	1058793	18.72%	2.091%
8	7.819	807	813	837	rBV	658460	1194459	21.11%	2.359%
9	8.554	931	938	955	rBV	377717	791781	14.00%	1.564%
10	8.995	1006	1013	1027	rBV	734353	1370769	24.23%	2.707%
11	9.719	1128	1136	1152	rBV	599457	1139170	20.14%	2.250%
12	10.260	1222	1228	1245	rBV	706528	1558566	27.55%	3.078%
13	10.630	1283	1291	1306	rBV	1084492	1869973	33.05%	3.693%
14	10.789	1311	1318	1338	rBV	242093	647968	11.45%	1.280%
15	12.242	1559	1565	1569	rBV3	9209	17941	0.32%	0.035%
16	13.377	1752	1758	1764	rBV2	13160	22808	0.40%	0.045%
17	13.895	1840	1846	1858	rBV	2131139	3158501	55.83%	6.238%
18	14.171	1887	1893	1916	rBV	2479772	3695864	65.33%	7.299%
19	14.371	1924	1927	1933	rVB6	4033	7476	0.13%	0.015%
20	14.477	1938	1945	1960	rBV	1804548	2695831	47.65%	5.324%
21	14.783	1989	1997	2001	rBV10	13873	41000	0.72%	0.081%
22	15.271	2073	2080	2084	rBV4	5524	9312	0.16%	0.018%
23	15.477	2108	2115	2132	rBV	3030483	4610419	81.50%	9.105%
24	15.607	2132	2137	2152	rVV	764292	1257086	22.22%	2.483%
25	15.718	2153	2156	2166	rVB3	18874	35344	0.62%	0.070%
26	15.848	2173	2178	2188	rVB	56675	95414	1.69%	0.188%
27	16.912	2354	2359	2362	rBV6	4750	7001	0.12%	0.014%
28	17.230	2407	2413	2424	rBV	2118129	3095695	54.72%	6.114%
29	17.330	2424	2430	2447	rVB	3426510	5009606	88.55%	9.894%
30	17.901	2522	2527	2531	rBV6	4908	8146	0.14%	0.016%
31	18.130	2561	2566	2575	rBV2	65156	128448	2.27%	0.254%
32	19.195	2742	2747	2754	rBV2	44682	74430	1.32%	0.147%
33	19.265	2755	2759	2764	rBV	38828	62302	1.10%	0.123%
34	19.412	2780	2784	2792	rBV3	36034	68458	1.21%	0.135%
35	19.553	2805	2808	2813	rBV4	19329	21093	0.37%	0.042%
36	19.630	2815	2821	2836	rBV	4040859	5657241	100.00%	11.173%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039536.D
Acq On : 20 Apr 2023 22:01
Operator : CG/JU
Sample : 02340-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE15

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	20.600	2984	2986	2989	rBV2	24506	26020	0.46%	0.051%
38	21.136	3073	3077	3086	rBV3	105645	239481	4.23%	0.473%
39	21.424	3121	3126	3136	rBV	1857483	2629552	46.48%	5.193%
40	23.635	3495	3502	3515	rBV2	2127253	4323810	76.43%	8.539%
41	23.788	3521	3528	3544	rVB2	1153193	2452940	43.36%	4.844%




Sum of corrected areas: 50635109

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039536.D
Acq On : 20 Apr 2023 22:01
Operator : CG/JU
Sample : 02340-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

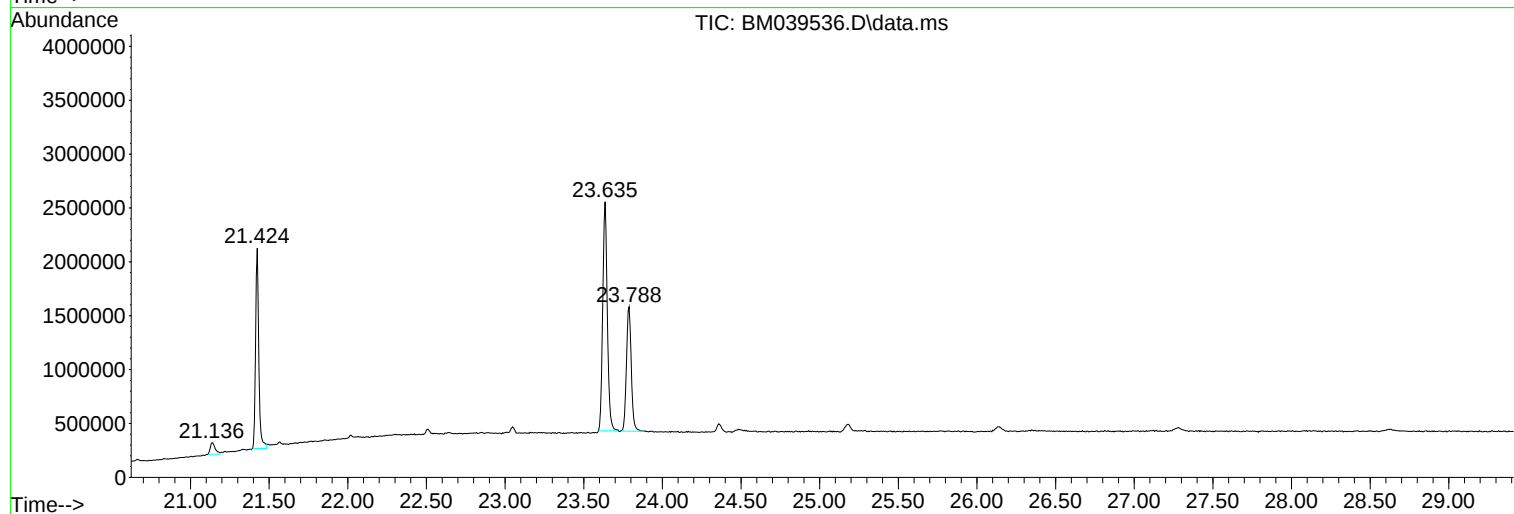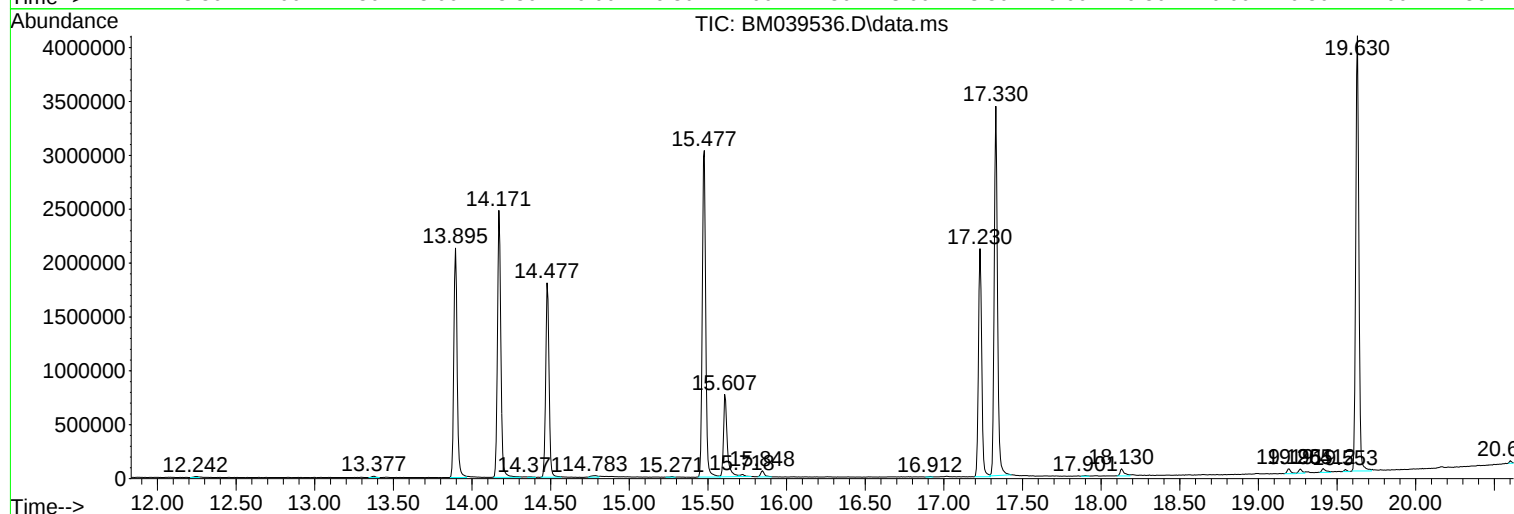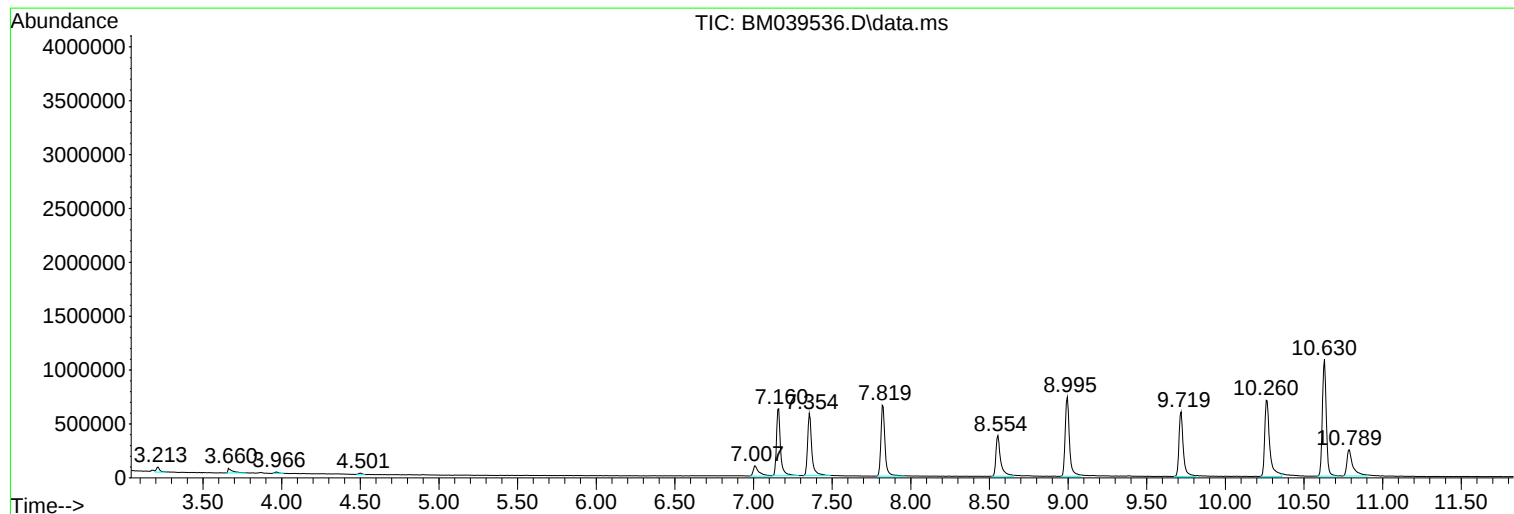

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039536.D
Acq On : 20 Apr 2023 22:01
Operator : CG/JU
Sample : 02340-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039536.D
Acq On : 20 Apr 2023 22:01
Operator : CG/JU
Sample : 02340-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc