

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
 Data File : BM039541.D
 Acq On : 21 Apr 2023 01:00
 Operator : CG/JU
 Sample : PB152246BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.213	26	30	40	rVB	67225	101729	1.77%	0.169%
2	3.637	99	102	128	rBV	580648	1008791	17.57%	1.673%
3	3.966	155	158	163	rVB	12987	17381	0.30%	0.029%
4	7.001	668	674	694	rBV	813849	1523198	26.53%	2.526%
5	7.154	694	700	723	rVV	767403	1326161	23.10%	2.199%
6	7.354	727	734	755	rBV	937348	1644154	28.63%	2.727%
7	7.819	806	813	828	rBV	758906	1322215	23.03%	2.193%
8	8.548	930	937	961	rBV	1065831	2039880	35.53%	3.383%
9	8.995	1006	1013	1038	rBV	861275	1629204	28.37%	2.702%
10	9.719	1129	1136	1153	rBV	727851	1378927	24.02%	2.287%
11	10.260	1219	1228	1258	rBV	997148	2075236	36.14%	3.441%
12	10.631	1283	1291	1304	rVV	1186137	2081427	36.25%	3.452%
13	10.783	1309	1317	1350	rVV	593638	1430193	24.91%	2.372%
14	12.260	1560	1568	1578	rBV5	9064	27941	0.49%	0.046%
15	13.372	1752	1757	1768	rBV	33916	58655	1.02%	0.097%
16	13.895	1839	1846	1861	rBV	2355762	3403857	59.28%	5.645%
17	14.171	1886	1893	1914	rBV	2750950	4084392	71.13%	6.773%
18	14.477	1937	1945	1955	rBV	2020315	3001077	52.27%	4.977%
19	14.719	1980	1986	2014	rBV	297003	1026164	17.87%	1.702%
20	15.471	2108	2114	2132	rBV	3327346	5002472	87.12%	8.296%
21	15.607	2132	2137	2151	rVV	822604	1324511	23.07%	2.196%
22	15.713	2152	2155	2165	rVB2	21976	41831	0.73%	0.069%
23	16.907	2353	2358	2363	rBV6	4175	8094	0.14%	0.013%
24	17.230	2406	2413	2424	rBV	2412707	3474603	60.51%	5.762%
25	17.330	2424	2430	2457	rVB	3519696	5331142	92.85%	8.841%
26	19.195	2742	2747	2755	rBV2	39681	71960	1.25%	0.119%
27	19.271	2755	2760	2764	rBV	30981	50491	0.88%	0.084%
28	19.630	2814	2821	2838	rBV	3975393	5741899	100.00%	9.522%
29	21.424	3121	3126	3139	rBV	1869350	2824211	49.19%	4.683%
30	23.630	3494	3501	3515	rBV2	2193958	4553778	79.31%	7.552%
31	23.783	3521	3527	3541	rVB2	1270216	2696304	46.96%	4.471%




Sum of corrected areas: 60301878

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039541.D
Acq On : 21 Apr 2023 01:00
Operator : CG/JU
Sample : PB152246BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK246

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

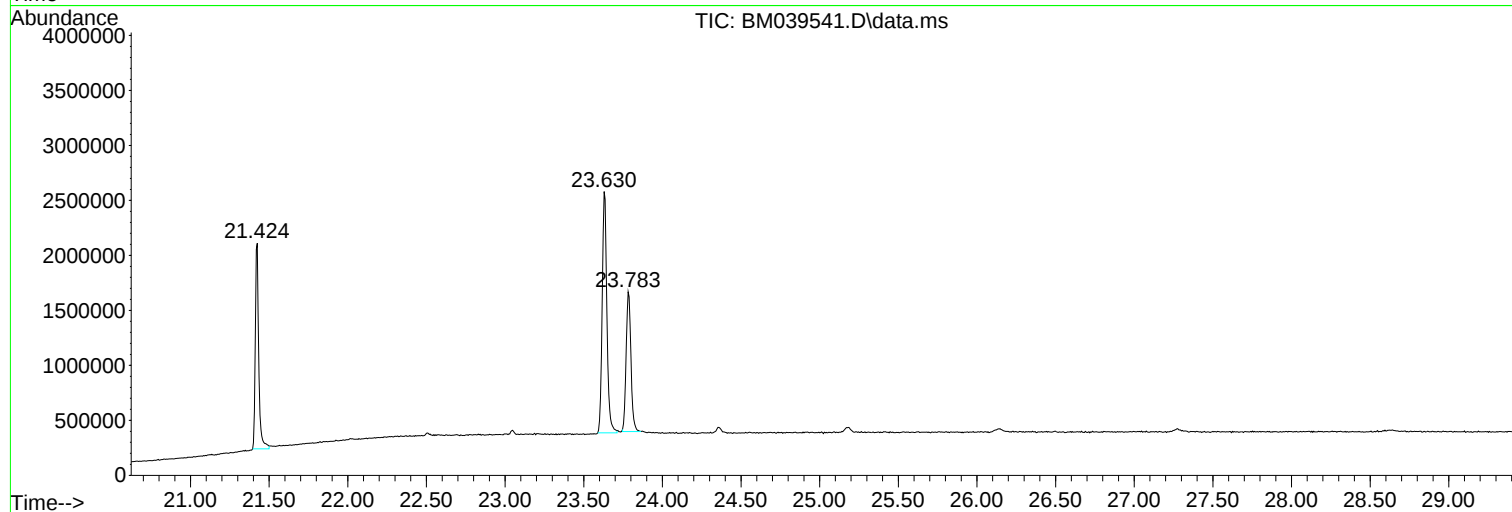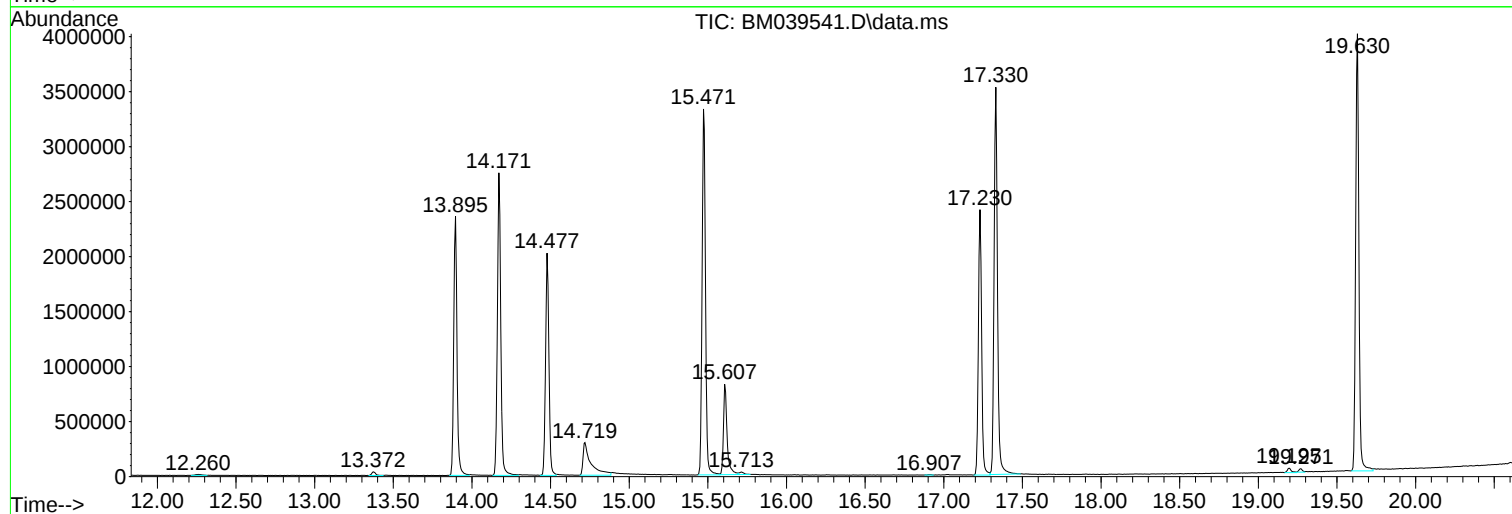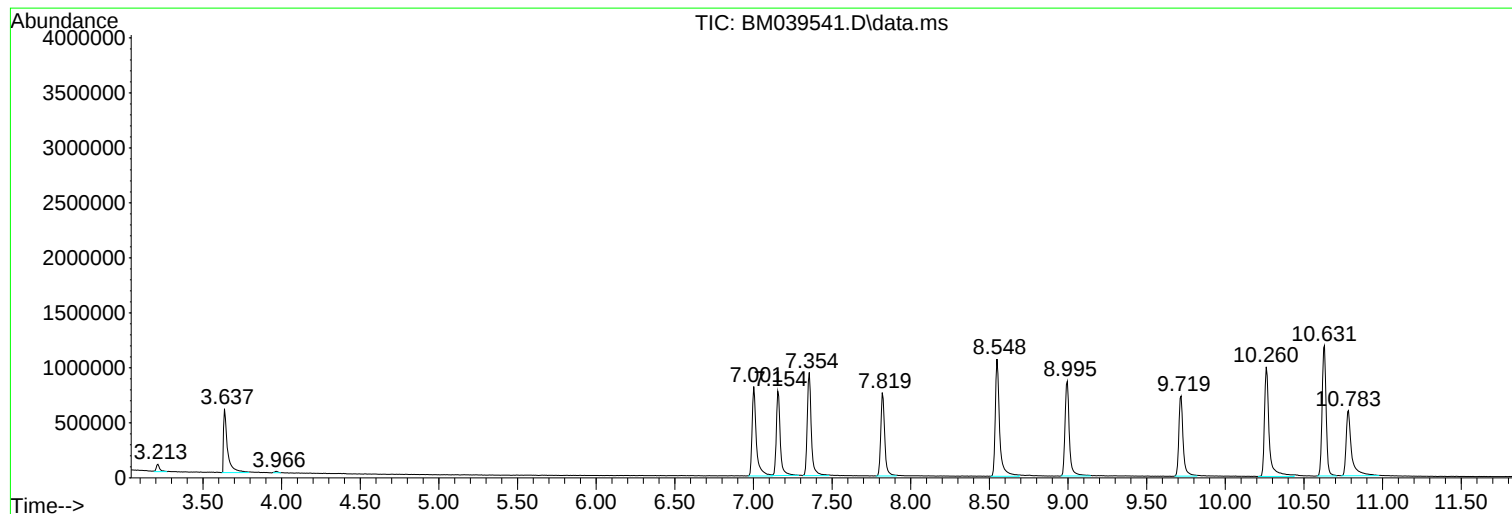

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039541.D
Acq On : 21 Apr 2023 01:00
Operator : CG/JU
Sample : PB152246BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK246

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042023\
Data File : BM039541.D
Acq On : 21 Apr 2023 01:00
Operator : CG/JU
Sample : PB152246BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK246

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc