

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
 Data File : BM045458.D
 Acq On : 21 Apr 2024 12:45
 Operator : MA/JU
 Sample : P2117-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 22 02:03:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 22 02:01:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.564	152	966	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.325	136	3109	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.210	164	1719	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.069	188	303078	0.400	ng/ul	# 0.06
17) Chrysene-d12	21.195	240	2310	0.400	ng/ul	-0.02
23) Perylene-d12	23.381	264	3371	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.167	96	4472	3.454	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.931	152	1437	0.350	ng/ul	-0.04
18) Fluoranthene-d10	19.020	212	3087	0.424	ng/ul	-0.02
Target Compounds						Qvalue
20) Pyrene	19.378	202	678	0.062	ng/ul#	1
26) Benzo(a)pyrene	23.232	252	1128	0.096	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045458.D
Acq On : 21 Apr 2024 12:45
Operator : MA/JU
Sample : P2117-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 22 02:03:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 02:01:19 2024
Response via : Initial Calibration

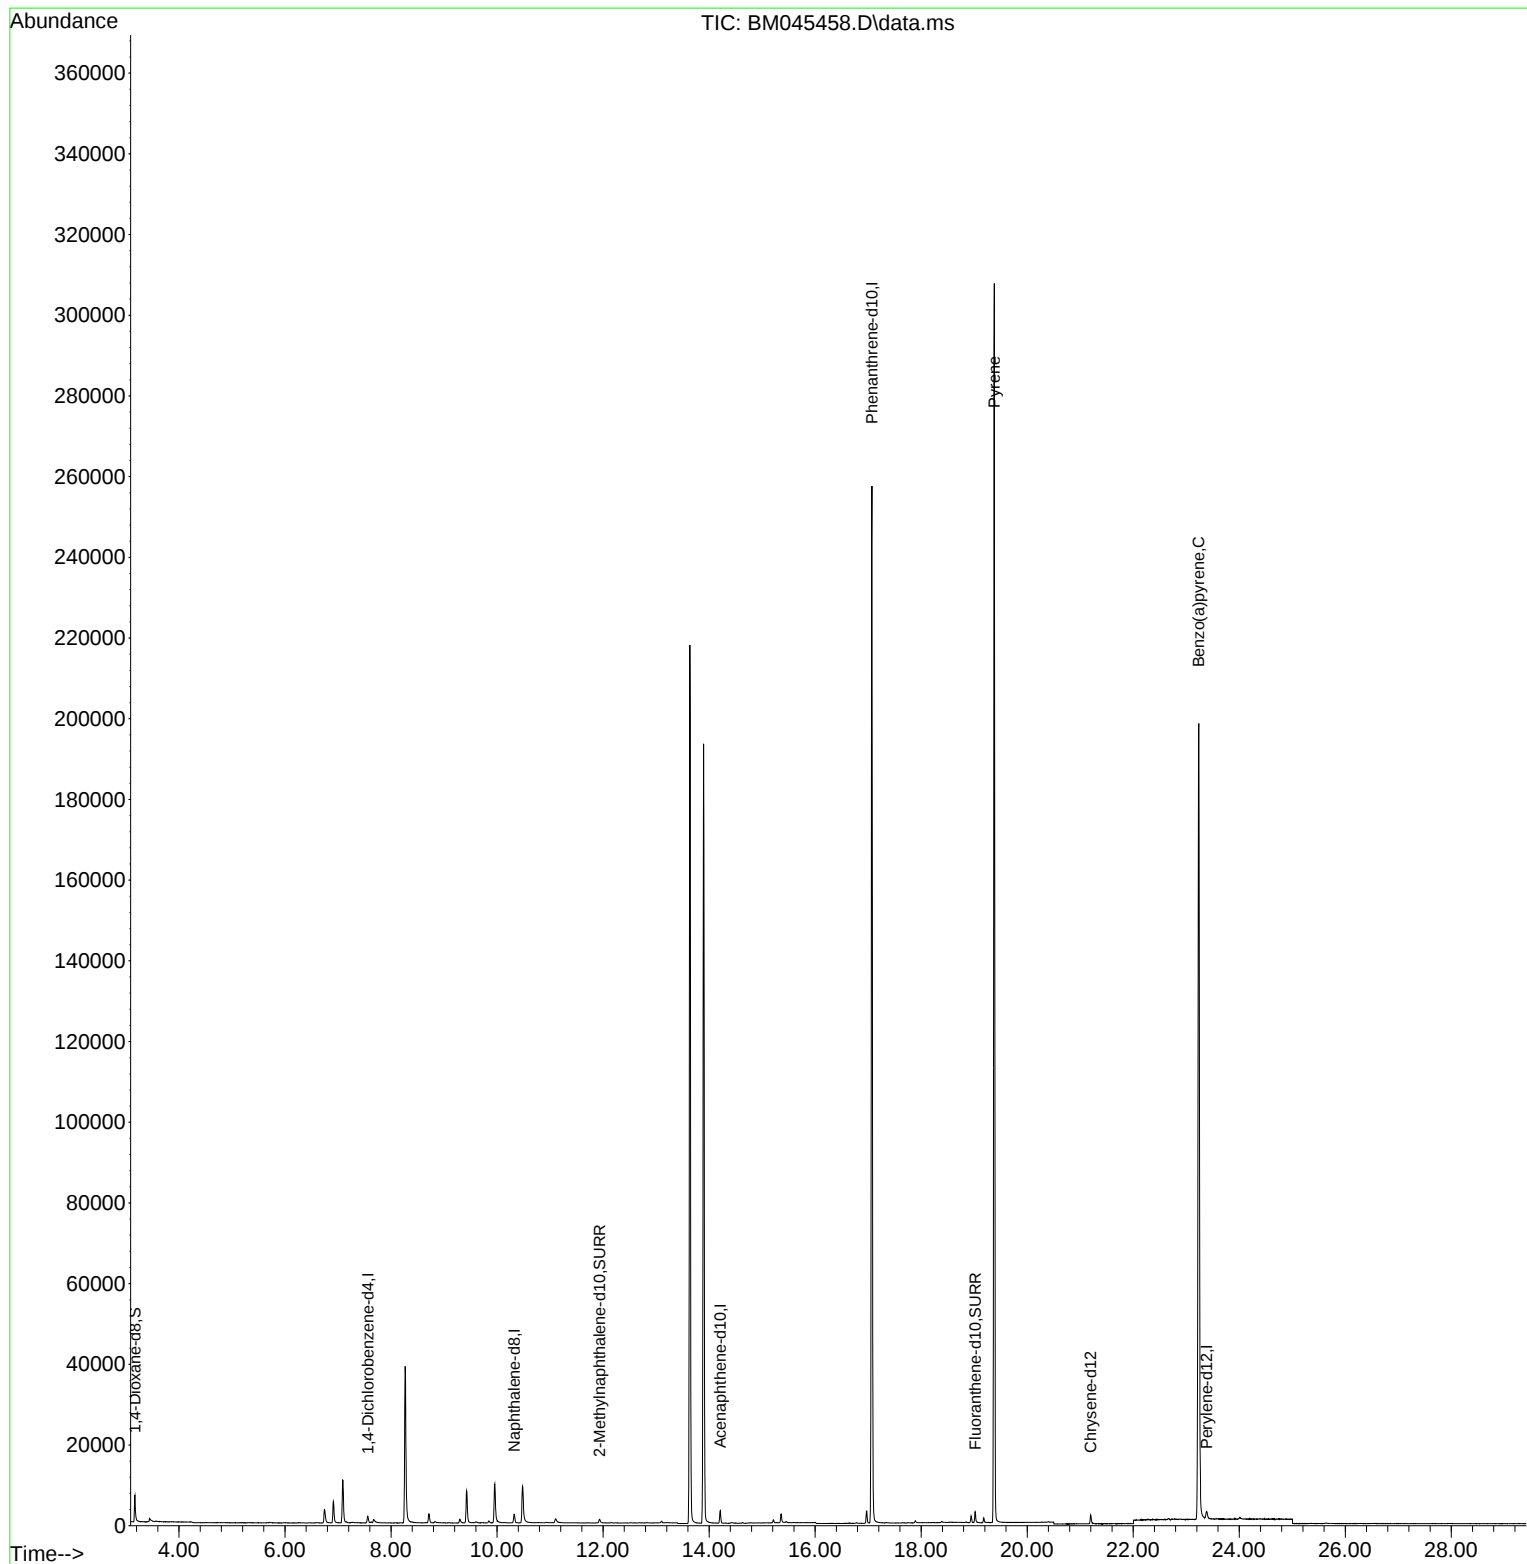

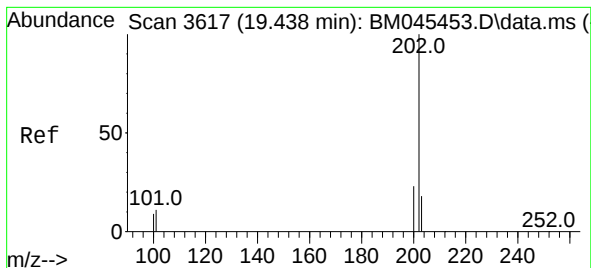

#20

Pyrene

Concen: 0.062 ng/ul

RT: 19.378 min Scan# 3

Delta R.T. -0.060 min

Lab File: BM045458.D

Acq: 21 Apr 2024 12:45





Instrument :

BNA_M

ClientSampleId :

Tgt Ion:202 Resp: 678

Ion	Ratio	Lower	Upper
202	100		
101	195.4	11.5	17.3#
100	1437.9	10.6	15.8#

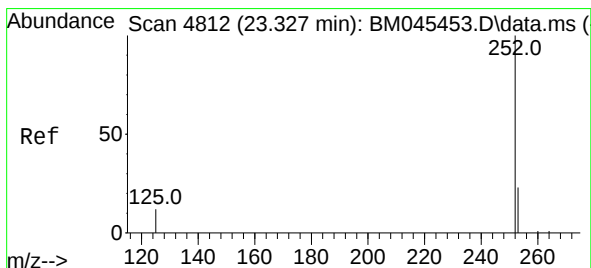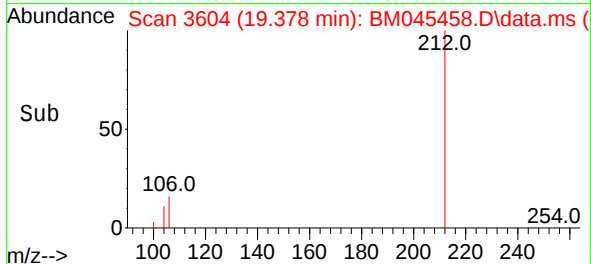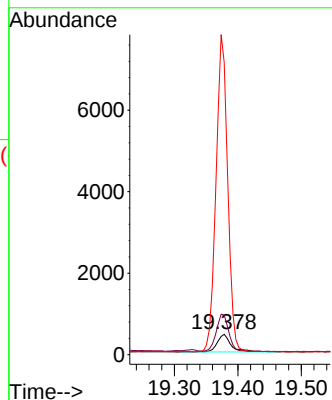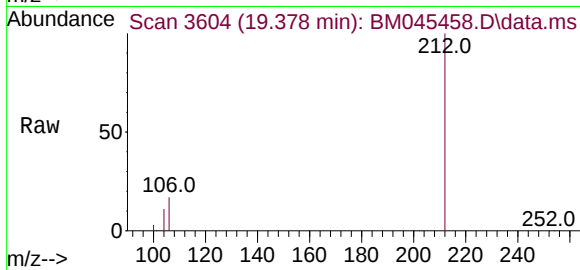

#26

Benzo(a)pyrene

Concen: 0.096 ng/ul

RT: 23.232 min Scan# 4780

Delta R.T. -0.094 min

Lab File: BM045458.D

Acq: 21 Apr 2024 12:45

Tgt Ion:252 Resp: 1128

Ion	Ratio	Lower	Upper
252	100		
253	71.7	31.6	47.4#
125	44.8	19.5	29.3#

