

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
 Data File : BM045464.D
 Acq On : 21 Apr 2024 16:21
 Operator : MA/JU
 Sample : P2140-09
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 22 02:04:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 22 02:01:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.559	152	896	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.325	136	2773	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.209	164	1448	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.068	188	285163	0.400	ng/ul	# 0.06
17) Chrysene-d12	21.213	240	1706	0.400	ng/ul	0.00
23) Perylene-d12	23.397	264	3352	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.167	96	4150	3.456	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.953	152	1592	0.435	ng/ul	-0.02
18) Fluoranthene-d10	19.015	212	2538	0.472	ng/ul	-0.03
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.209	88	87	0.075	ng/ul#	72
20) Pyrene	19.377	202	559	0.069	ng/ul#	1
26) Benzo(a)pyrene	23.233	252	1130	0.097	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045464.D
Acq On : 21 Apr 2024 16:21
Operator : MA/JU
Sample : P2140-09
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Apr 22 02:04:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 02:01:19 2024
Response via : Initial Calibration

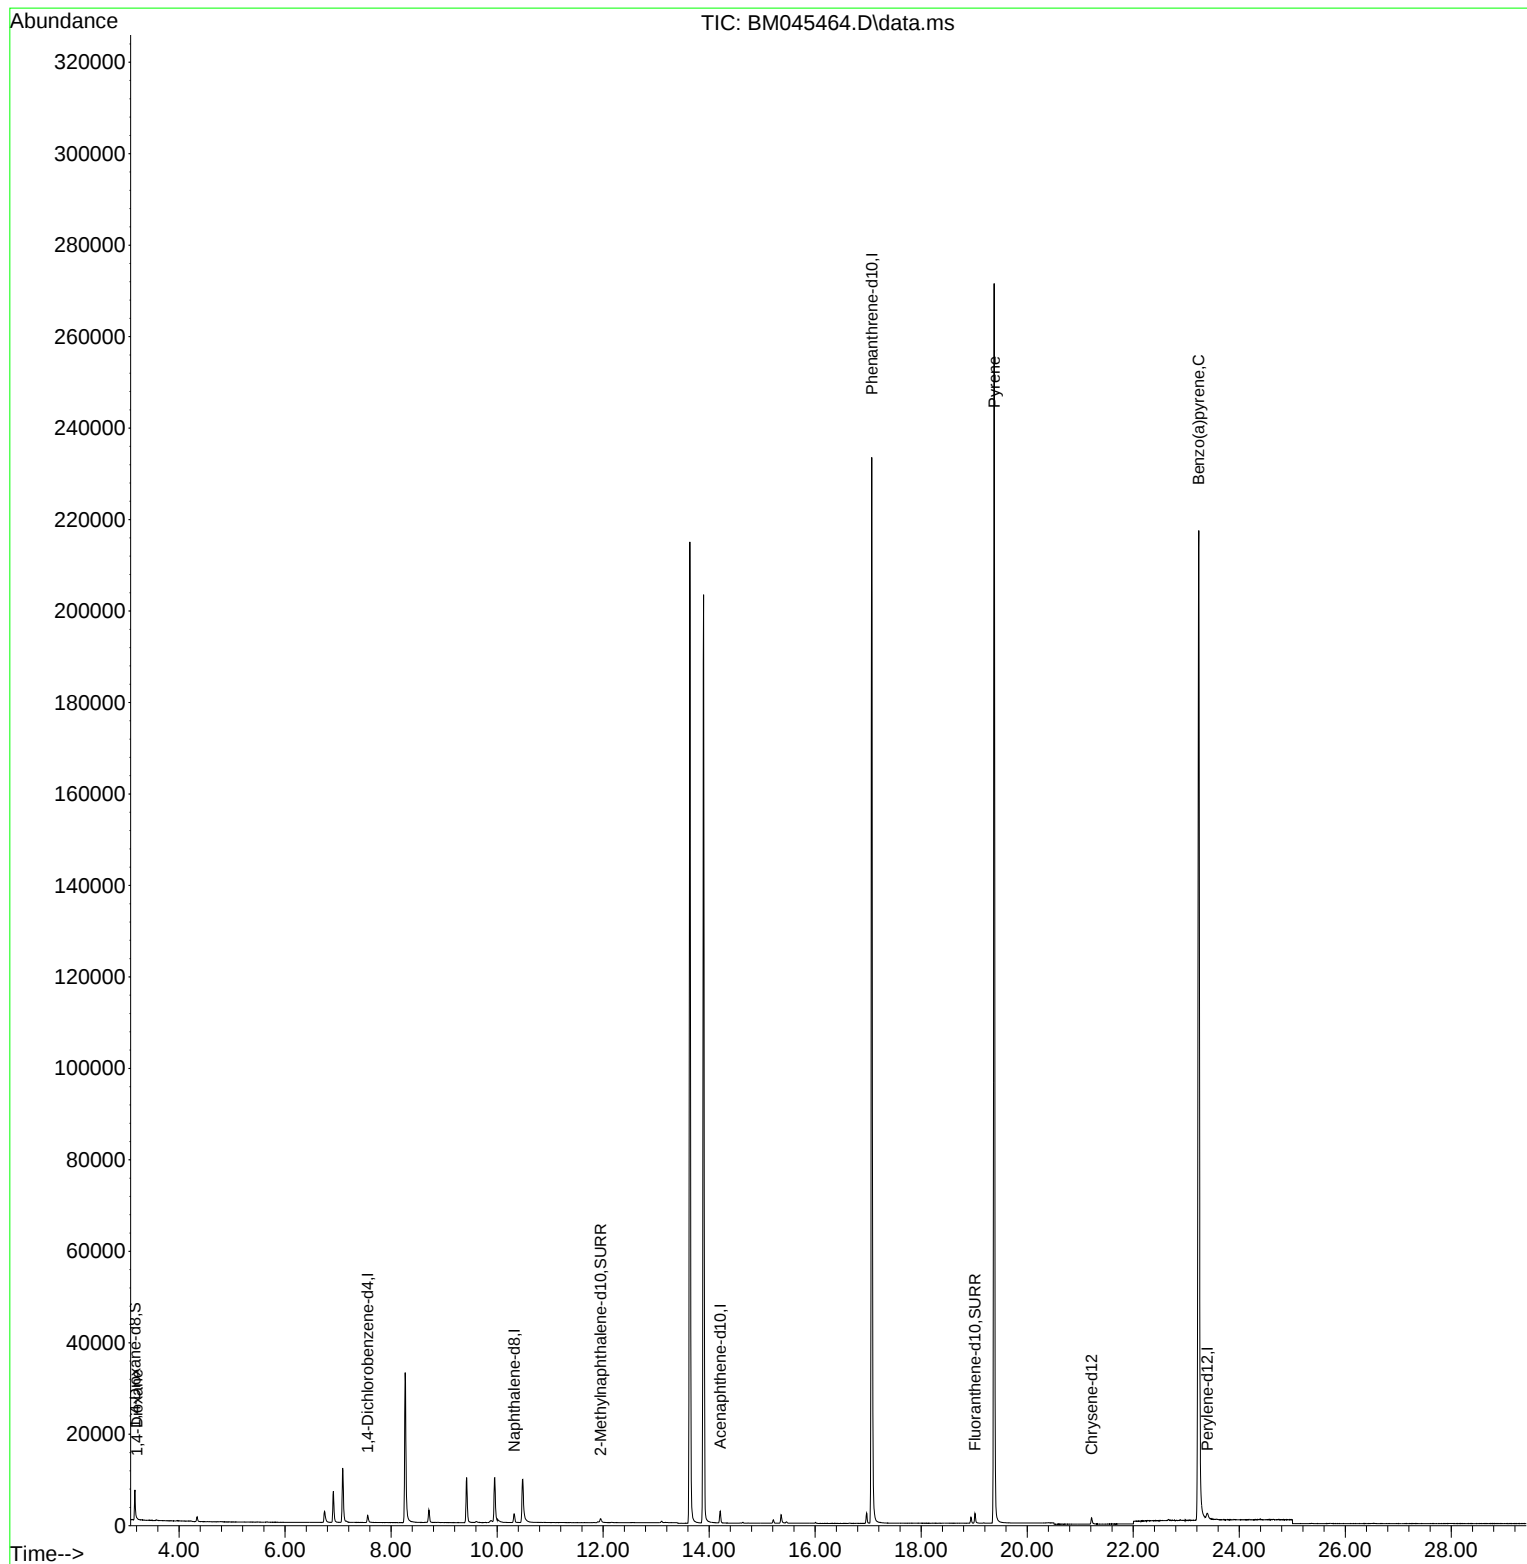



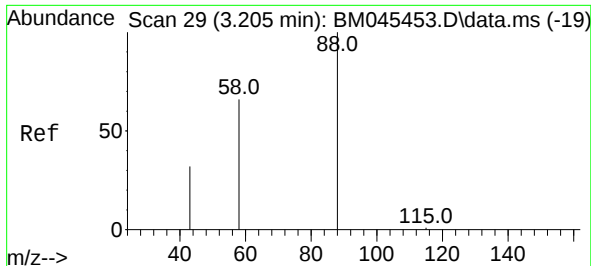


#2
1,4-Dioxane
Concen: 0.075 ng/ul
RT: 3.209 min Scan# 30
Delta R.T. 0.004 min
Lab File: BM045464.D
Acq: 21 Apr 2024 16:21


Instrument :
BNA_M
ClientSampleId :

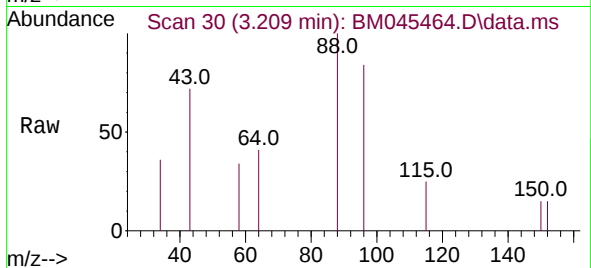



Tgt Ion: 88 Resp: 87
Ion Ratio Lower Upper
88 100
43 72.0 36.8 55.2#
58 33.8 35.4 53.2#

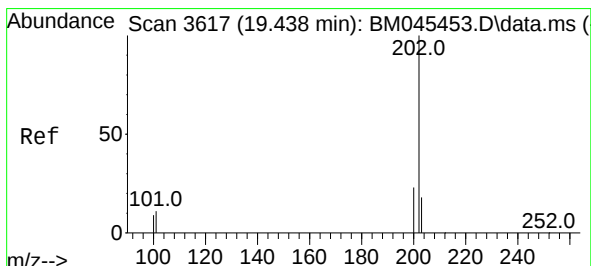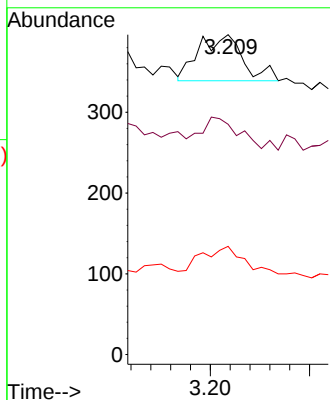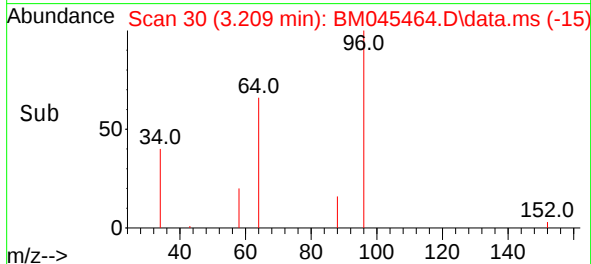


#20
Pyrene
Concen: 0.069 ng/ul
RT: 19.377 min Scan# 3604
Delta R.T. -0.061 min
Lab File: BM045464.D
Acq: 21 Apr 2024 16:21

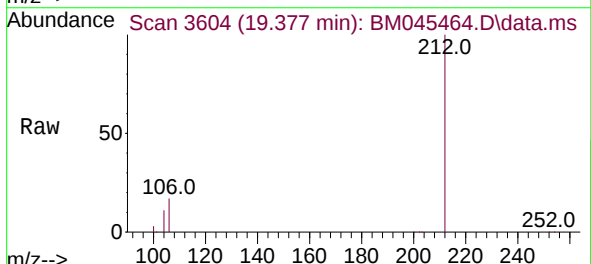

Tgt Ion: 202 Resp: 559
Ion Ratio Lower Upper
202 100
101 204.2 11.5 17.3#
100 1519.1 10.6 15.8#

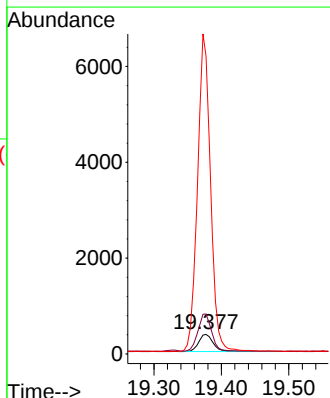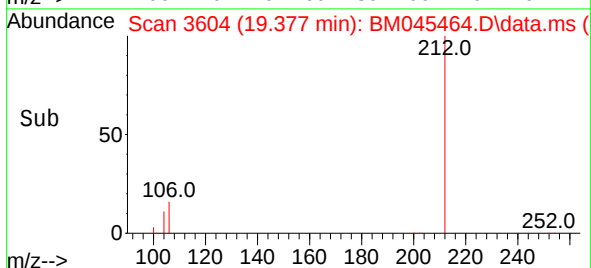

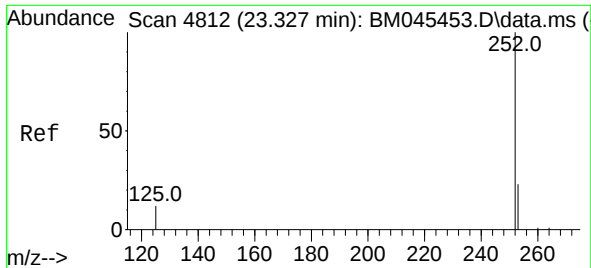

#26

Benzo(a)pyrene

Concen: 0.097 ng/ul

RT: 23.233 min Scan# 41

Delta R.T. -0.094 min


Lab File: BM045464.D

Acq: 21 Apr 2024 16:21

Instrument :

BNA_M

ClientSampleId :

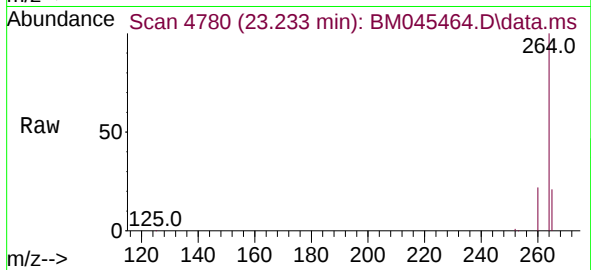

Tgt Ion:252 Resp: 1130

Ion Ratio Lower Upper

252 100

253 58.7 31.6 47.4#

125 41.7 19.5 29.3#

