




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045437.D
Acq On : 20 Apr 2024 23:29
Operator : MA/JU
Sample : PB160291BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK291

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 21 05:11:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

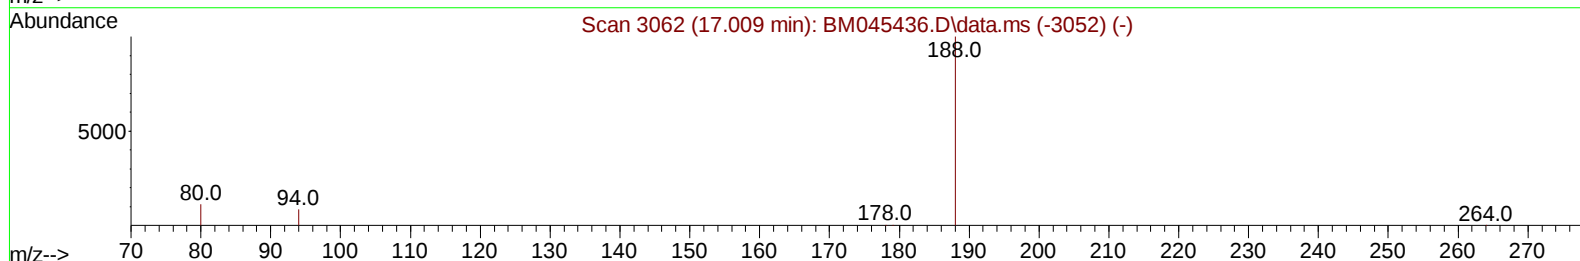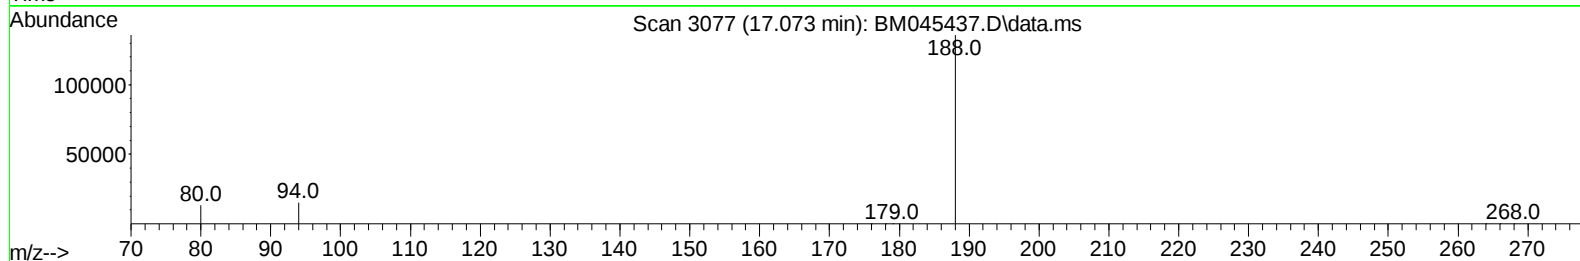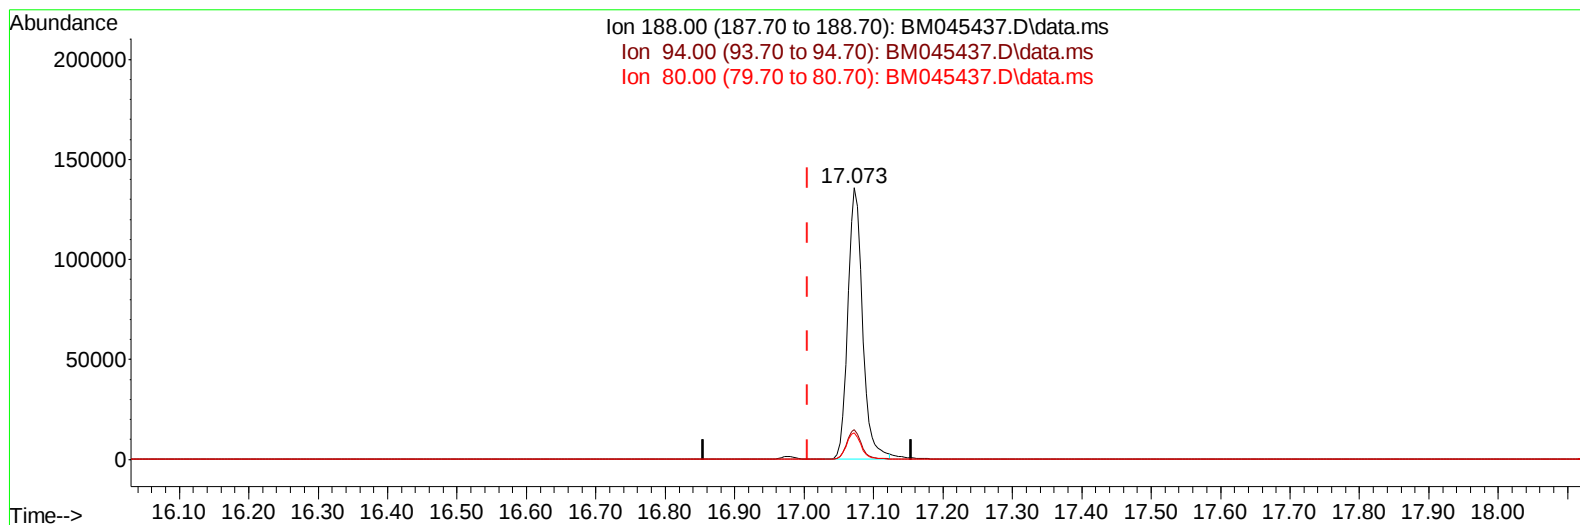

TIC: BM045437.D\data.ms

(13) Phenanthrene-d10 (I)

17.073min (+ 0.068) 0.40 ng/u1

response 199618

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.80	11.09#
80.00	14.80	9.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045437.D
Acq On : 20 Apr 2024 23:29
Operator : MA/JU
Sample : PB160291BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK291

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 21 05:11:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

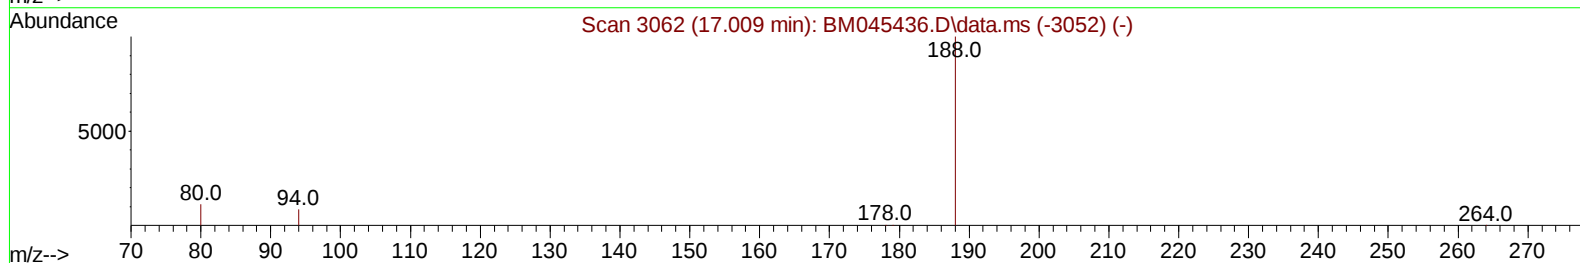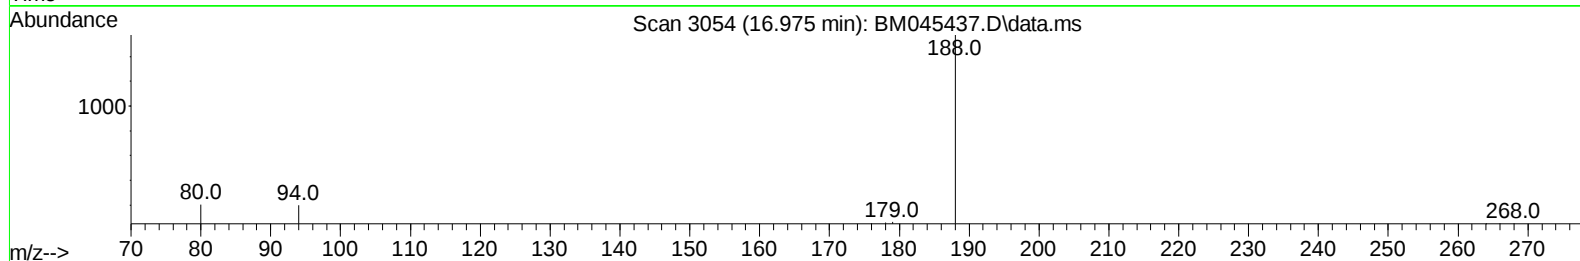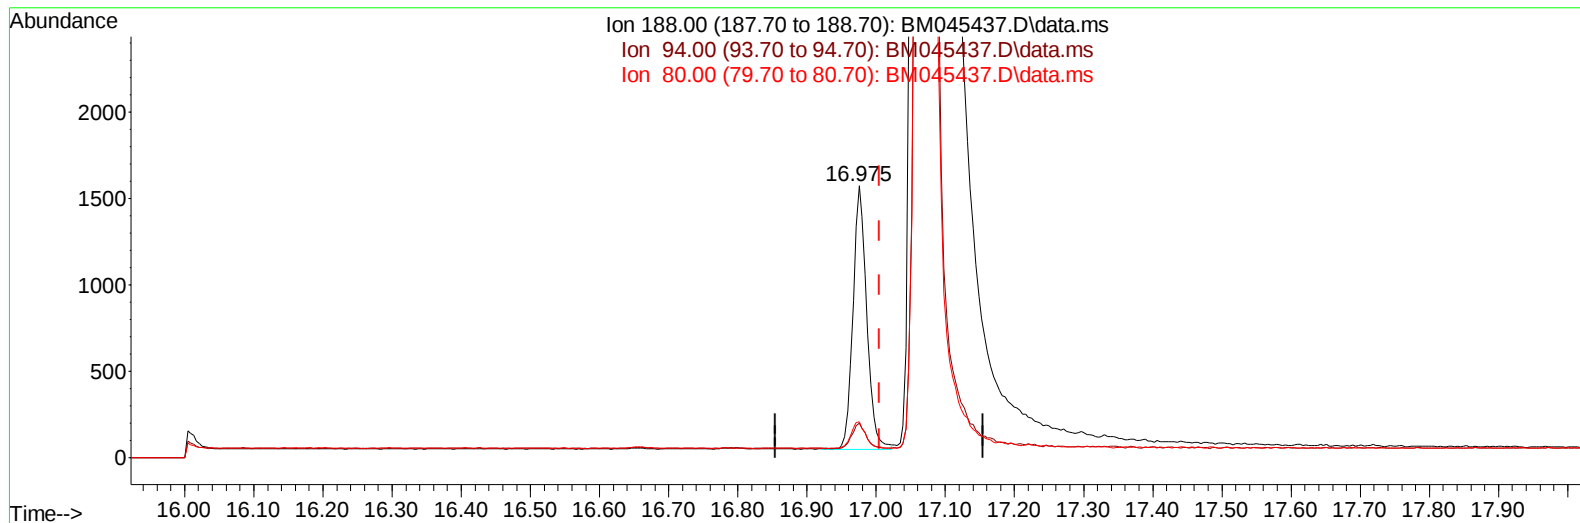

TIC: BM045437.D\data.ms

(13) Phenanthrene-d10 (I)

16.975min (-0.030) 0.40 ng/ul m

response 2115

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.80	12.65
80.00	14.80	13.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
 Data File : BM045437.D
 Acq On : 20 Apr 2024 23:29
 Operator : MA/JU
 Sample : PB160291BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK291

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:25:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 21 05:11:22 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/24/2024

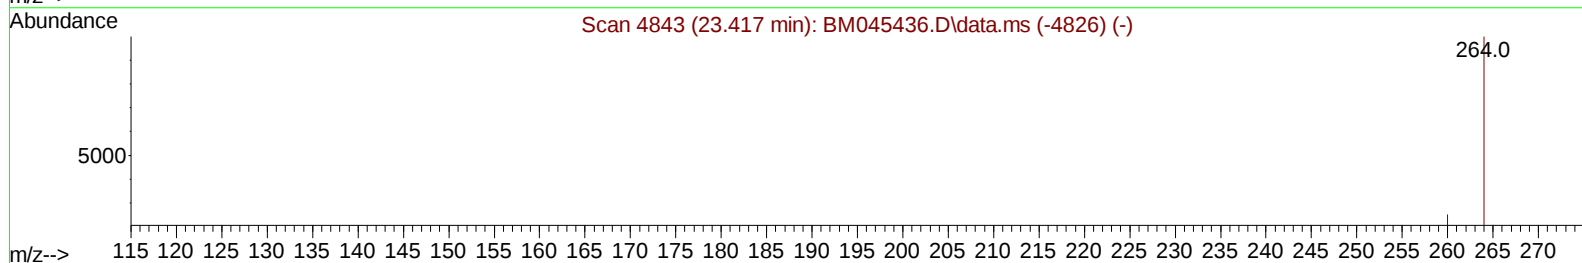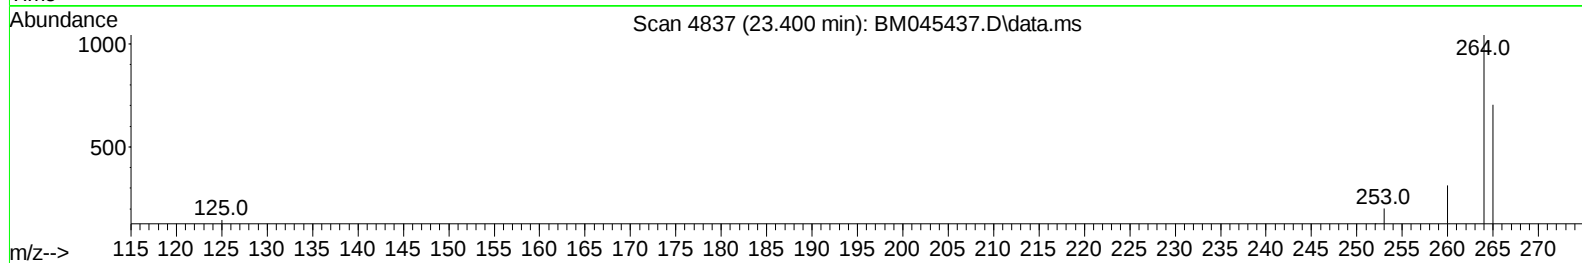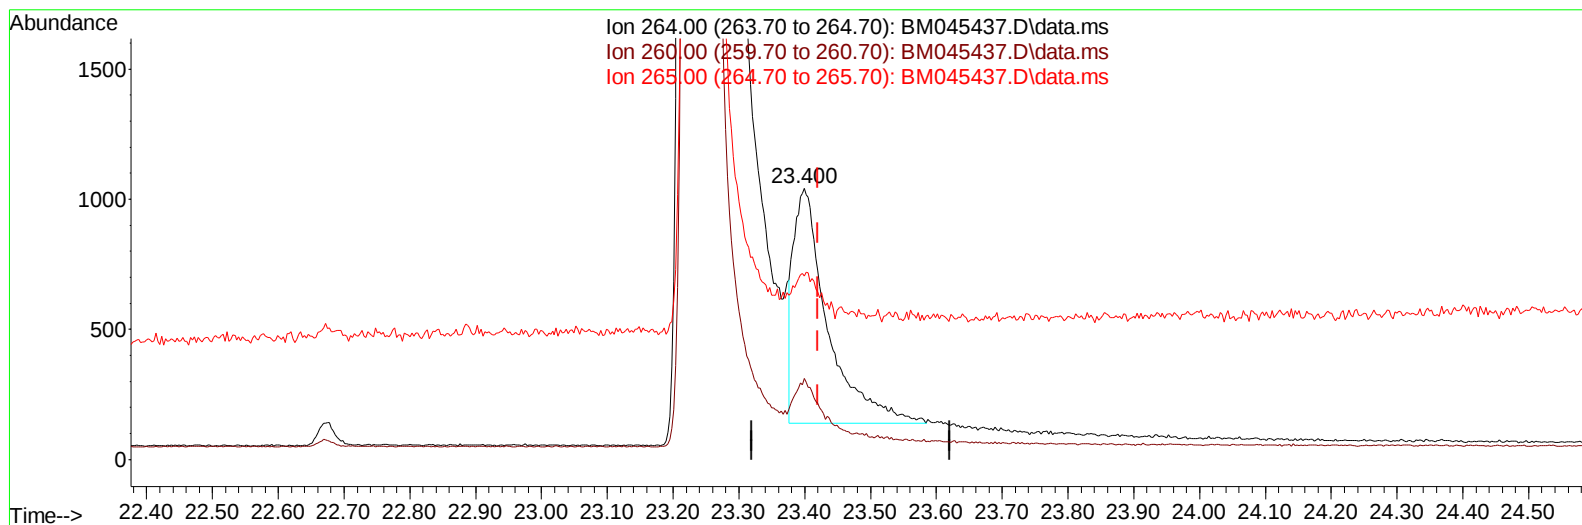

TIC: BM045437.D\data.ms

(23) Perylene-d12 (I)

23.400min (-0.020) 0.40 ng/u1

response 3266

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	30.50	29.91
265.00	86.70	67.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045437.D
Acq On : 20 Apr 2024 23:29
Operator : MA/JU
Sample : PB160291BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK291

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 21 05:11:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

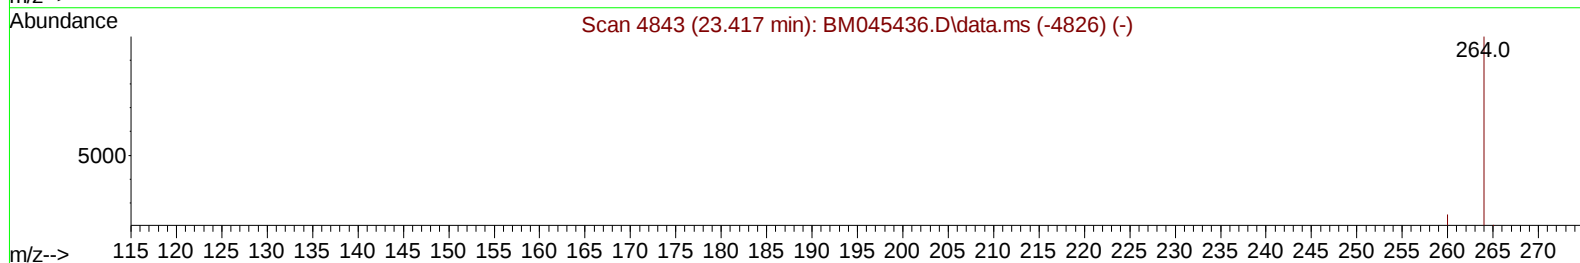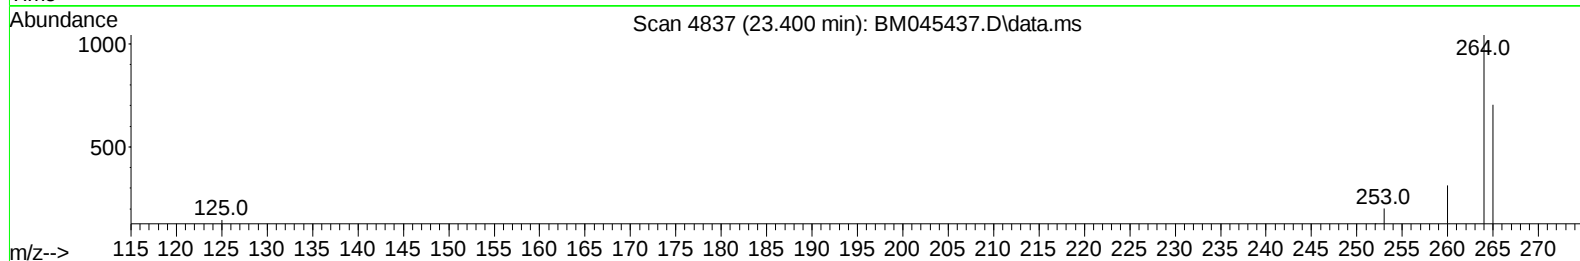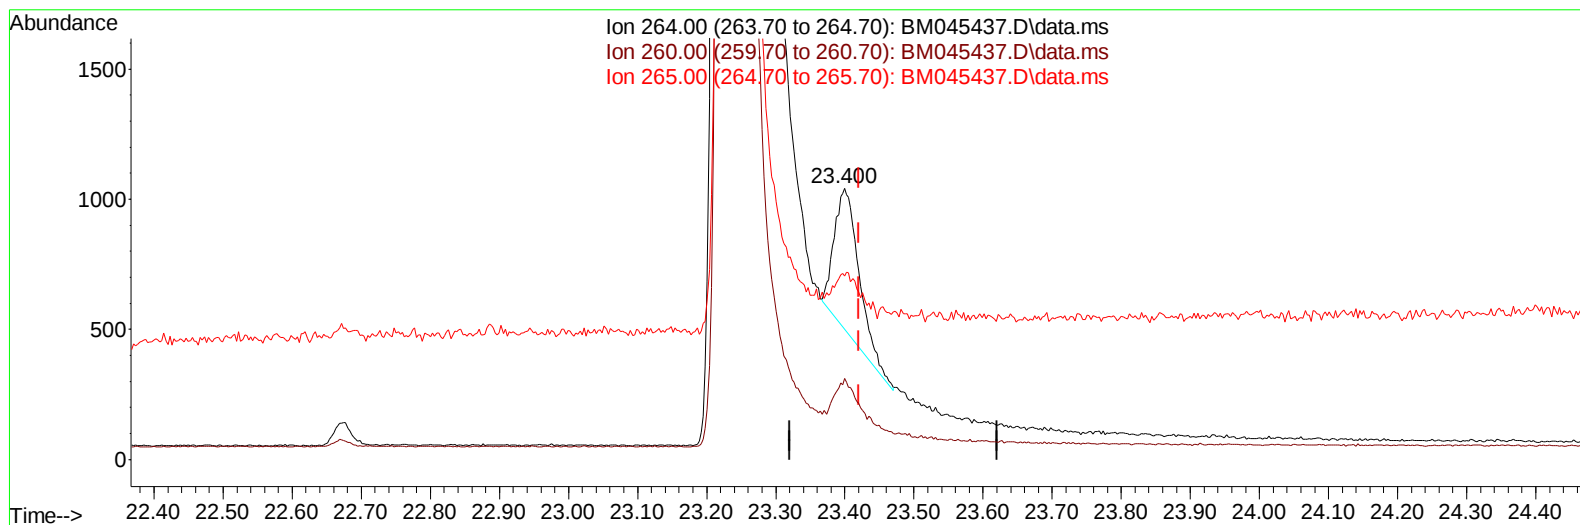

TIC: BM045437.D\data.ms

(23) Perylene-d12 (I)

23.400min (-0.020) 0.40 ng/ul m

response 1322

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	30.50	29.91
265.00	86.70	67.50#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
 Data File : BM045437.D
 Acq On : 20 Apr 2024 23:29
 Operator : MA/JU
 Sample : PB160291BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK291

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/24/2024

Quant Time: Apr 21 05:25:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 21 05:11:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.568	152	712	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.330	136	2133	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.214	164	1106	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.975	188	2115m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.225	240	1470	0.400	ng/ul	0.00
23) Perylene-d12	23.400	264	1322m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.167	96	6013	6.301	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.975	152	975	0.347	ng/ul	0.00
18) Fluoranthene-d10	19.024	212	1705	0.368	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045437.D
Acq On : 20 Apr 2024 23:29
Operator : MA/JU
Sample : PB160291BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK291

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:25:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 21 05:11:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

