




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045440.D
Acq On : 21 Apr 2024 01:19
Operator : MA/JU
Sample : P2117-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG8

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:31:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 21 05:11:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

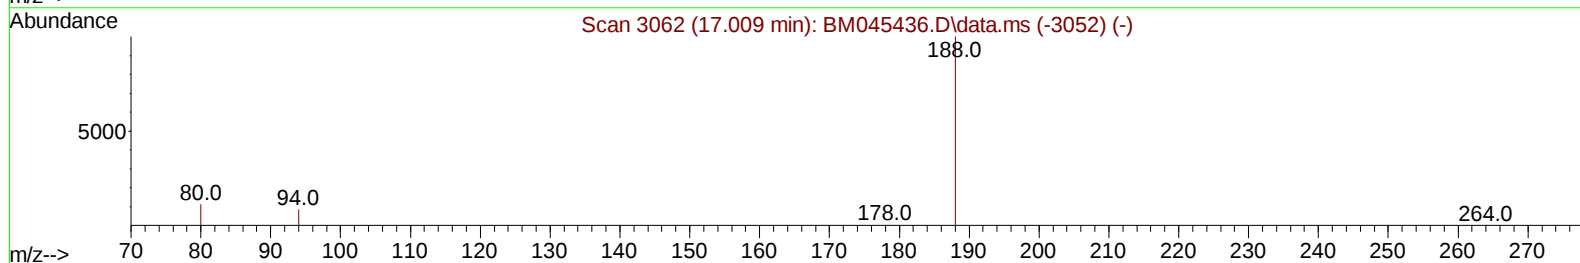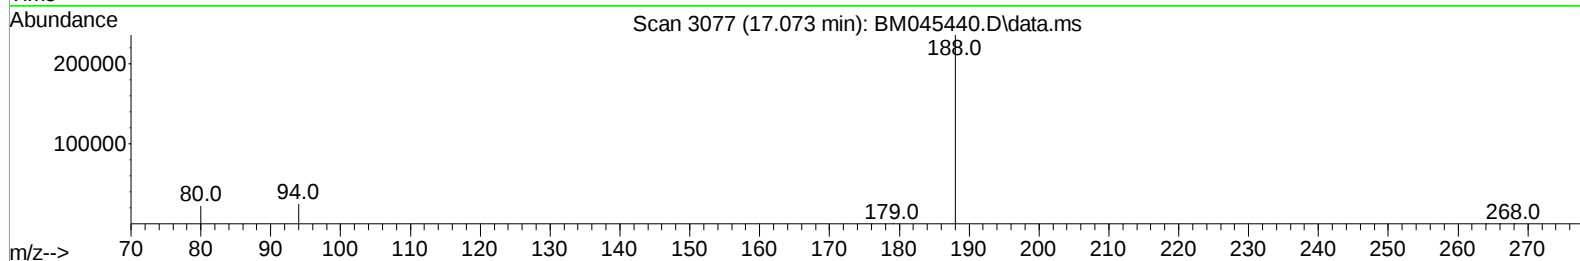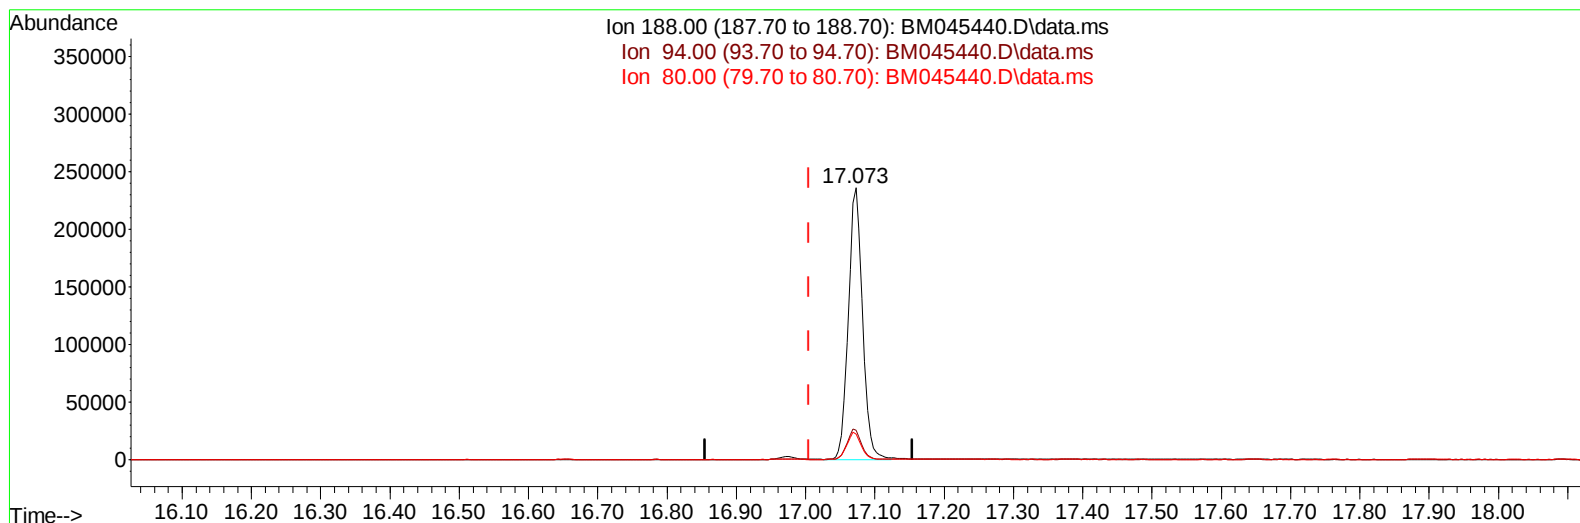

TIC: BM045440.D\data.ms

(13) Phenanthrene-d10 (I)

17.073min (+ 0.068) 0.40 ng/u1

response 335093

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.80	10.67#
80.00	14.80	9.44#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045440.D
Acq On : 21 Apr 2024 01:19
Operator : MA/JU
Sample : P2117-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG8

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:31:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 21 05:11:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

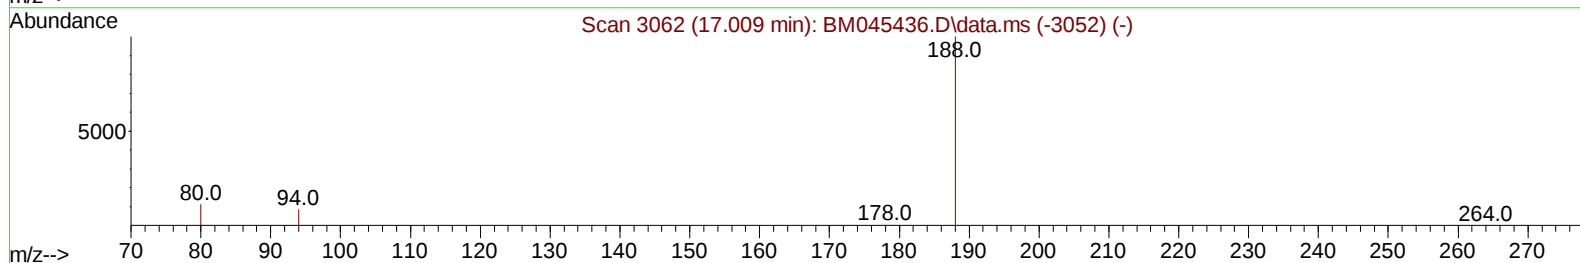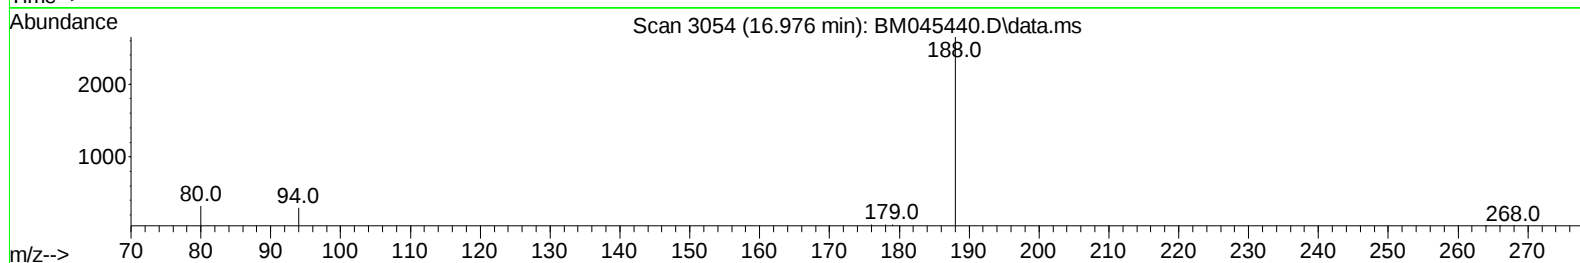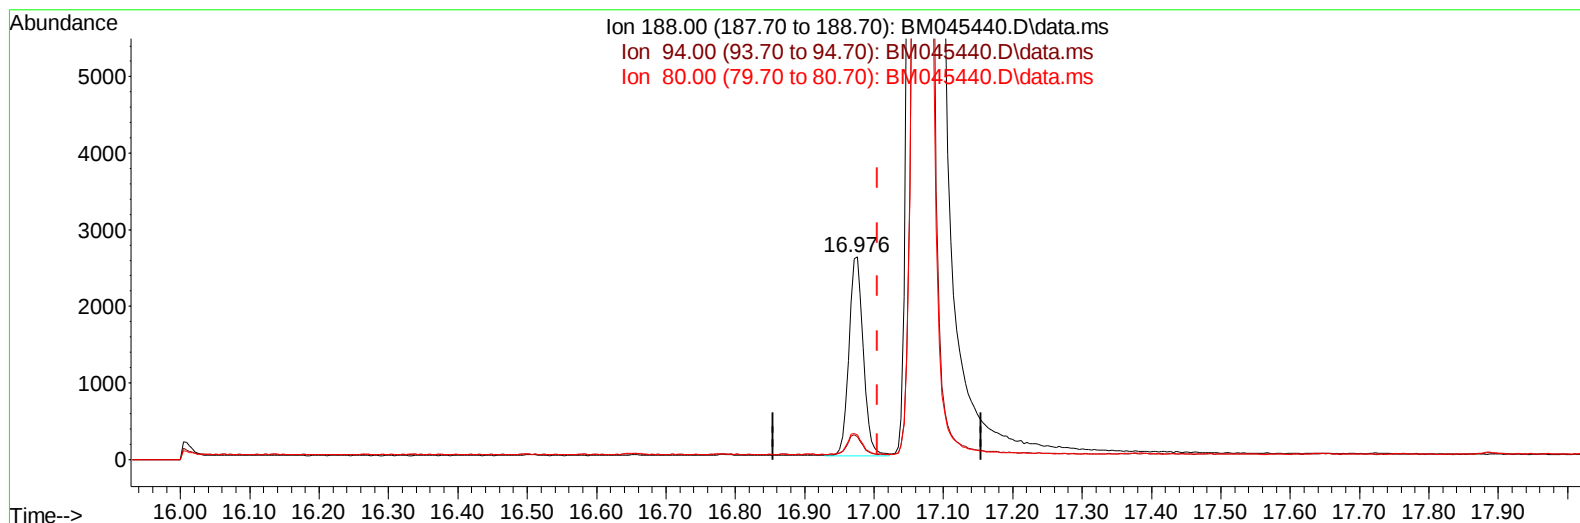

TIC: BM045440.D\data.ms

(13) Phenanthrene-d10 (I)

16.976min (-0.029) 0.40 ng/ul m

response 3700

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	14.80	11.36#
80.00	14.80	12.15
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
 Data File : BM045440.D
 Acq On : 21 Apr 2024 01:19
 Operator : MA/JU
 Sample : P2117-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MG8

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:31:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 21 05:11:22 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/24/2024

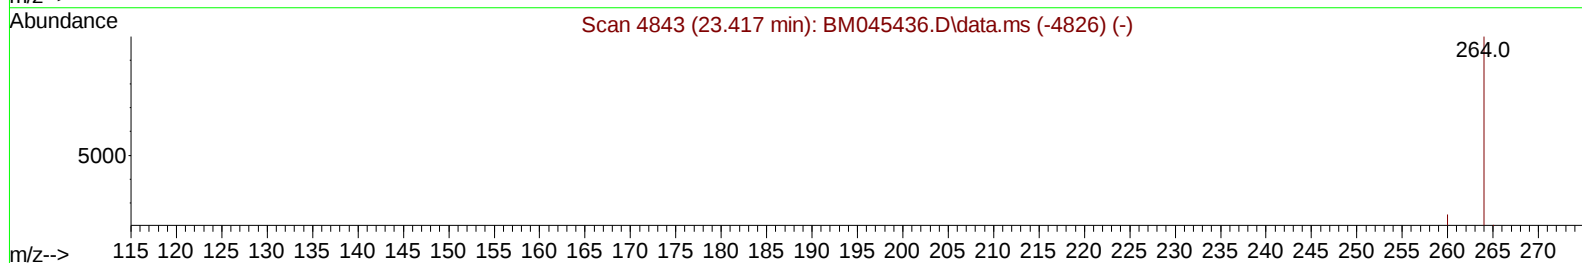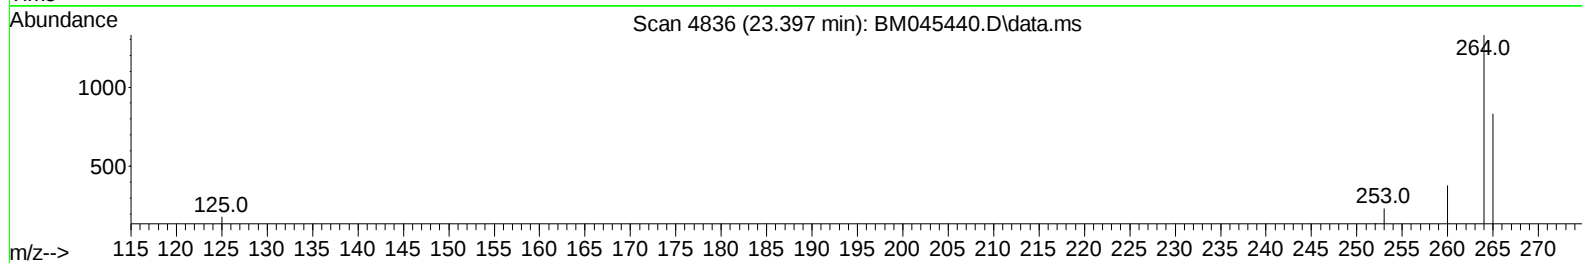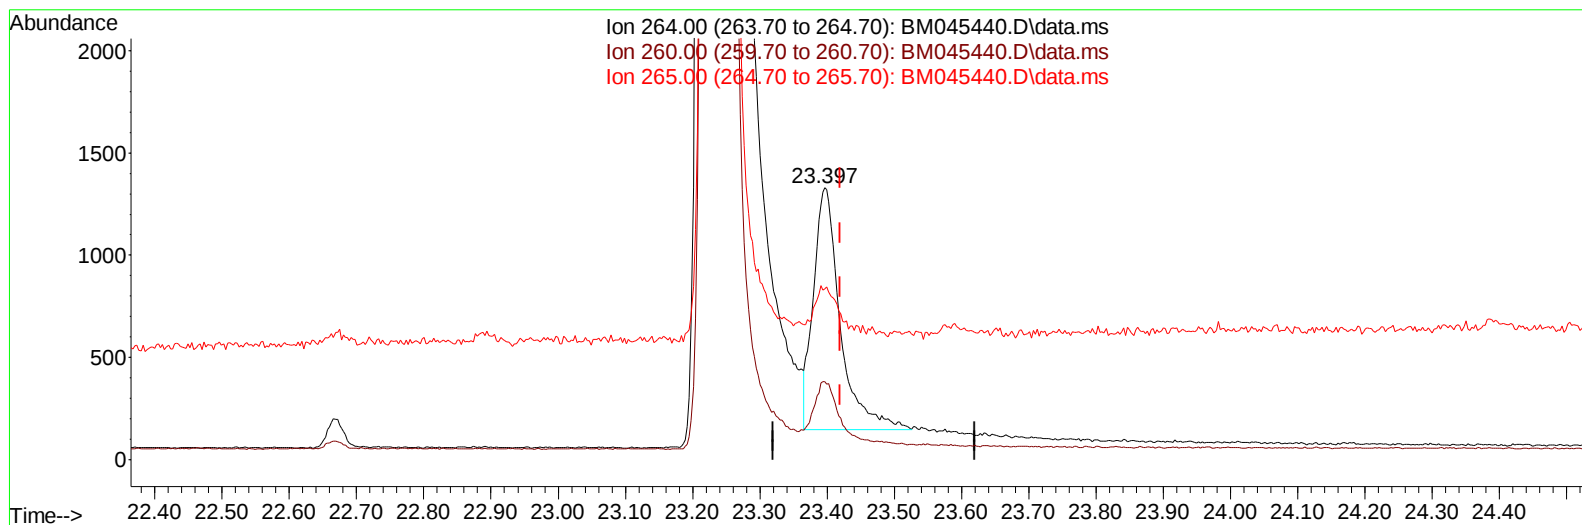

TIC: BM045440.D\data.ms

(23) Perylene-d12 (I)

23.397min (-0.023) 0.40 ng/u1

response 3303

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	30.50	28.67
265.00	86.70	62.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045440.D
Acq On : 21 Apr 2024 01:19
Operator : MA/JU
Sample : P2117-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG8

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:31:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 21 05:11:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

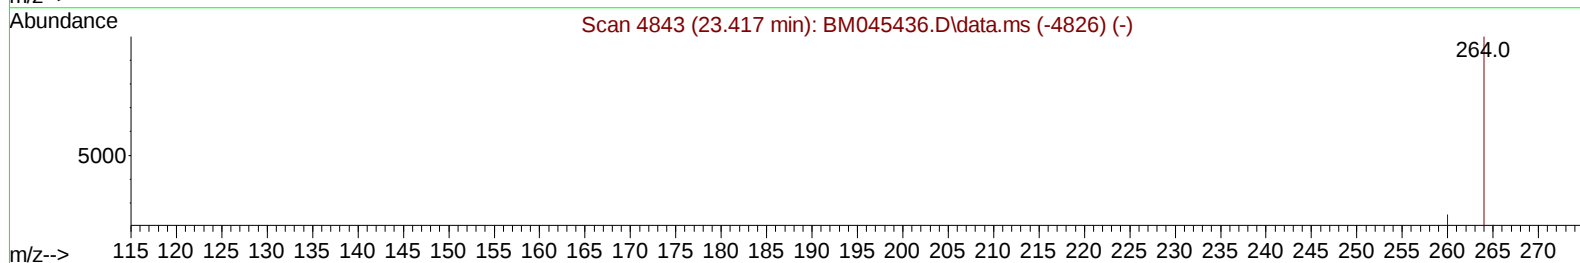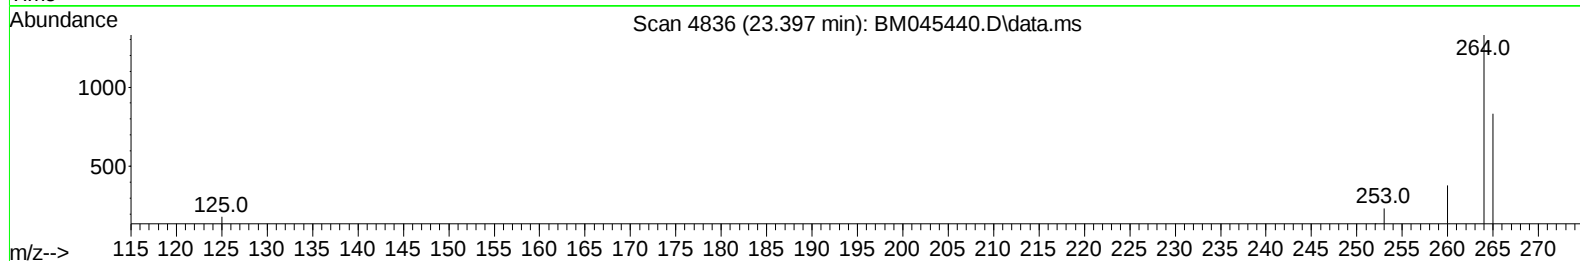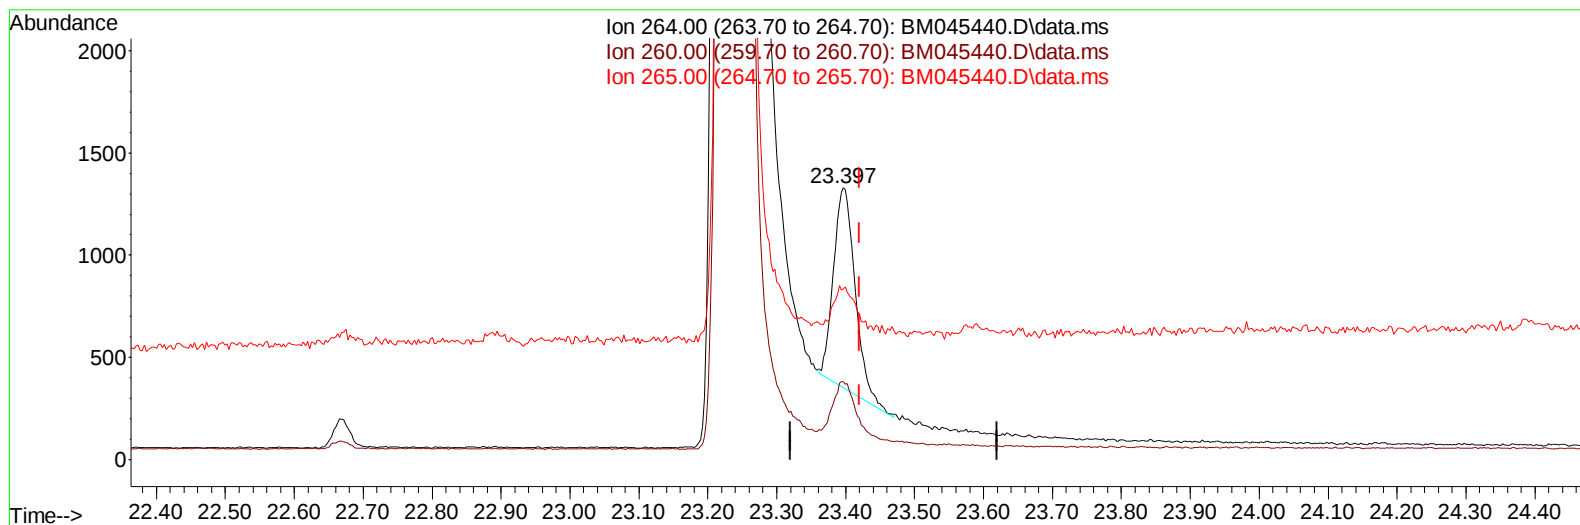

TIC: BM045440.D\data.ms

(23) Perylene-d12 (I)

23.397min (-0.023) 0.40 ng/u1 m

response 2126

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	30.50	28.67
265.00	86.70	62.75#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
 Data File : BM045440.D
 Acq On : 21 Apr 2024 01:19
 Operator : MA/JU
 Sample : P2117-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MG8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/24/2024
 Supervised By :mohammad ahmed 04/24/2024

Quant Time: Apr 21 05:31:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 21 05:11:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.564	152	939	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.325	136	3016	0.400	ng/ul	#-0.05
9) Acenaphthene-d10	14.214	164	1718	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.976	188	3700m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.202	240	2421	0.400	ng/ul	-0.01
23) Perylene-d12	23.397	264	2126m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.167	96	3870	3.075	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.947	152	1482	0.373	ng/ul	-0.03
18) Fluoranthene-d10	19.020	212	3306	0.434	ng/ul	-0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042024\
Data File : BM045440.D
Acq On : 21 Apr 2024 01:19
Operator : MA/JU
Sample : P2117-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MG8

Manual IntegrationsAPPROVED

Quant Time: Apr 21 05:31:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 21 05:11:22 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/24/2024
Supervised By :mohammad ahmed 04/24/2024

