
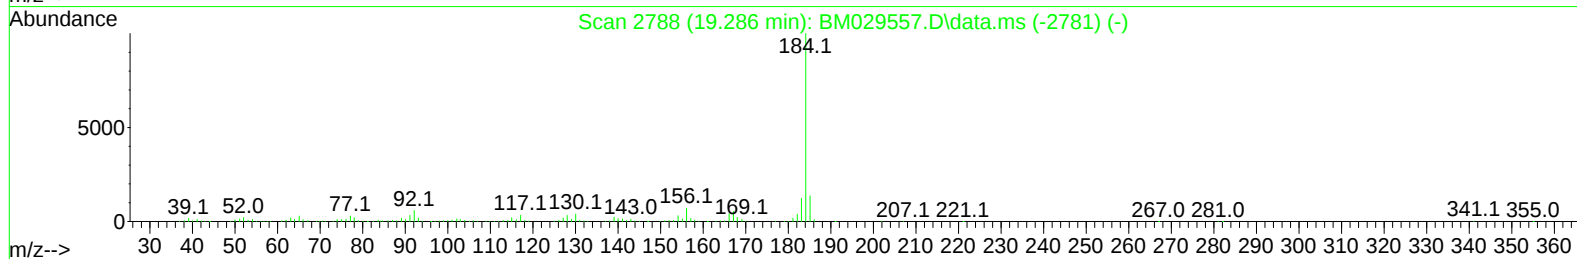
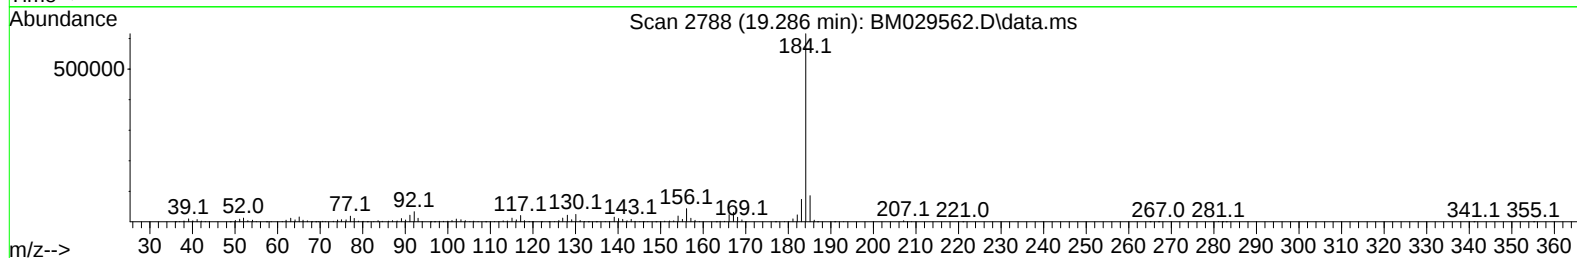


Quant Time: Apr 21 13:00:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 12:55:47 2021
Response via : Initial Calibration

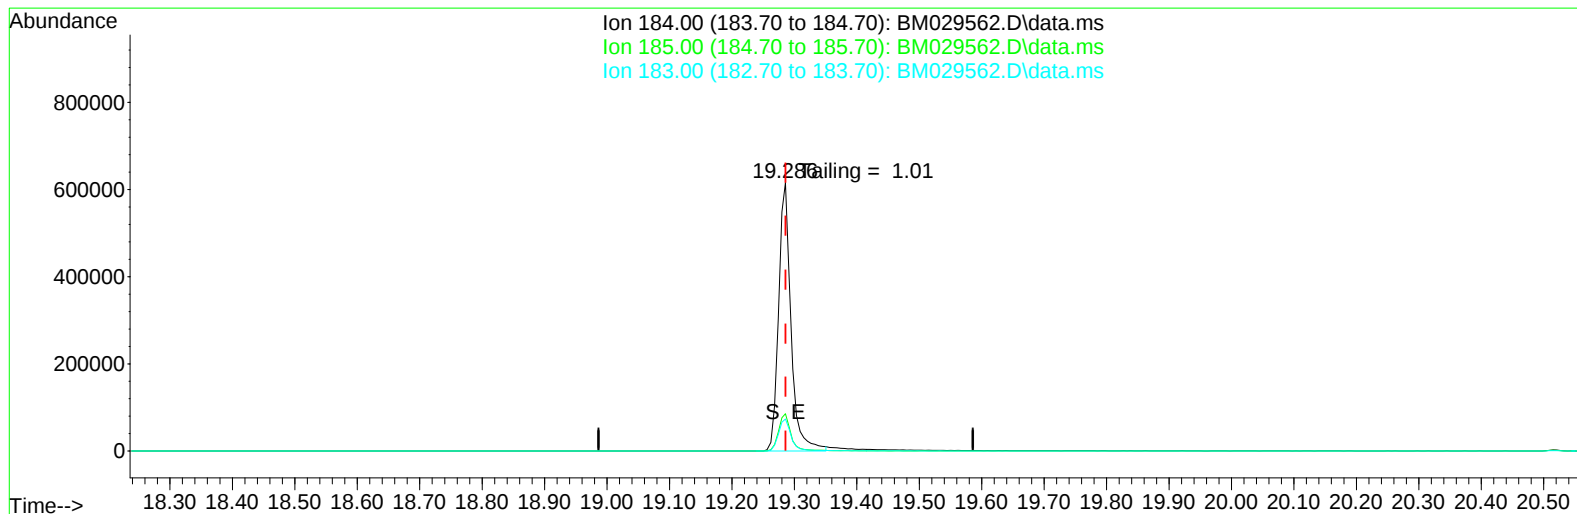

TIC: BM029562.D\data.ms

(77) Benzidine




19.286min (-0.000) 0.00 ng

response **896317**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.92
183.00	12.30	11.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
Data File : BM029562.D
Acq On : 21 Apr 2021 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 13:00:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 12:55:47 2021
Response via : Initial Calibration

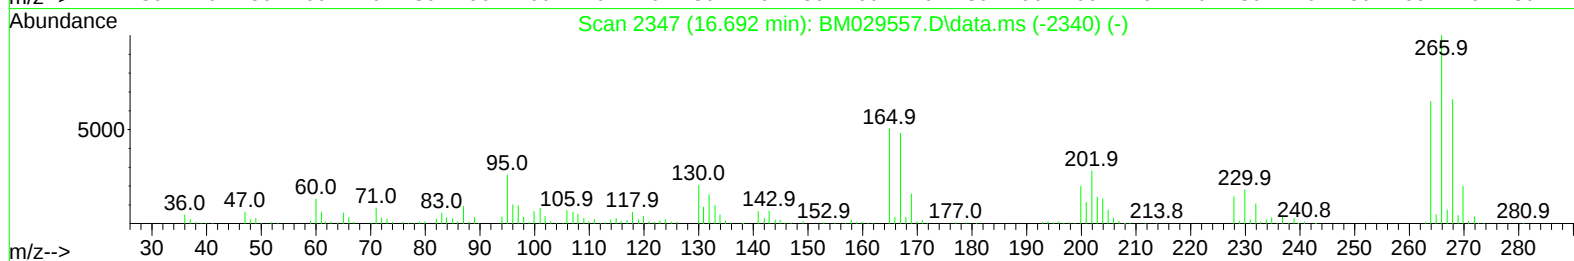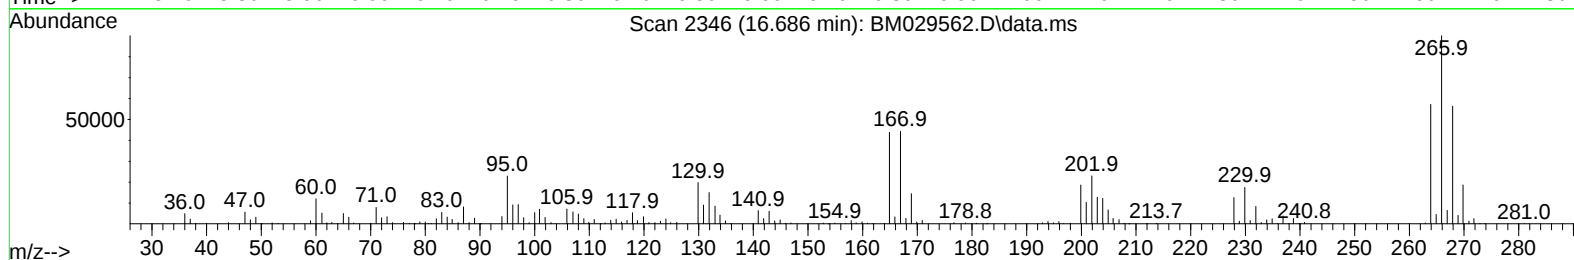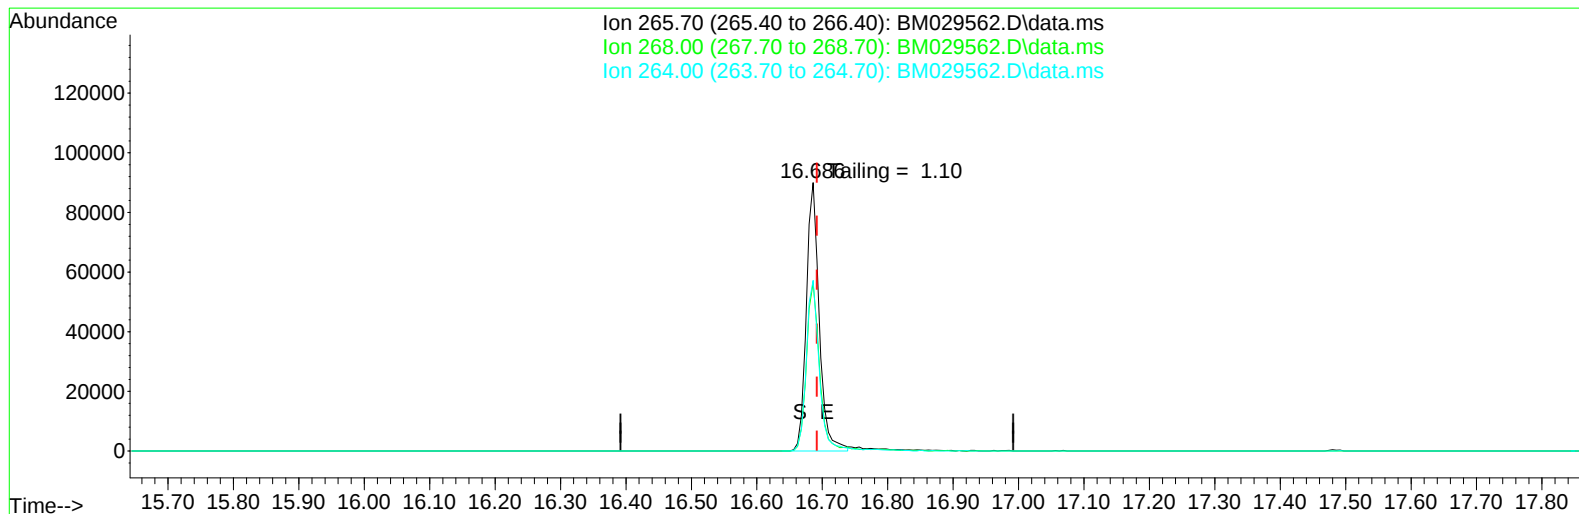

TIC: BM029562.D\data.ms

(70) Pentachlorophenol (C)

16.686min (-0.006) 0.00 ng

response 126918

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	62.66
264.00	64.90	63.58
0.00	0.00	0.00