
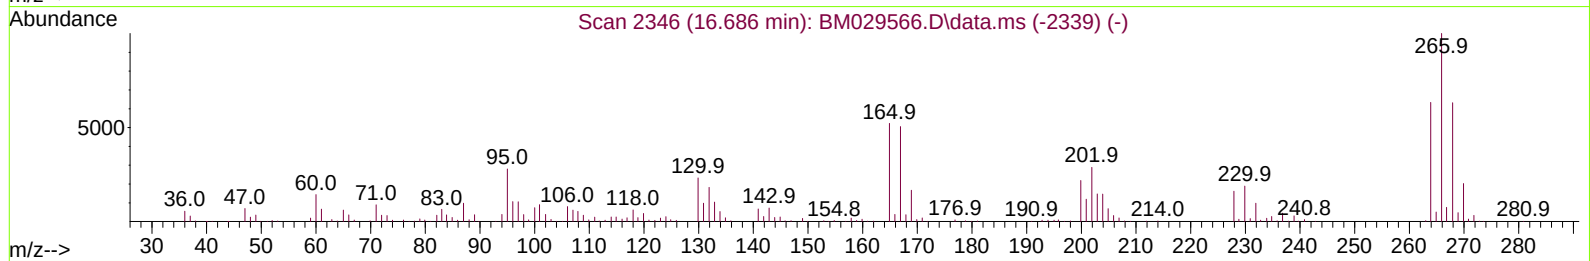
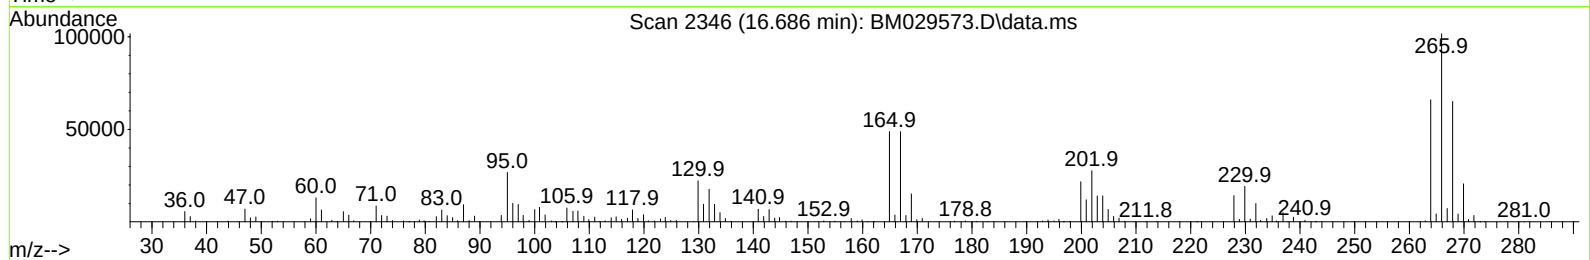


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
Data File : BM029573.D
Acq On : 21 Apr 2021 19:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 05:00:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 15:14:18 2021
Response via : Initial Calibration

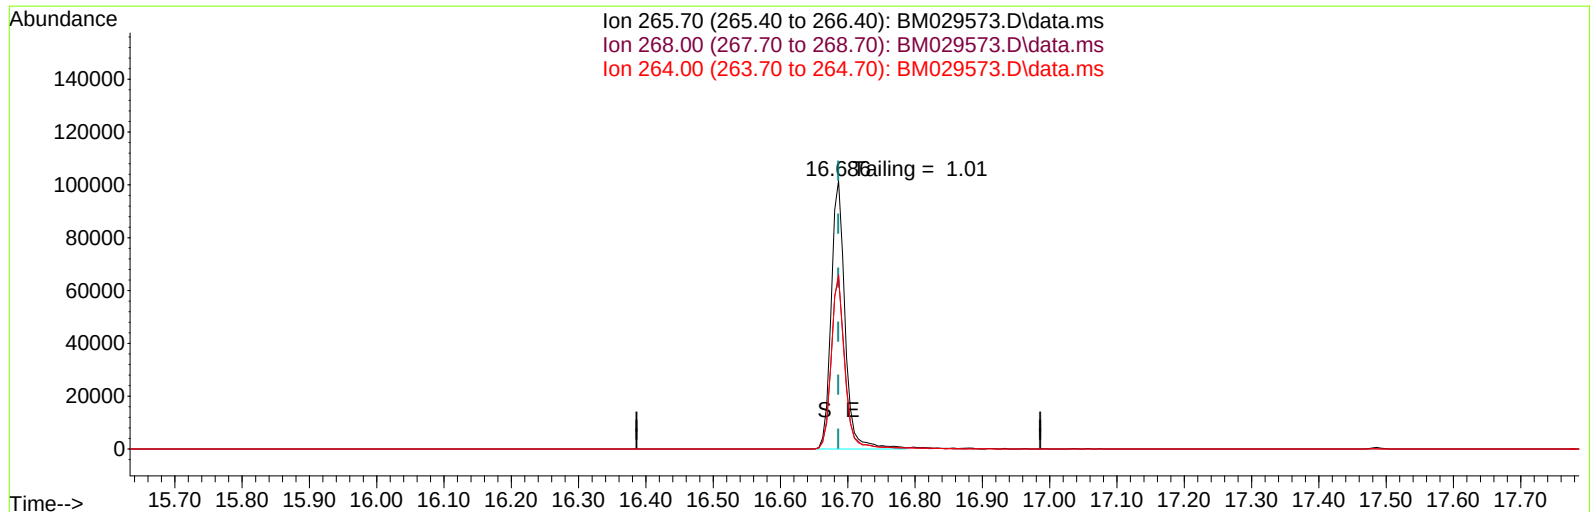

TIC: BM029573.D\data.ms

(70) Pentachlorophenol (C)




16.686min (+ 0.000) 0.00 ng

response 145959

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.03
264.00	64.90	64.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
 Data File : BM029573.D
 Acq On : 21 Apr 2021 19:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 05:00:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 21 15:14:18 2021
 Response via : Initial Calibration

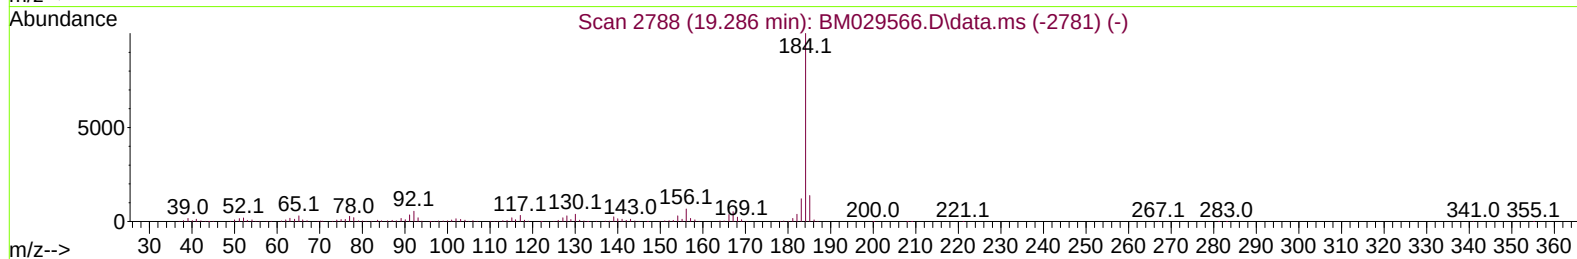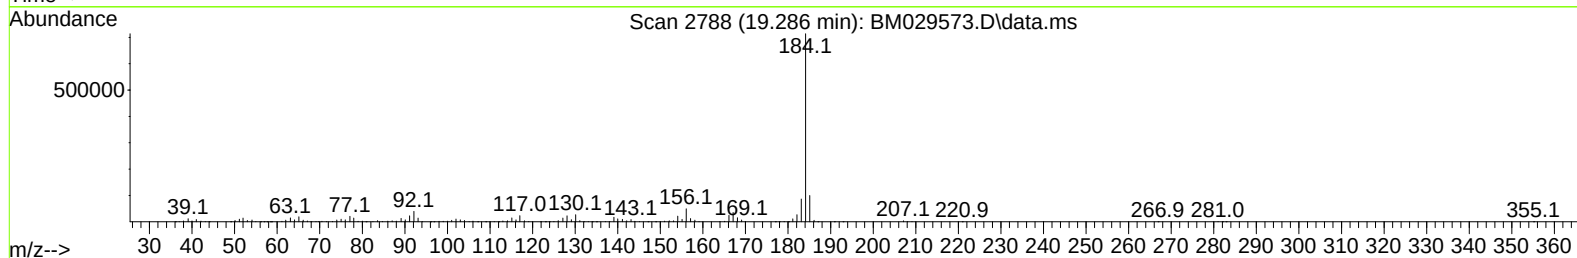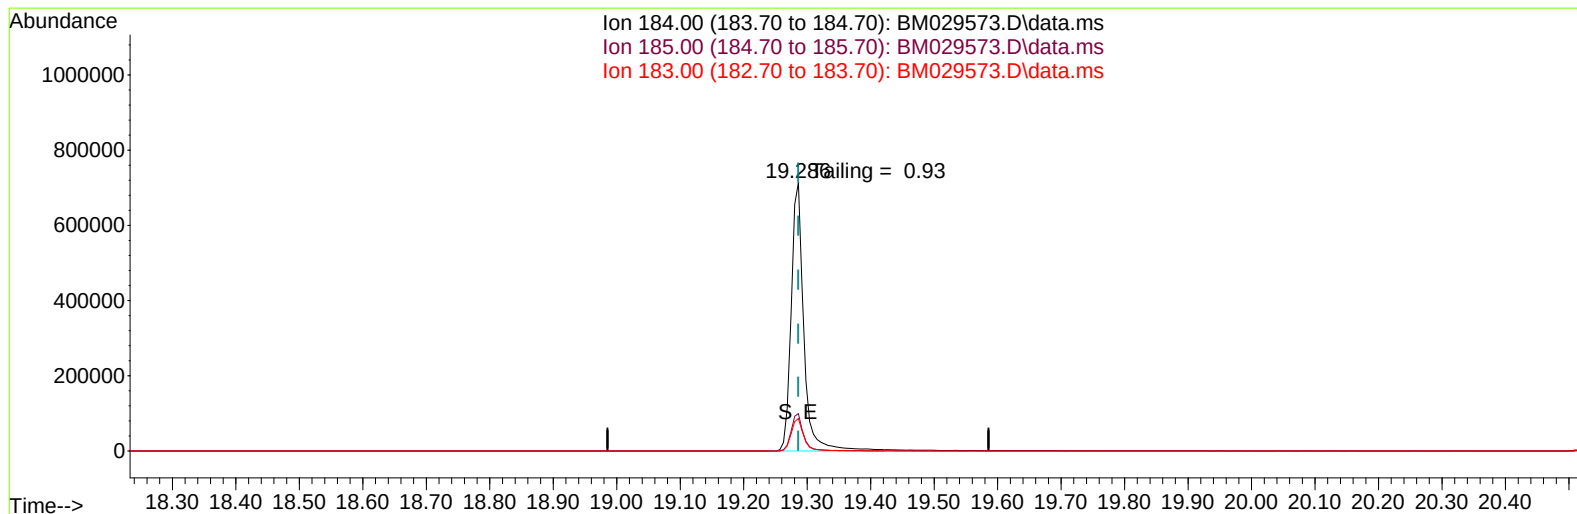

TIC: BM029573.D\data.ms

(77) Benzidine

19.286min (+ 0.000) 0.00 ng

response 1003129

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.95
183.00	12.30	12.15
0.00	0.00	0.00