

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
 Data File : BM029587.D
 Acq On : 22 Apr 2021 03:52
 Operator : CG/JU
 Sample : M2114-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FB-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.240	394	400	414	rBV	462437	725431	8.14%	2.812%
2	6.822	663	669	685	rBV	285677	496812	5.57%	1.926%
3	7.645	802	809	818	rBV	210872	346300	3.89%	1.342%
4	8.798	998	1005	1025	rBV	772307	1319213	14.80%	5.113%
5	10.422	1273	1281	1298	rBV	285241	511445	5.74%	1.982%
6	12.904	1697	1703	1720	rBV	2855111	4219115	47.34%	16.353%
7	14.286	1932	1938	1947	rBV	599088	869479	9.76%	3.370%
8	15.780	2185	2192	2211	rBV	2897973	3885956	43.60%	15.062%
9	17.027	2398	2404	2416	rBV	775940	1135012	12.73%	4.399%
10	19.662	2846	2852	2863	rBV	7741464	8912717	100.00%	34.545%
11	20.939	3064	3069	3077	rBV2	129968	207929	2.33%	0.806%
12	21.209	3110	3115	3124	rBV	1228067	1526903	17.13%	5.918%
13	23.403	3481	3488	3504	rVB	855472	1644268	18.45%	6.373%




Sum of corrected areas: 25800580

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
Data File : BM029587.D
Acq On : 22 Apr 2021 03:52
Operator : CG/JU
Sample : M2114-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

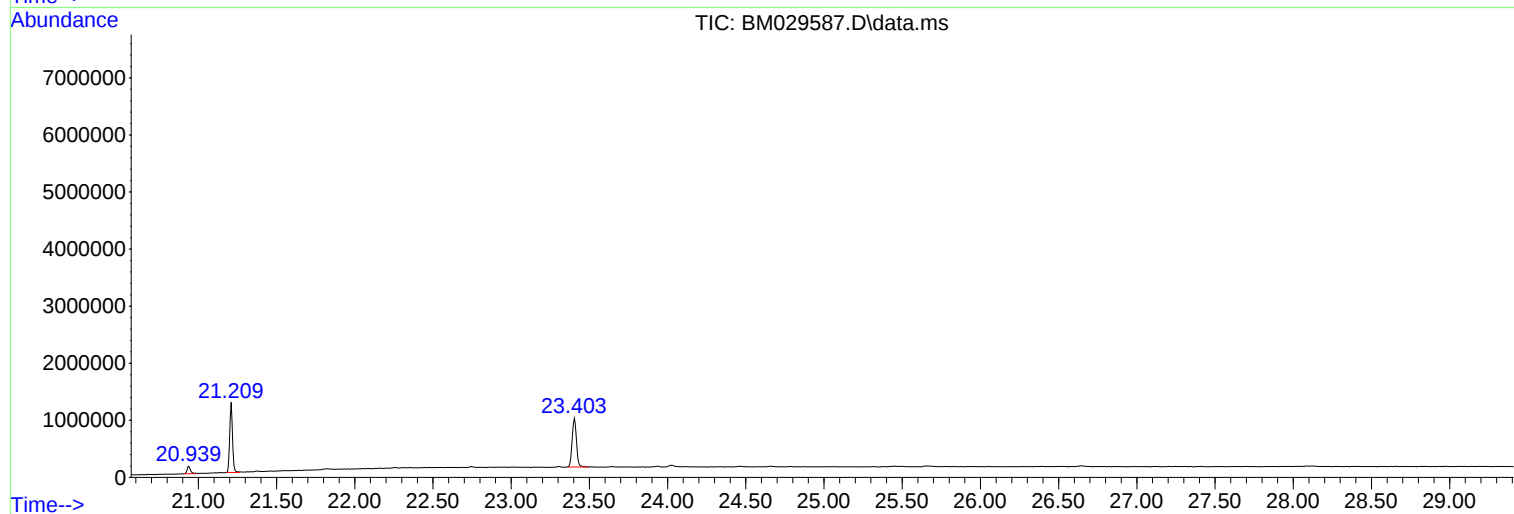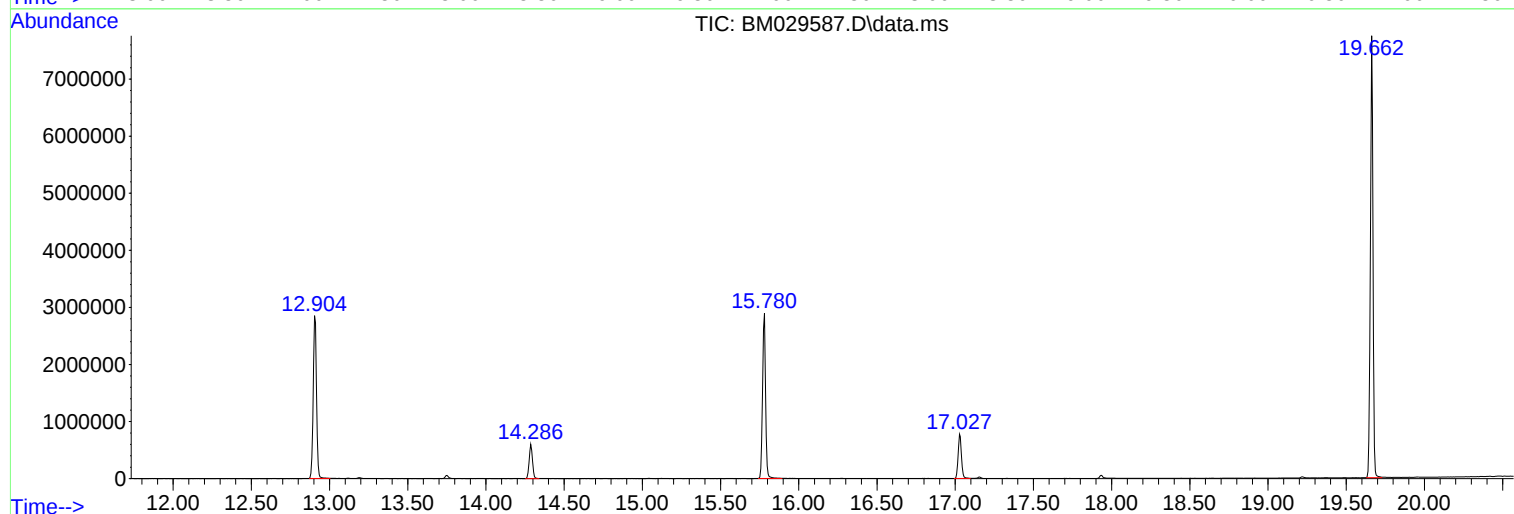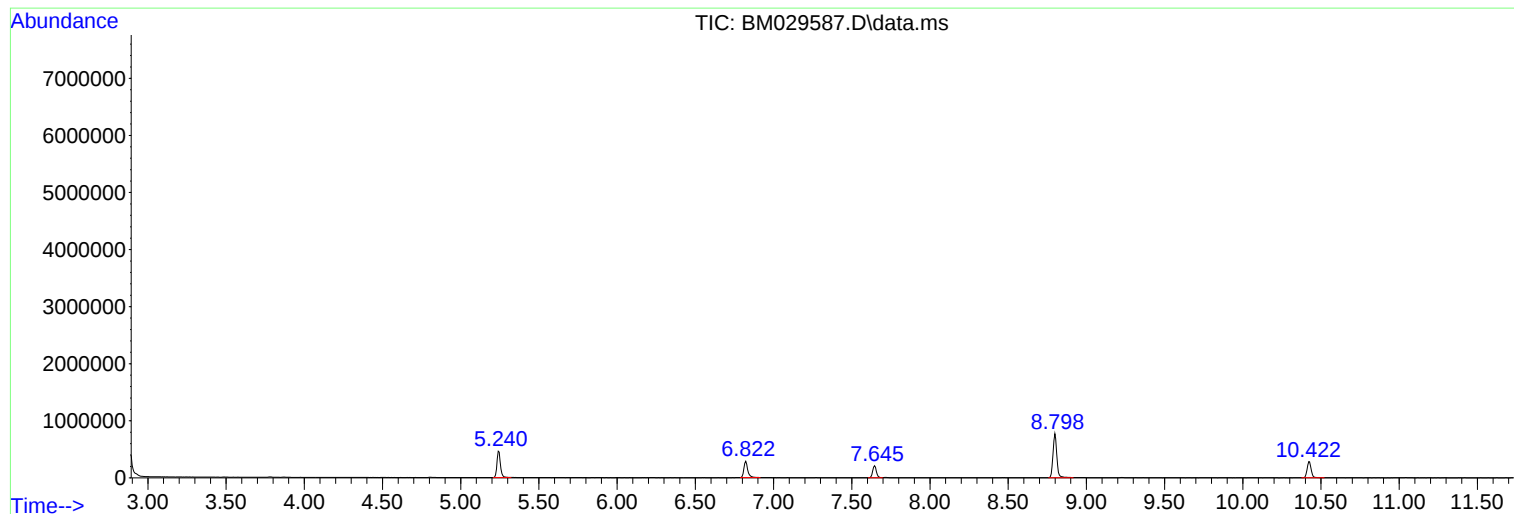

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
Data File : BM029587.D
Acq On : 22 Apr 2021 03:52
Operator : CG/JU
Sample : M2114-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-02










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 3-Eicosene, (E)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.939	2.72 ng	207929	Chrysene-d12	21.209

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Eicosene, (E)-	280	C20H40	074685-33-9	99
2			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
3			E-7-Octadecene	252	C18H36	1000130-92-0	92
4			1-Nonadecene	266	C19H38	018435-45-5	91
5			2- Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	91

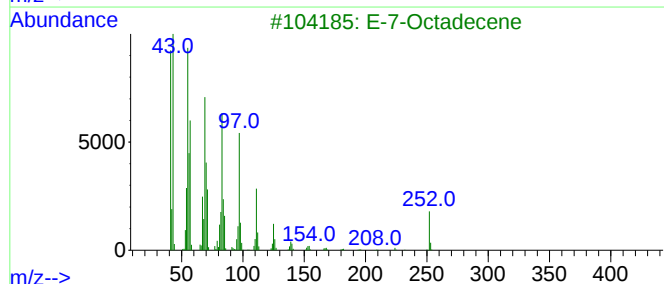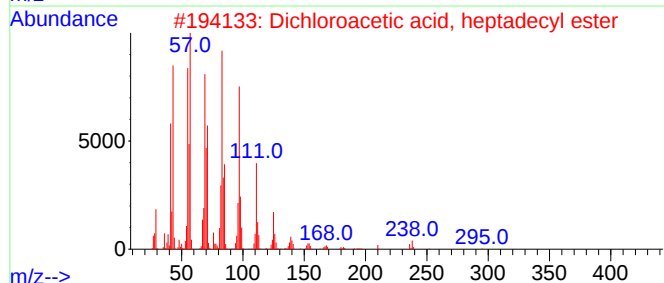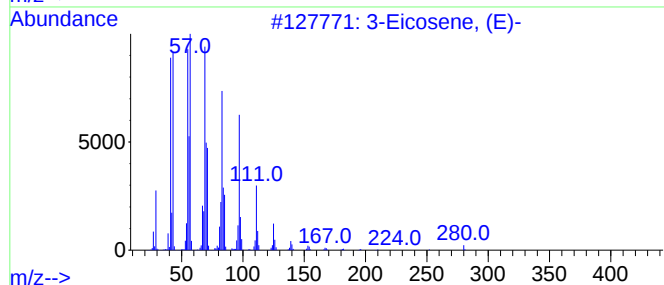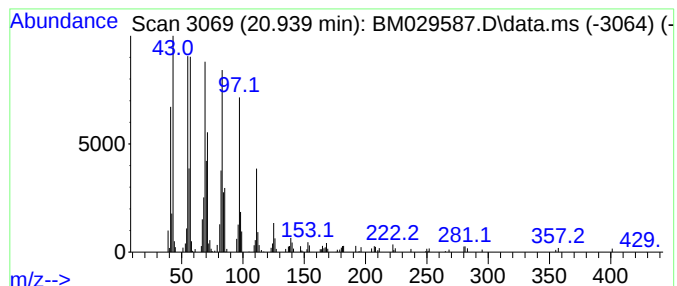

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
Data File : BM029587.D
Acq On : 22 Apr 2021 03:52
Operator : CG/JU
Sample : M2114-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
3-Eicosene, (E)-	20.939	2.7	ng	207929	5	21.209	1526900	20.0