
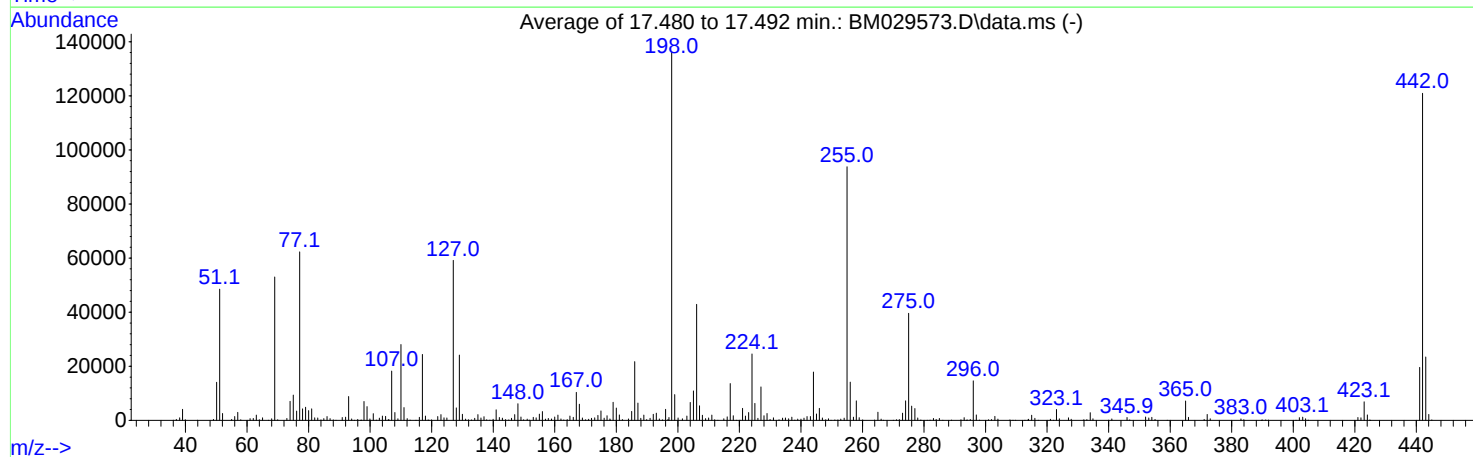


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
 Data File : BM029573.D
 Acq On : 21 Apr 2021 19:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 22 15:55:11 2021

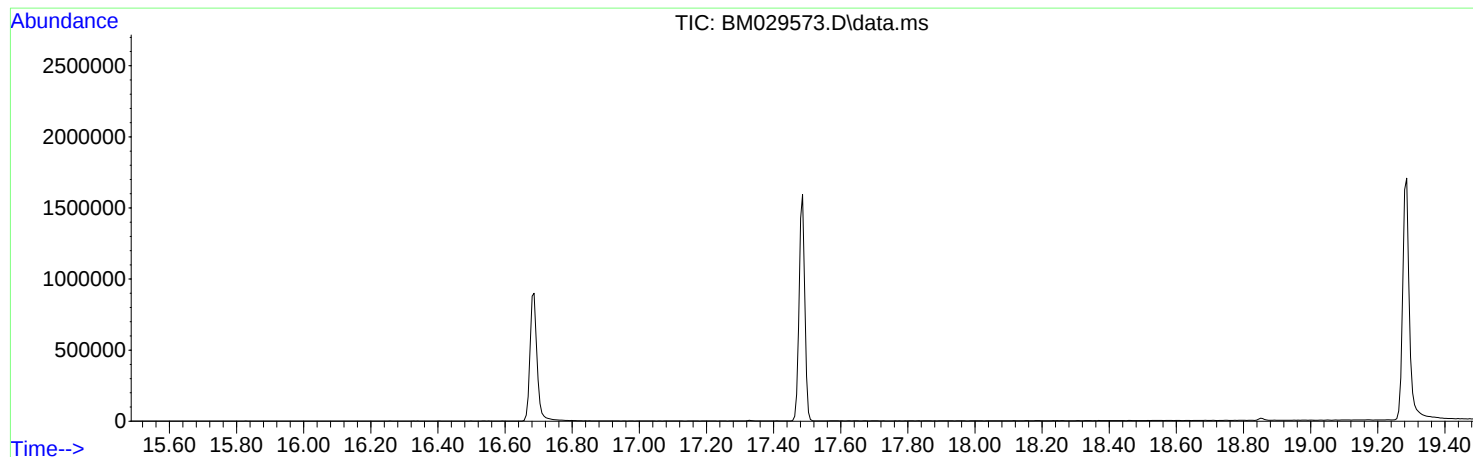




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	48531	PASS
68	69	0.00	2	1.1	601	PASS
69	198	0.00	100	39.0	52997	PASS
70	69	0.00	2	0.4	232	PASS
127	198	10	80	43.5	59147	PASS
197	198	0.00	2	0.8	1051	PASS
198	198	100	100	100.0	136021	PASS
199	198	5	9	7.0	9514	PASS
275	198	10	60	29.1	39603	PASS
365	198	1	100	5.3	7189	PASS
441	198	0.01	100	14.4	19570	PASS
442	442	50	100	100.0	120947	PASS
443	442	15	24	19.4	23427	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
Data File : BM029573.D
Acq On : 21 Apr 2021 19:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 22 05:00:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 15:14:18 2021
Response via : Initial Calibration

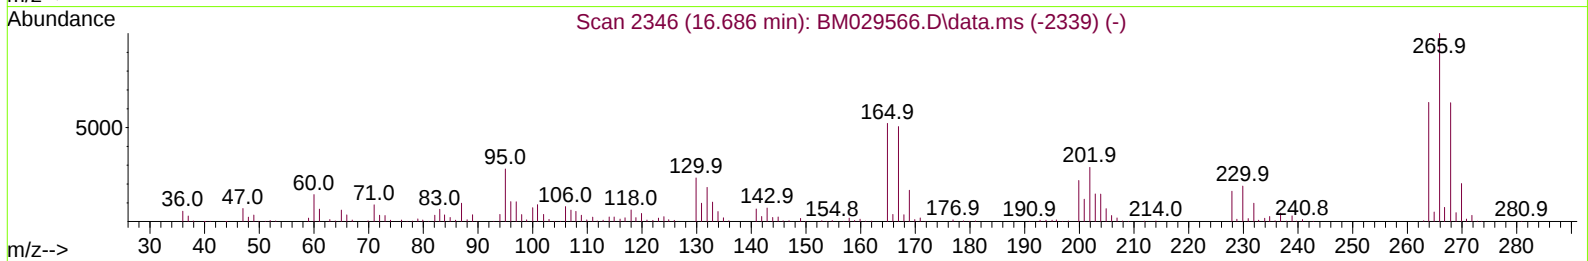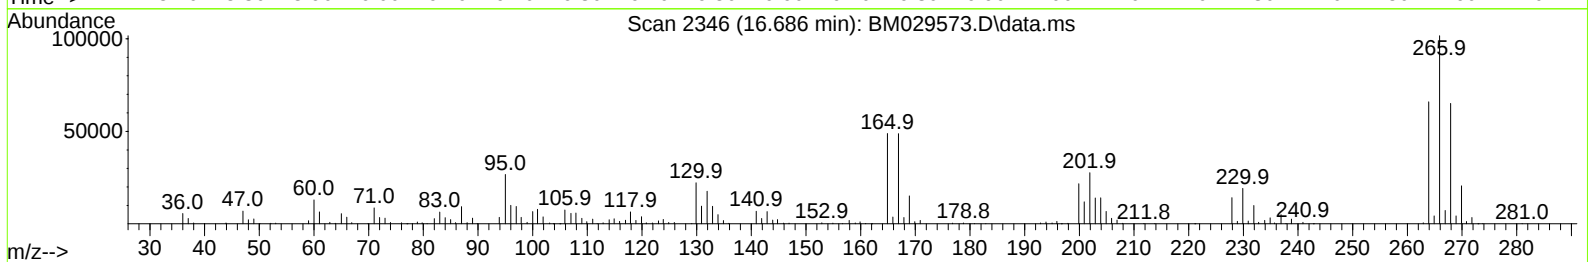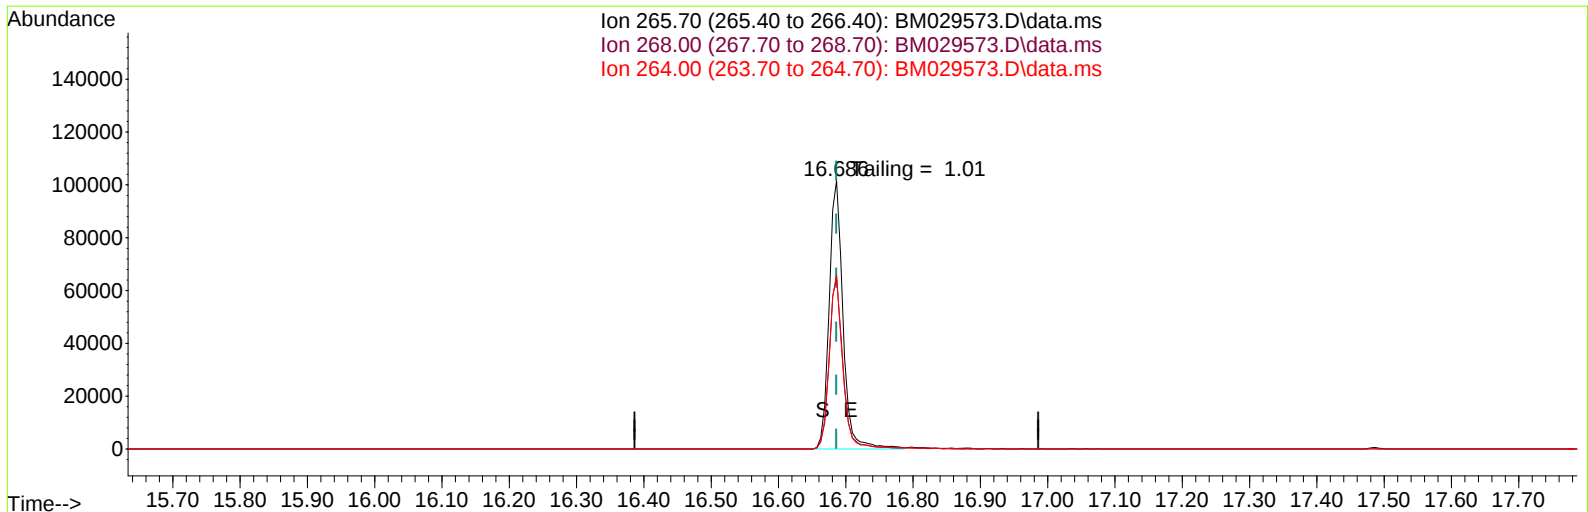

TIC: BM029573.D\data.ms

(70) Pentachlorophenol (C)

16.686min (+ 0.000) 0.00 ng




response 145959

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.03
264.00	64.90	64.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042121\
 Data File : BM029573.D
 Acq On : 21 Apr 2021 19:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 22 05:00:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 21 15:14:18 2021
 Response via : Initial Calibration

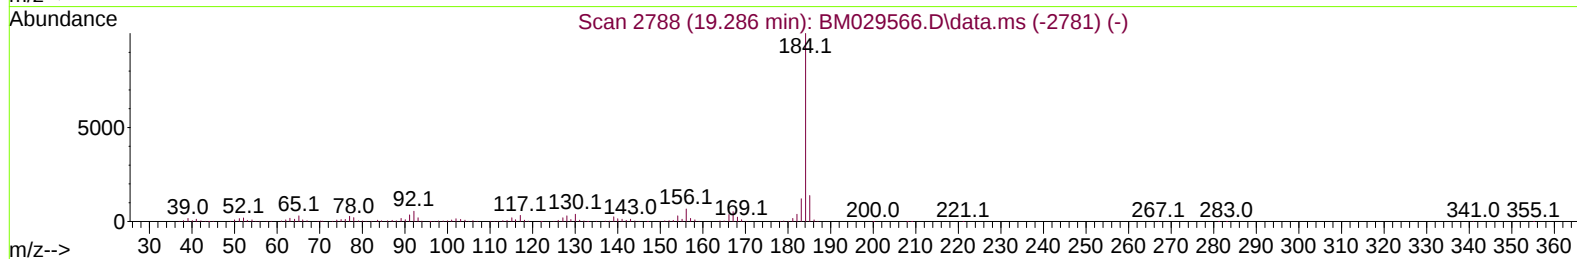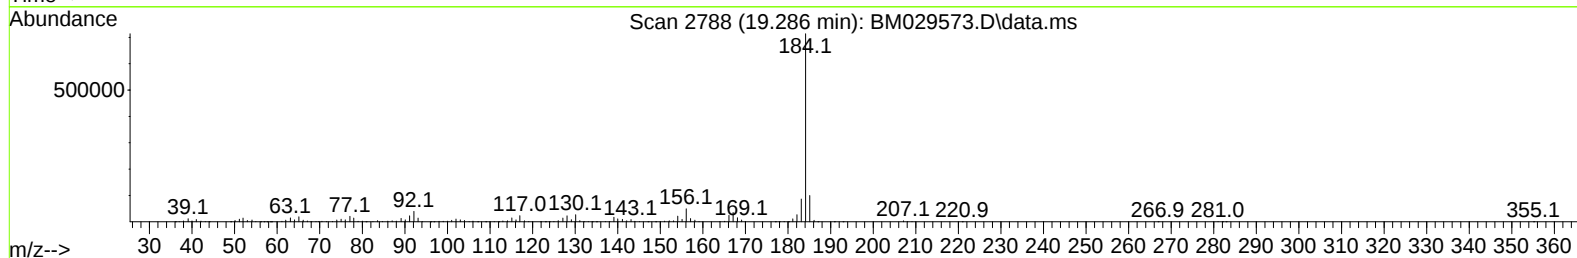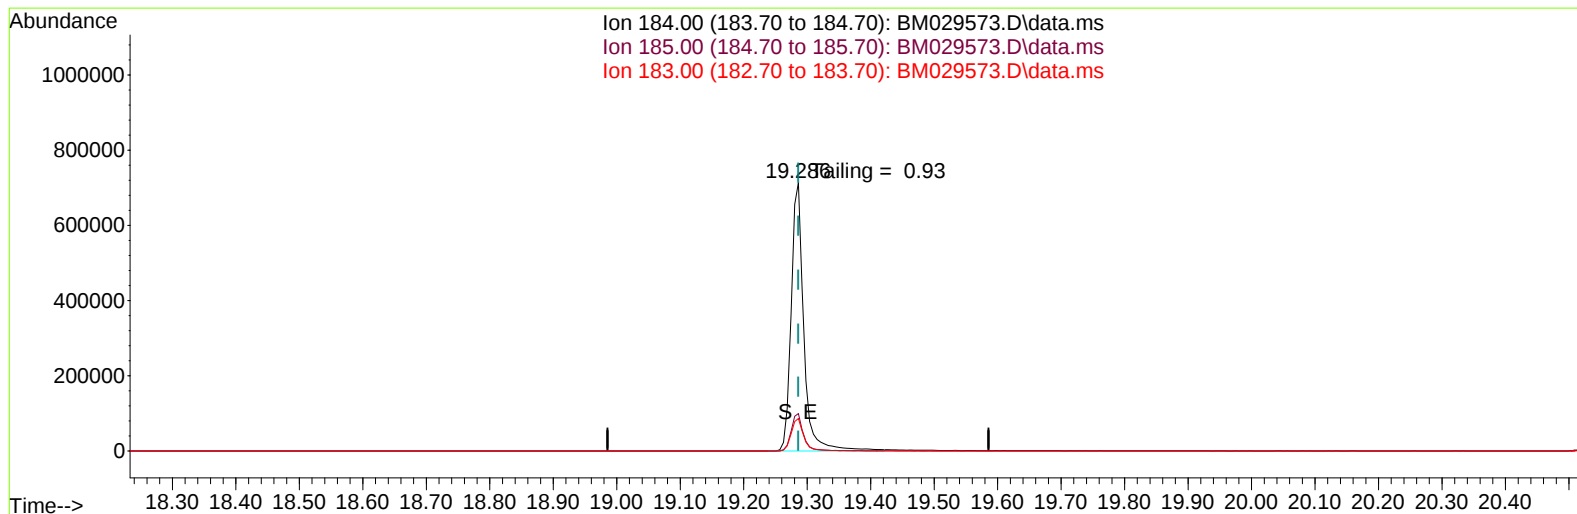

TIC: BM029573.D\data.ms

(77) Benzidine

19.286min (+ 0.000) 0.00 ng

response 1003129

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.95
183.00	12.30	12.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/21/2021	BNA_M	<u>BM029573.D</u>
Compound Name	Response	Retention Time
DDT	538601	20.515
DDD	5874	20.08
DDE	865	19.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6739	545340	1.24