
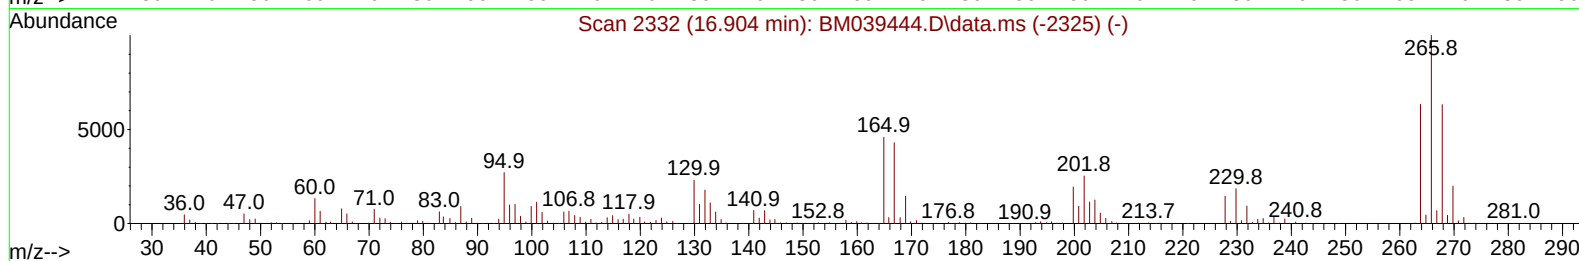
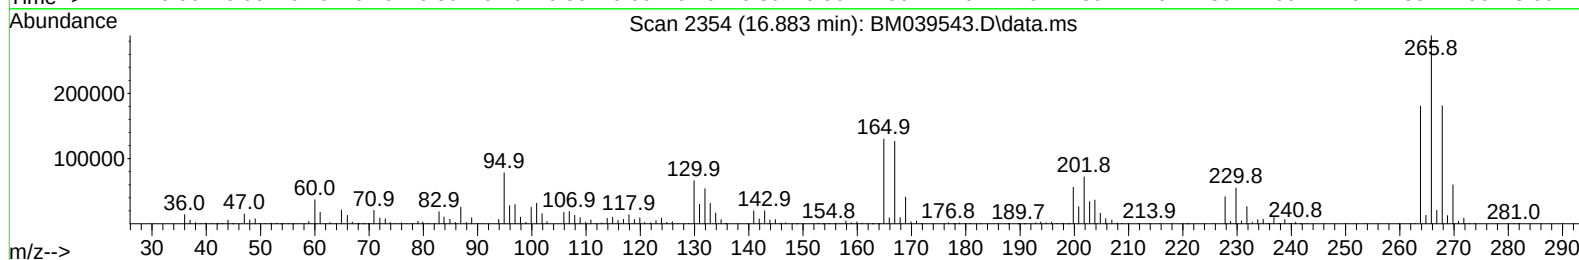


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
Data File : BM039543.D
Acq On : 21 Apr 2023 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 05:46:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 12:46:01 2023
Response via : Initial Calibration

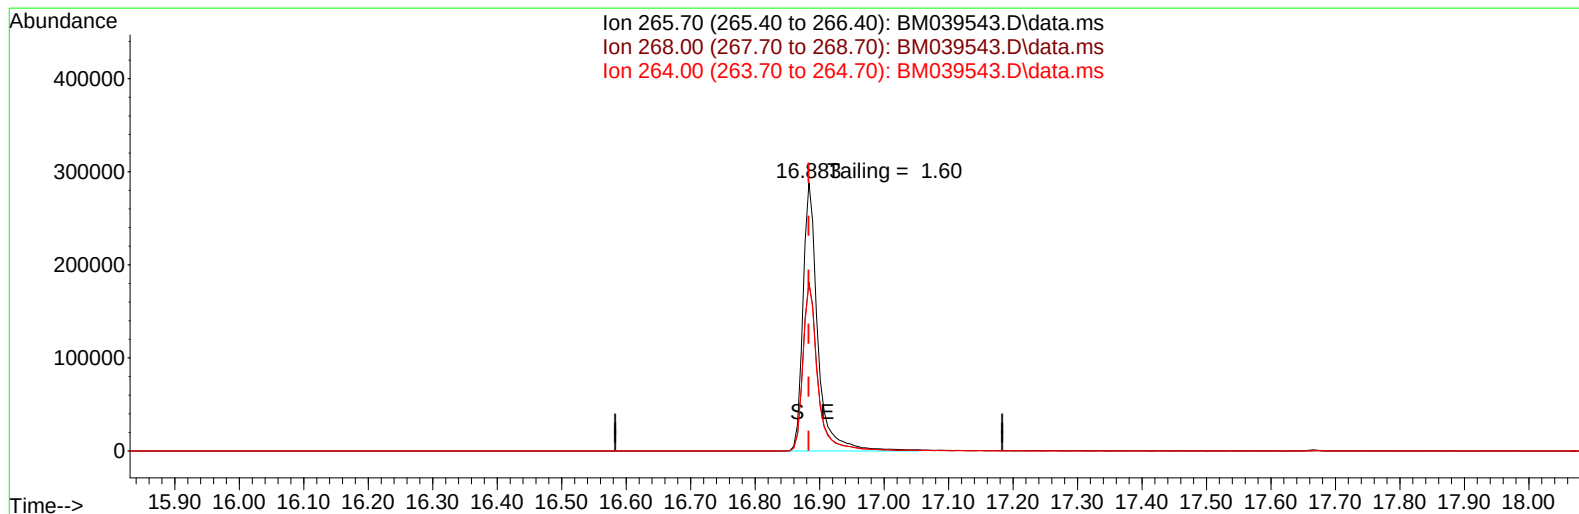

TIC: BM039543.D\data.ms

(70) Pentachlorophenol (C)




16.883min (+ 0.000) 0.00 ng

response 463563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.77
264.00	63.30	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
 Data File : BM039543.D
 Acq On : 21 Apr 2023 09:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 05:46:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 12:46:01 2023
 Response via : Initial Calibration

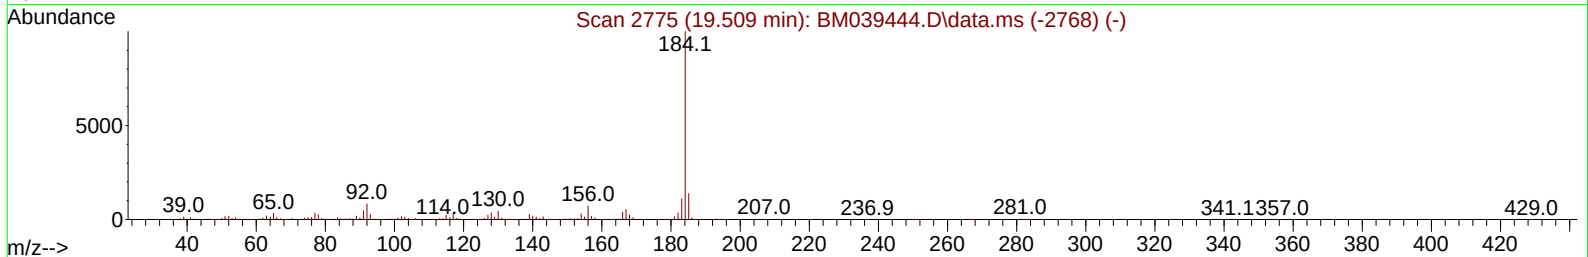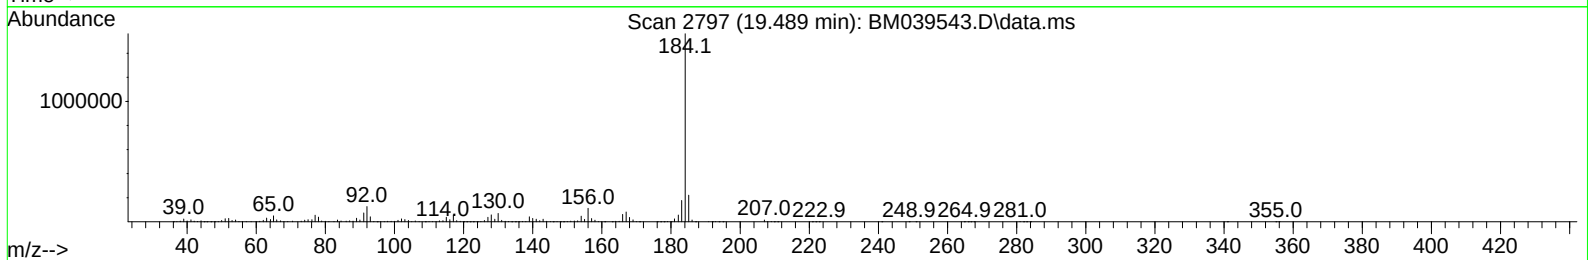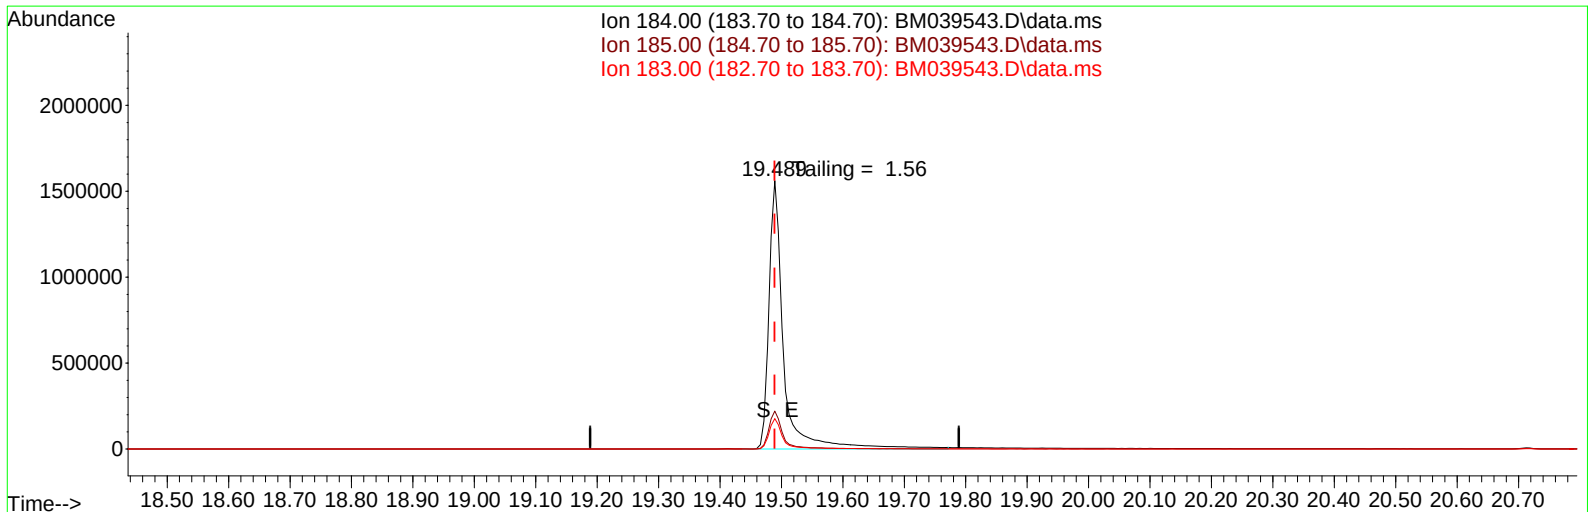

TIC: BM039543.D\data.ms

(77) Benzidine**19.489min (+ 0.000) 984077.82 ng****response 2631258**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.16
183.00	11.00	11.34
0.00	0.00	0.00