
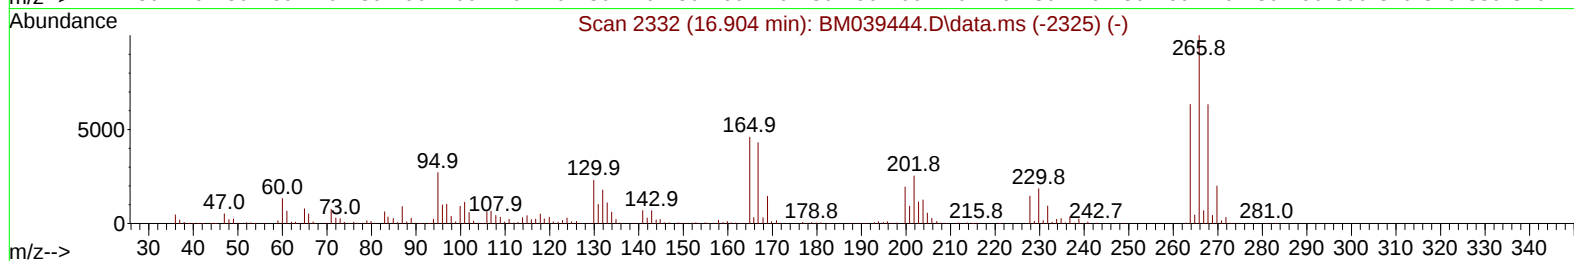
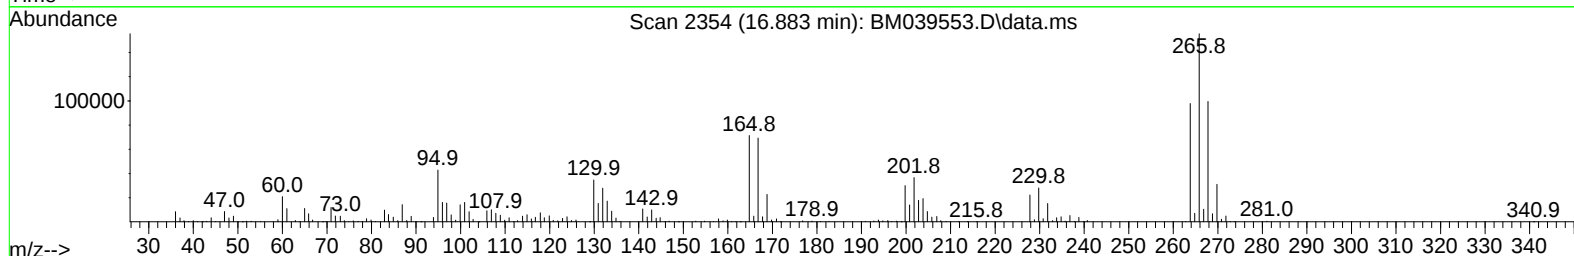


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
Data File : BM039553.D
Acq On : 21 Apr 2023 16:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 05:48:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 12:46:01 2023
Response via : Initial Calibration

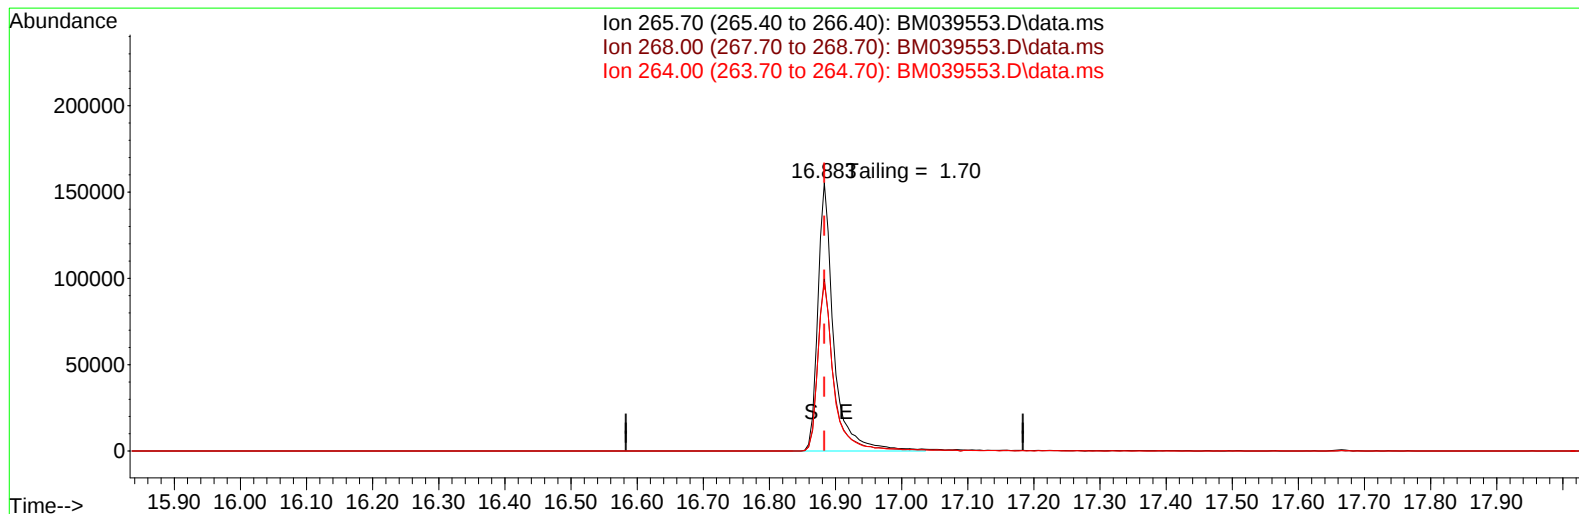

TIC: BM039553.D\data.ms

(70) Pentachlorophenol (C)




16.883min (-0.000) 0.00 ng

response 260034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.03
264.00	63.30	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
Data File : BM039553.D
Acq On : 21 Apr 2023 16:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 05:48:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 12:46:01 2023
Response via : Initial Calibration

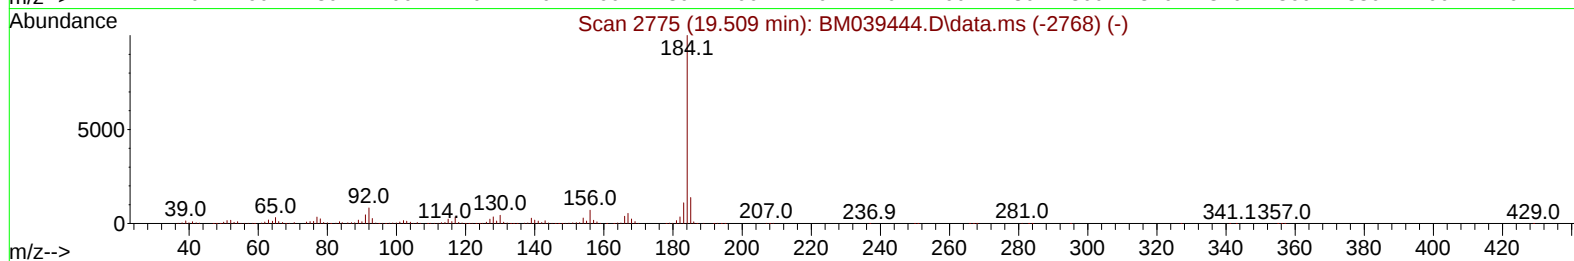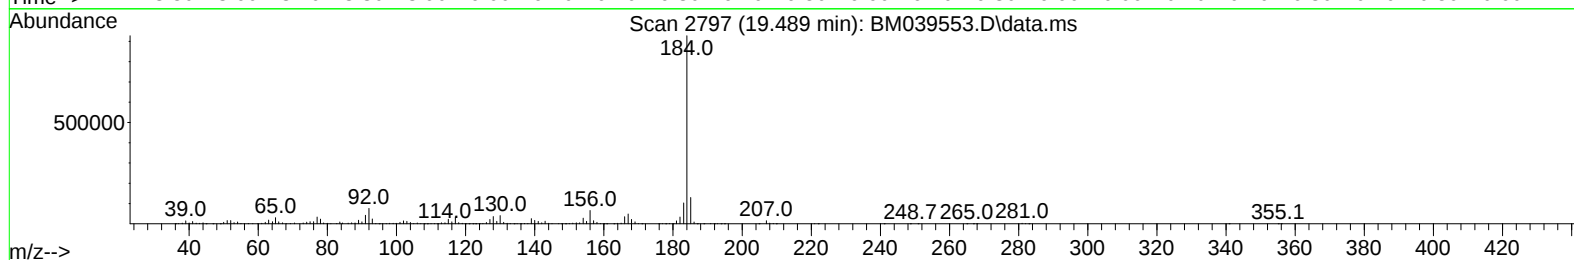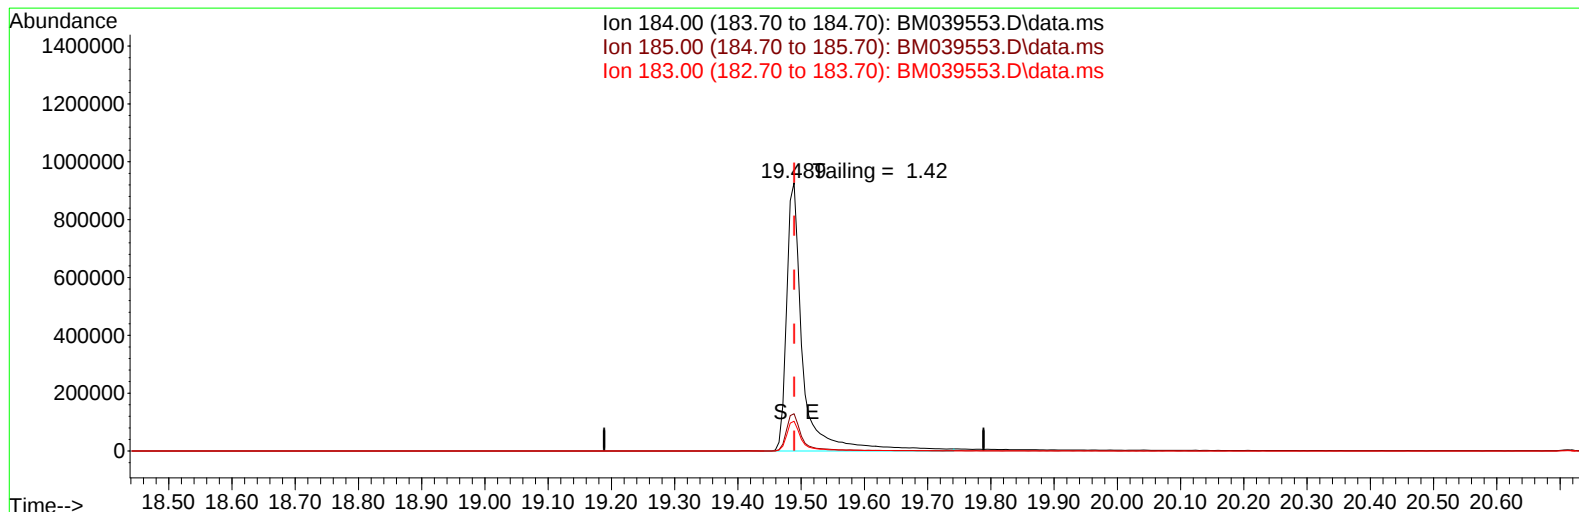

TIC: BM039553.D\data.ms

(77) Benzidine**19.489min (-0.000) 161614.38 ng****response 1655276**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.94
183.00	11.00	11.11
0.00	0.00	0.00