
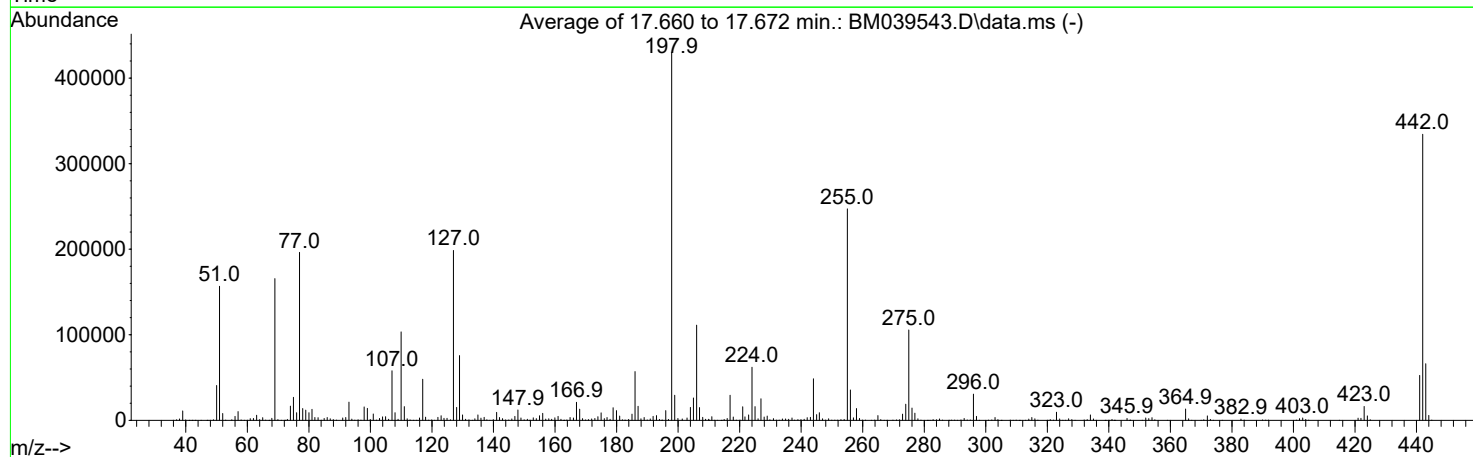


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
 Data File : BM039543.D
 Acq On : 21 Apr 2023 09:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 21 12:46:01 2023

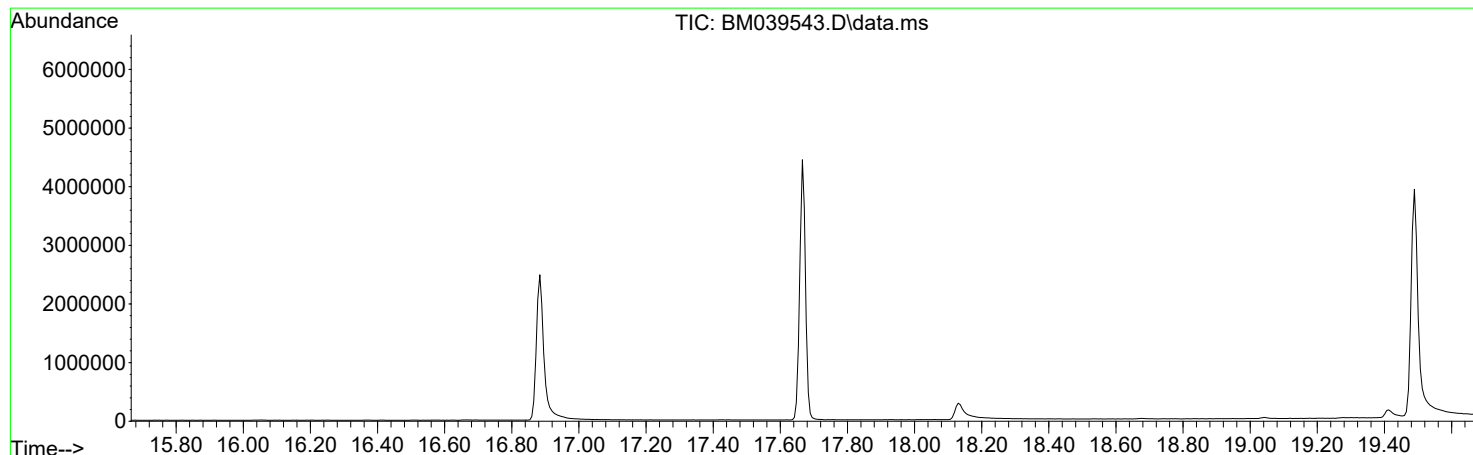

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	156631	PASS
68	69	0.00	2	1.5	2528	PASS
69	198	0.00	100	38.5	165605	PASS
70	69	0.00	2	0.5	906	PASS
127	198	10	80	46.2	198635	PASS
197	198	0.00	2	0.3	1220	PASS
198	198	100	100	100.0	429909	PASS
199	198	5	9	6.8	29376	PASS
275	198	10	60	24.6	105739	PASS
365	198	1	100	3.1	13326	PASS
441	198	0.01	100	12.2	52619	PASS
442	442	50	100	100.0	334336	PASS
443	442	15	24	19.8	66128	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/21/2023	BNA_M	<u>BM039543.D</u>
Compound Name	Response	Retention Time
DDT	1446536	20.712
DDD	14814	20.324
DDE	762	19.771
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15576	1462112	1.07

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
Data File : BM039543.D
Acq On : 21 Apr 2023 09:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 22 05:46:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 12:46:01 2023
Response via : Initial Calibration

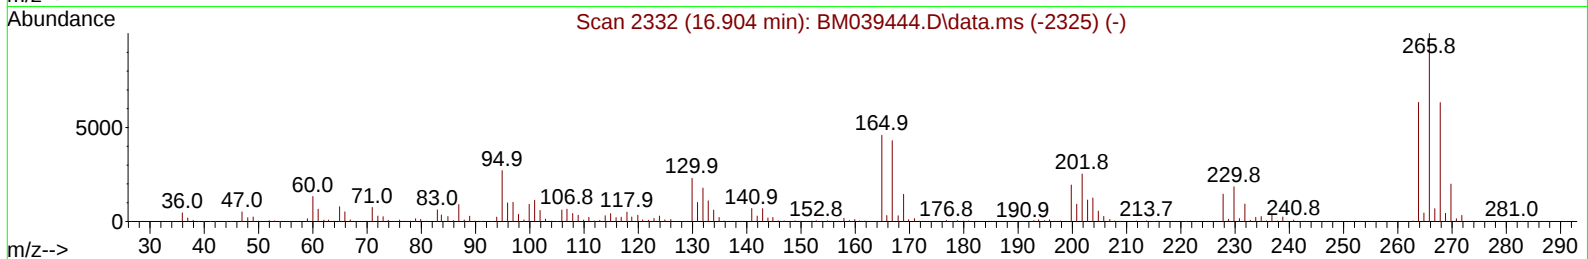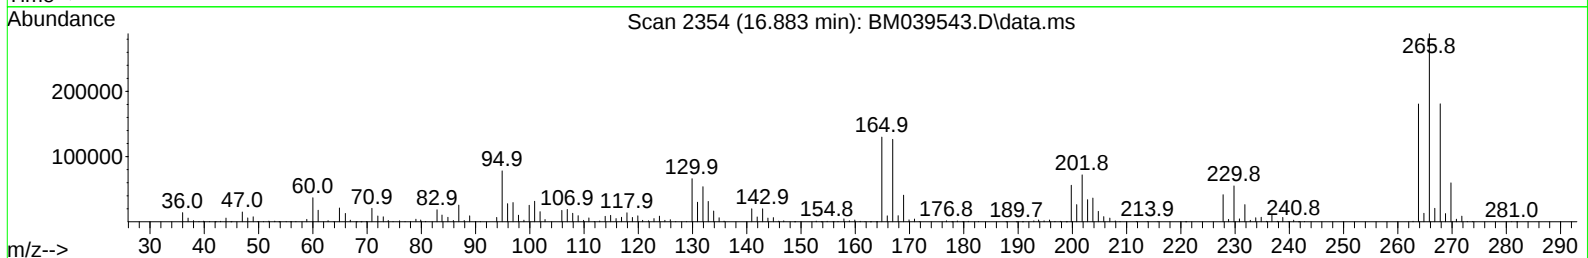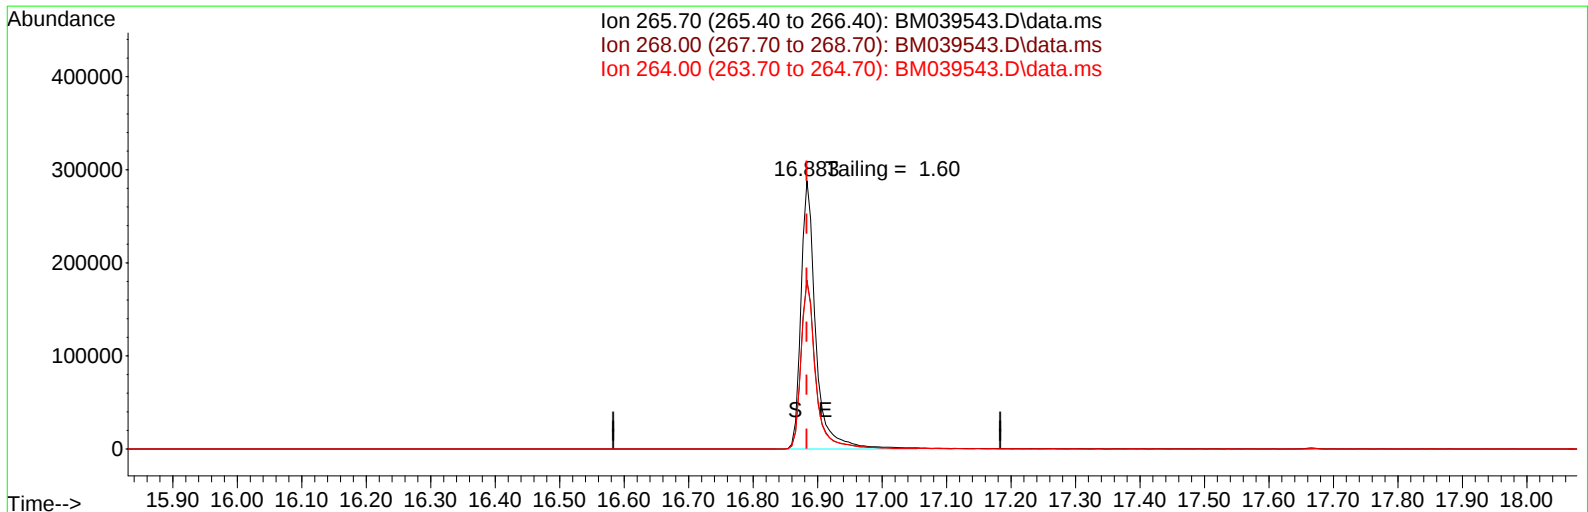

TIC: BM039543.D\data.ms

(70) Pentachlorophenol (C)

16.883min (+ 0.000) 0.00 ng




response 463563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	62.77
264.00	63.30	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
 Data File : BM039543.D
 Acq On : 21 Apr 2023 09:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 22 05:46:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 12:46:01 2023
 Response via : Initial Calibration

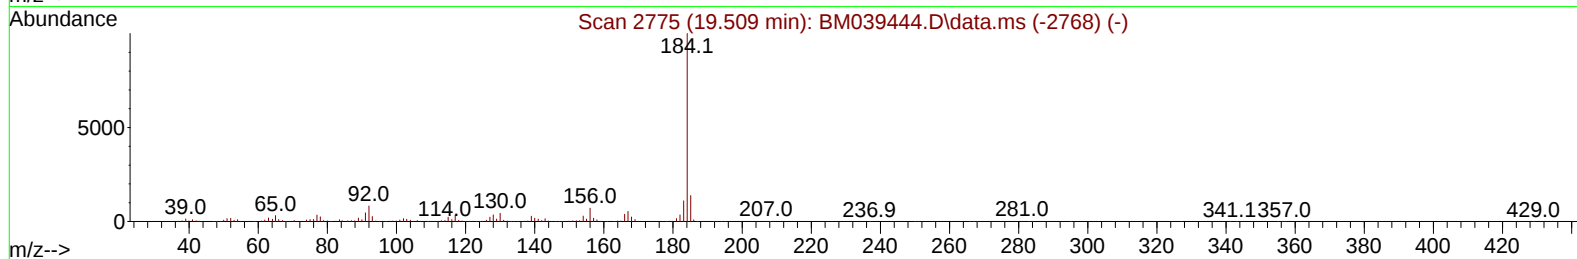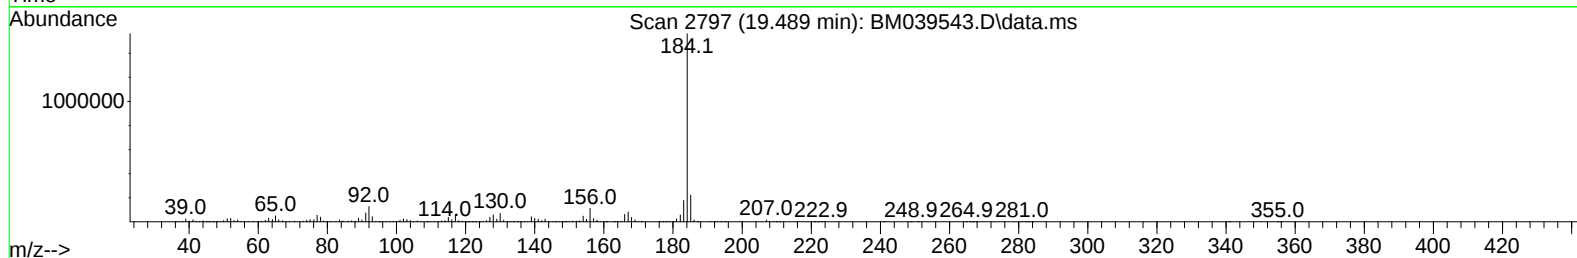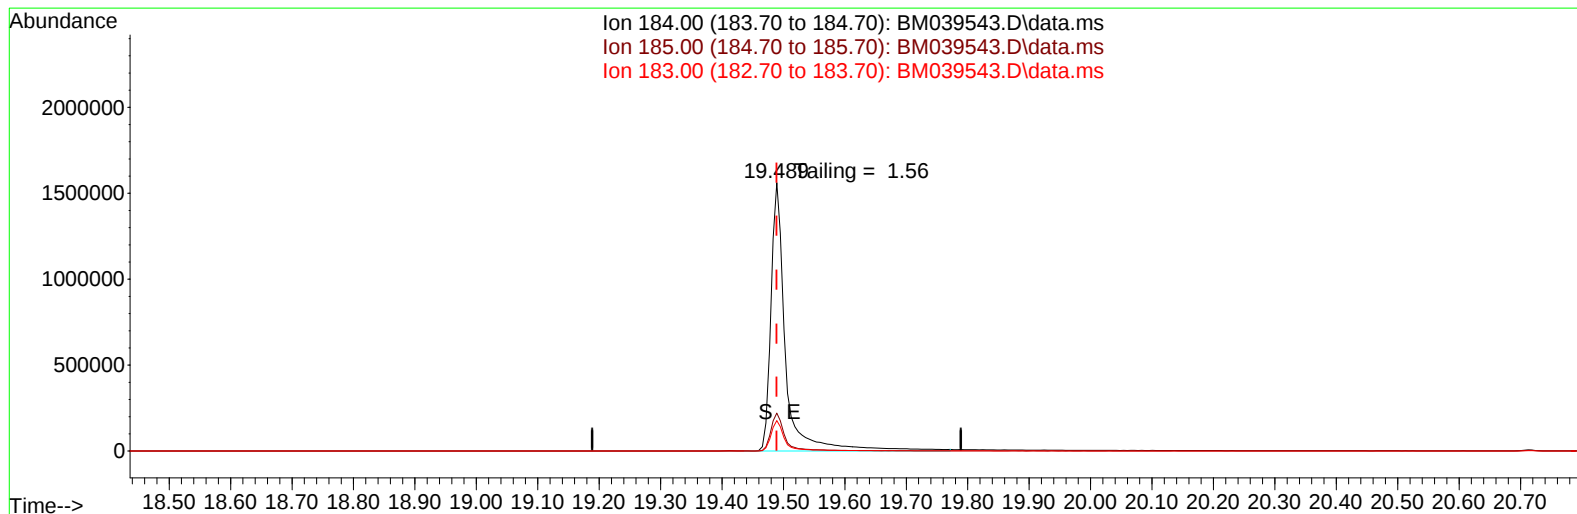

TIC: BM039543.D\data.ms

(77) Benzidine**19.489min (+ 0.000) 984077.82 ng****response 2631258**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.16
183.00	11.00	11.34
0.00	0.00	0.00