
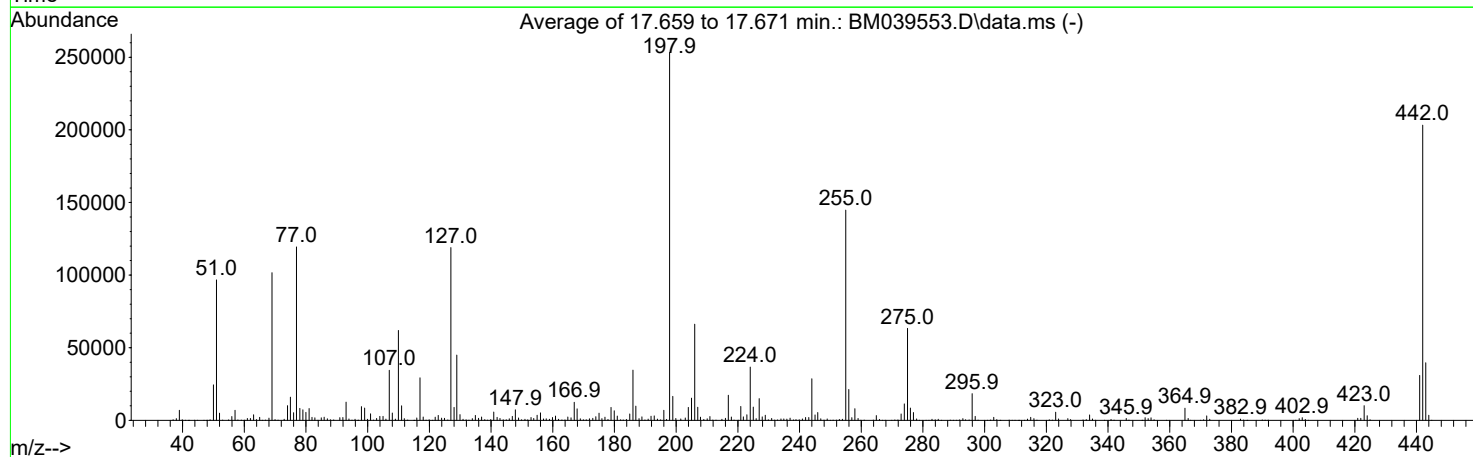


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
 Data File : BM039553.D
 Acq On : 21 Apr 2023 16:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 21 12:46:01 2023

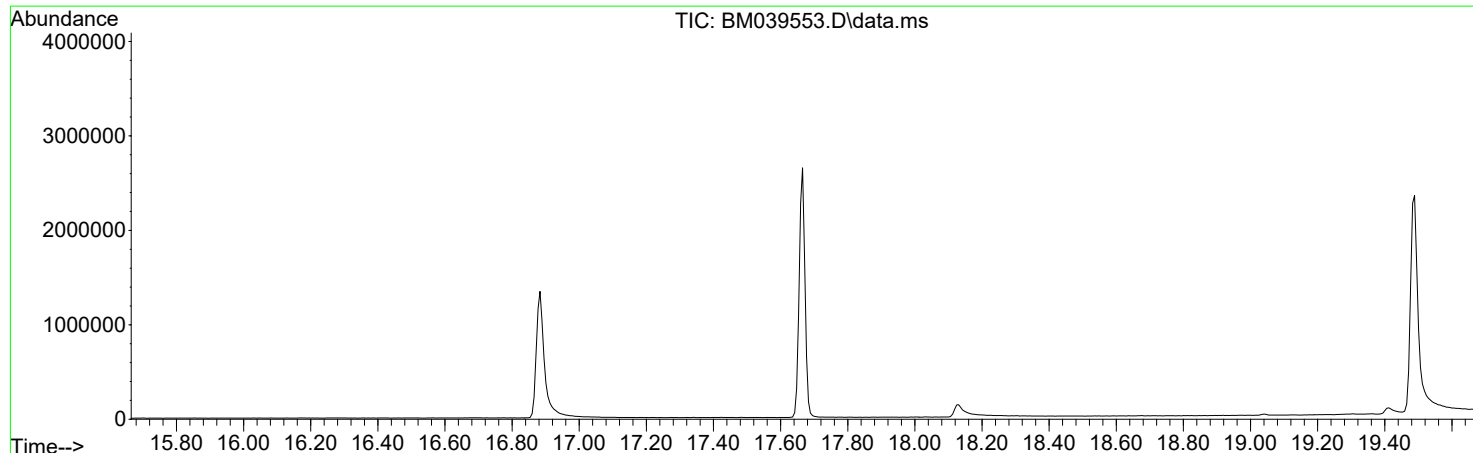

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	96742	PASS
68	69	0.00	2	1.6	1589	PASS
69	198	0.00	100	40.2	101696	PASS
70	69	0.00	2	0.6	589	PASS
127	198	10	80	47.0	118933	PASS
197	198	0.00	2	0.3	668	PASS
198	198	100	100	100.0	253269	PASS
199	198	5	9	6.5	16482	PASS
275	198	10	60	25.0	63317	PASS
365	198	1	100	3.3	8401	PASS
441	198	0.01	100	12.2	30976	PASS
442	442	50	100	100.0	203285	PASS
443	442	15	24	19.5	39691	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/21/2023	BNA_M	<u>BM039553.D</u>
Compound Name	Response	Retention Time
DDT	841601	20.712
DDD	14930	20.277
DDE	382	19.771
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15312	856913	1.79

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
 Data File : BM039553.D
 Acq On : 21 Apr 2023 16:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 22 05:48:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 21 12:46:01 2023
 Response via : Initial Calibration

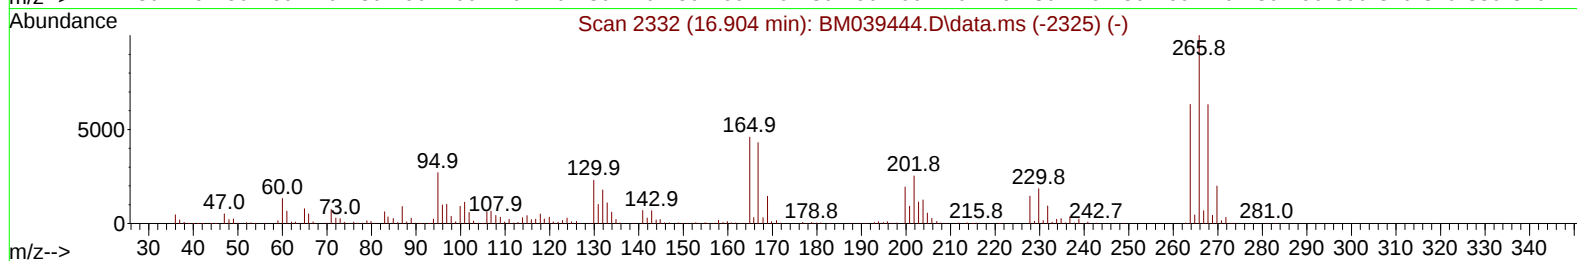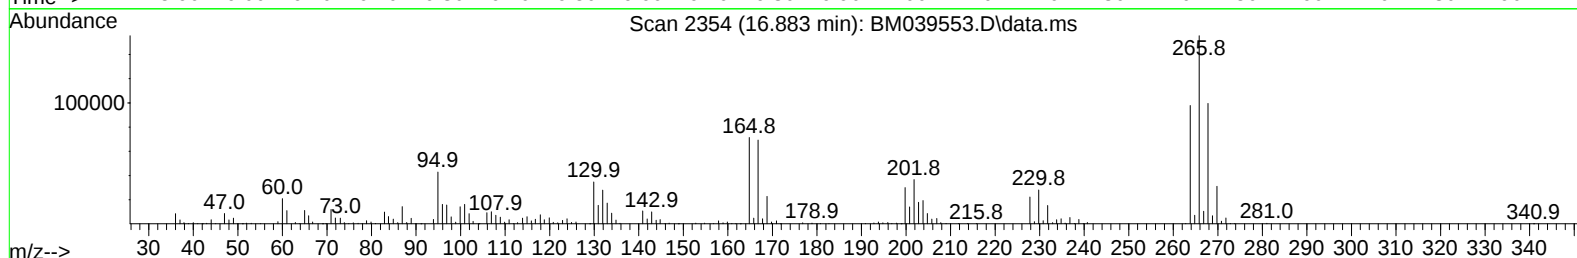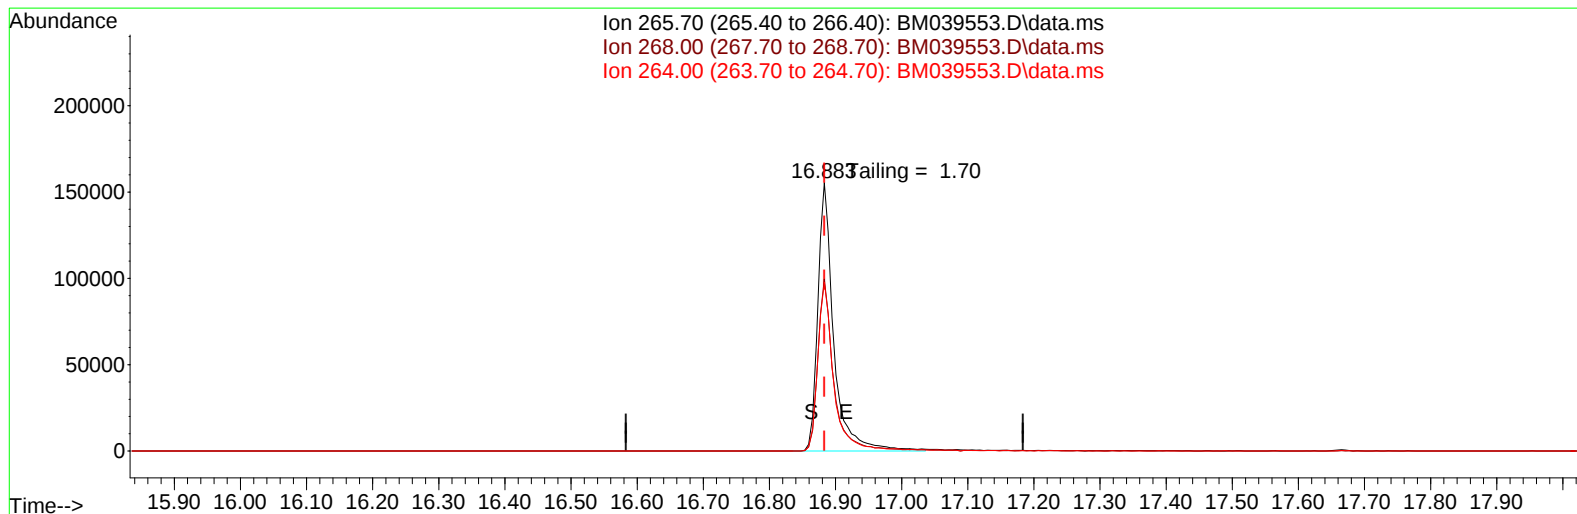

TIC: BM039553.D\data.ms

(70) Pentachlorophenol (C)

16.883min (-0.000) 0.00 ng




response 260034

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.03
264.00	63.30	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042123\
Data File : BM039553.D
Acq On : 21 Apr 2023 16:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 22 05:48:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM041723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 21 12:46:01 2023
Response via : Initial Calibration

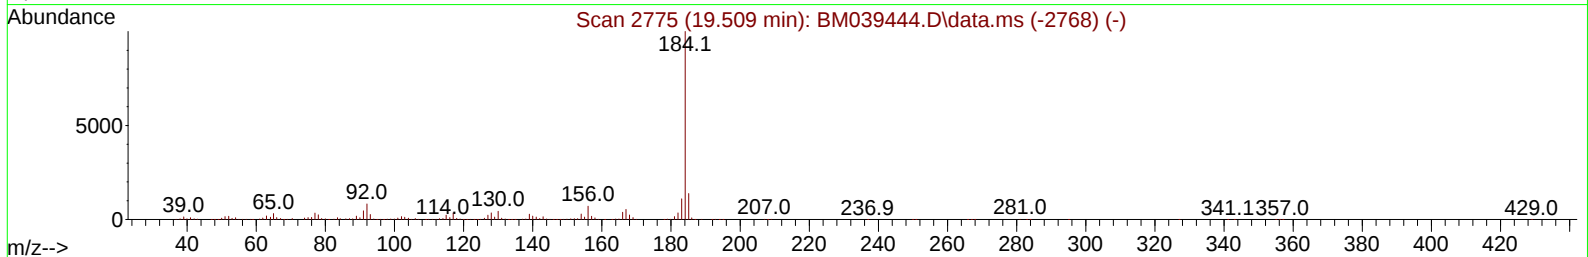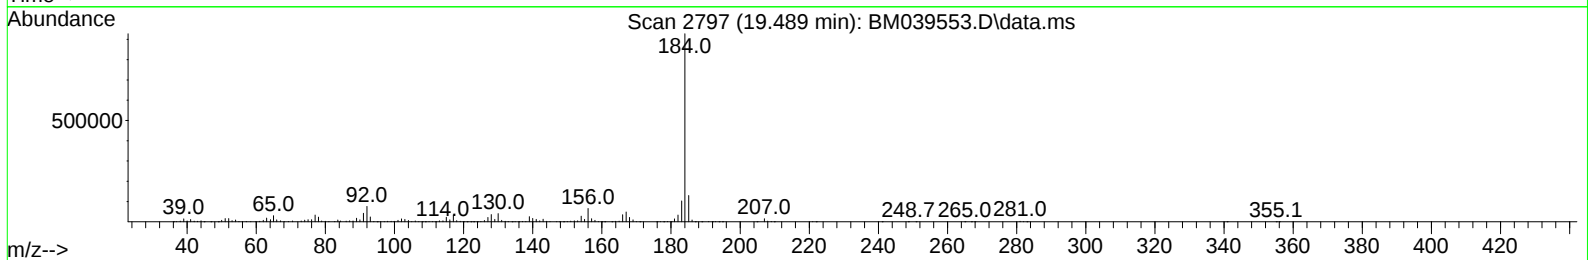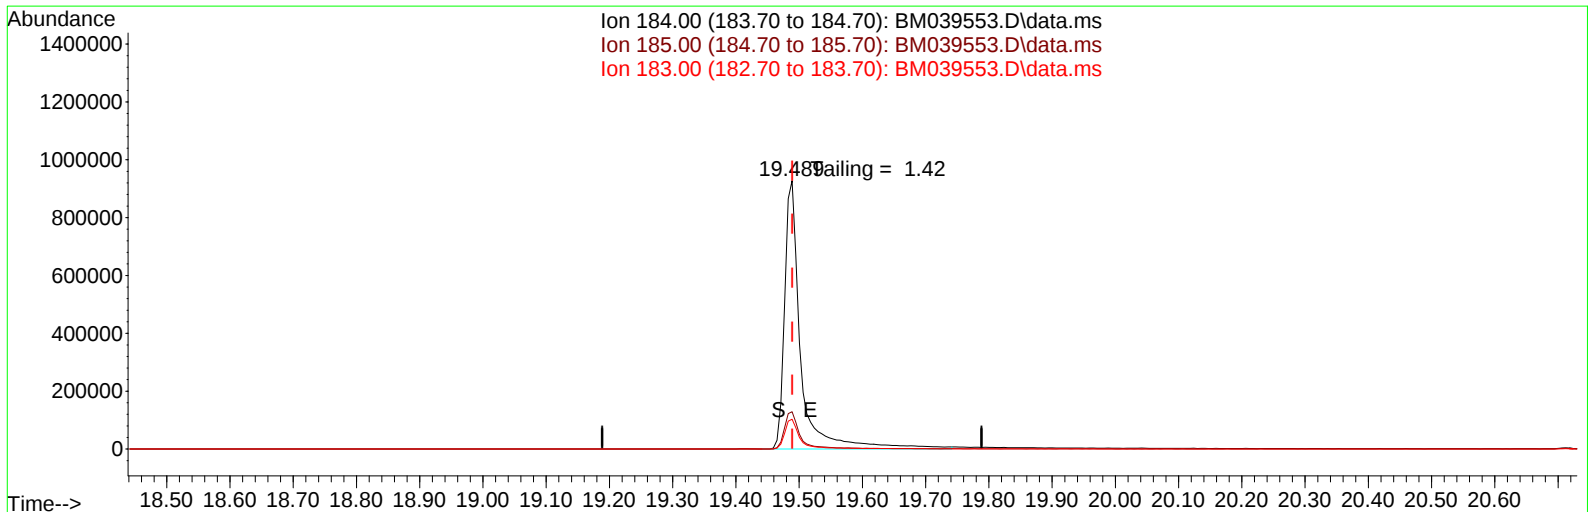

TIC: BM039553.D\data.ms

(77) Benzidine

19.489min (-0.000) 161614.38 ng

response 1655276

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.94
183.00	11.00	11.11
0.00	0.00	0.00